

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031116\
 Data File : BF085418.D
 Acq On : 12 Mar 2016 14:04
 Operator : UM/SJ
 Sample : H1731-26
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-30-COMP

Quant Time: Mar 14 01:43:31 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 04 00:54:58 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	151872	20.00	ng	-0.05
21) Naphthalene-d8	8.22	136	574013	20.00	ng	-0.05
38) Acenaphthene-d10	9.98	164	168207	20.00	ng	-0.05
63) Phenanthrene-d10	11.46	188	261331	20.00	ng	-0.05
75) Chrysene-d12	14.11	240	213356	20.00	ng	-0.05
86) Perylene-d12	15.57	264	171379	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.54	112	1155316	127.60	ng	-0.03
7) Phenol-d6	6.57	99	1688612	142.35	ng	-0.03
23) Nitrobenzene-d5	7.50	82	888892	82.87	ng	-0.05
41) 2,4,6-Tribromophenol	10.77	330	180308	125.28	ng	-0.05
44) 2-Fluorobiphenyl	9.30	172	1047343	94.69	ng	-0.05
78) Terphenyl-d14	13.05	244	713950	77.68	ng	-0.03
Target Compounds						Qvalue
49) Dimethylphthalate	9.69	163	211577	16.39	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031116\
Data File : BF085418.D
Acq On : 12 Mar 2016 14:04
Operator : UM/SJ
Sample : H1731-26
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-30-COMP

Quant Time: Mar 14 01:43:31 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

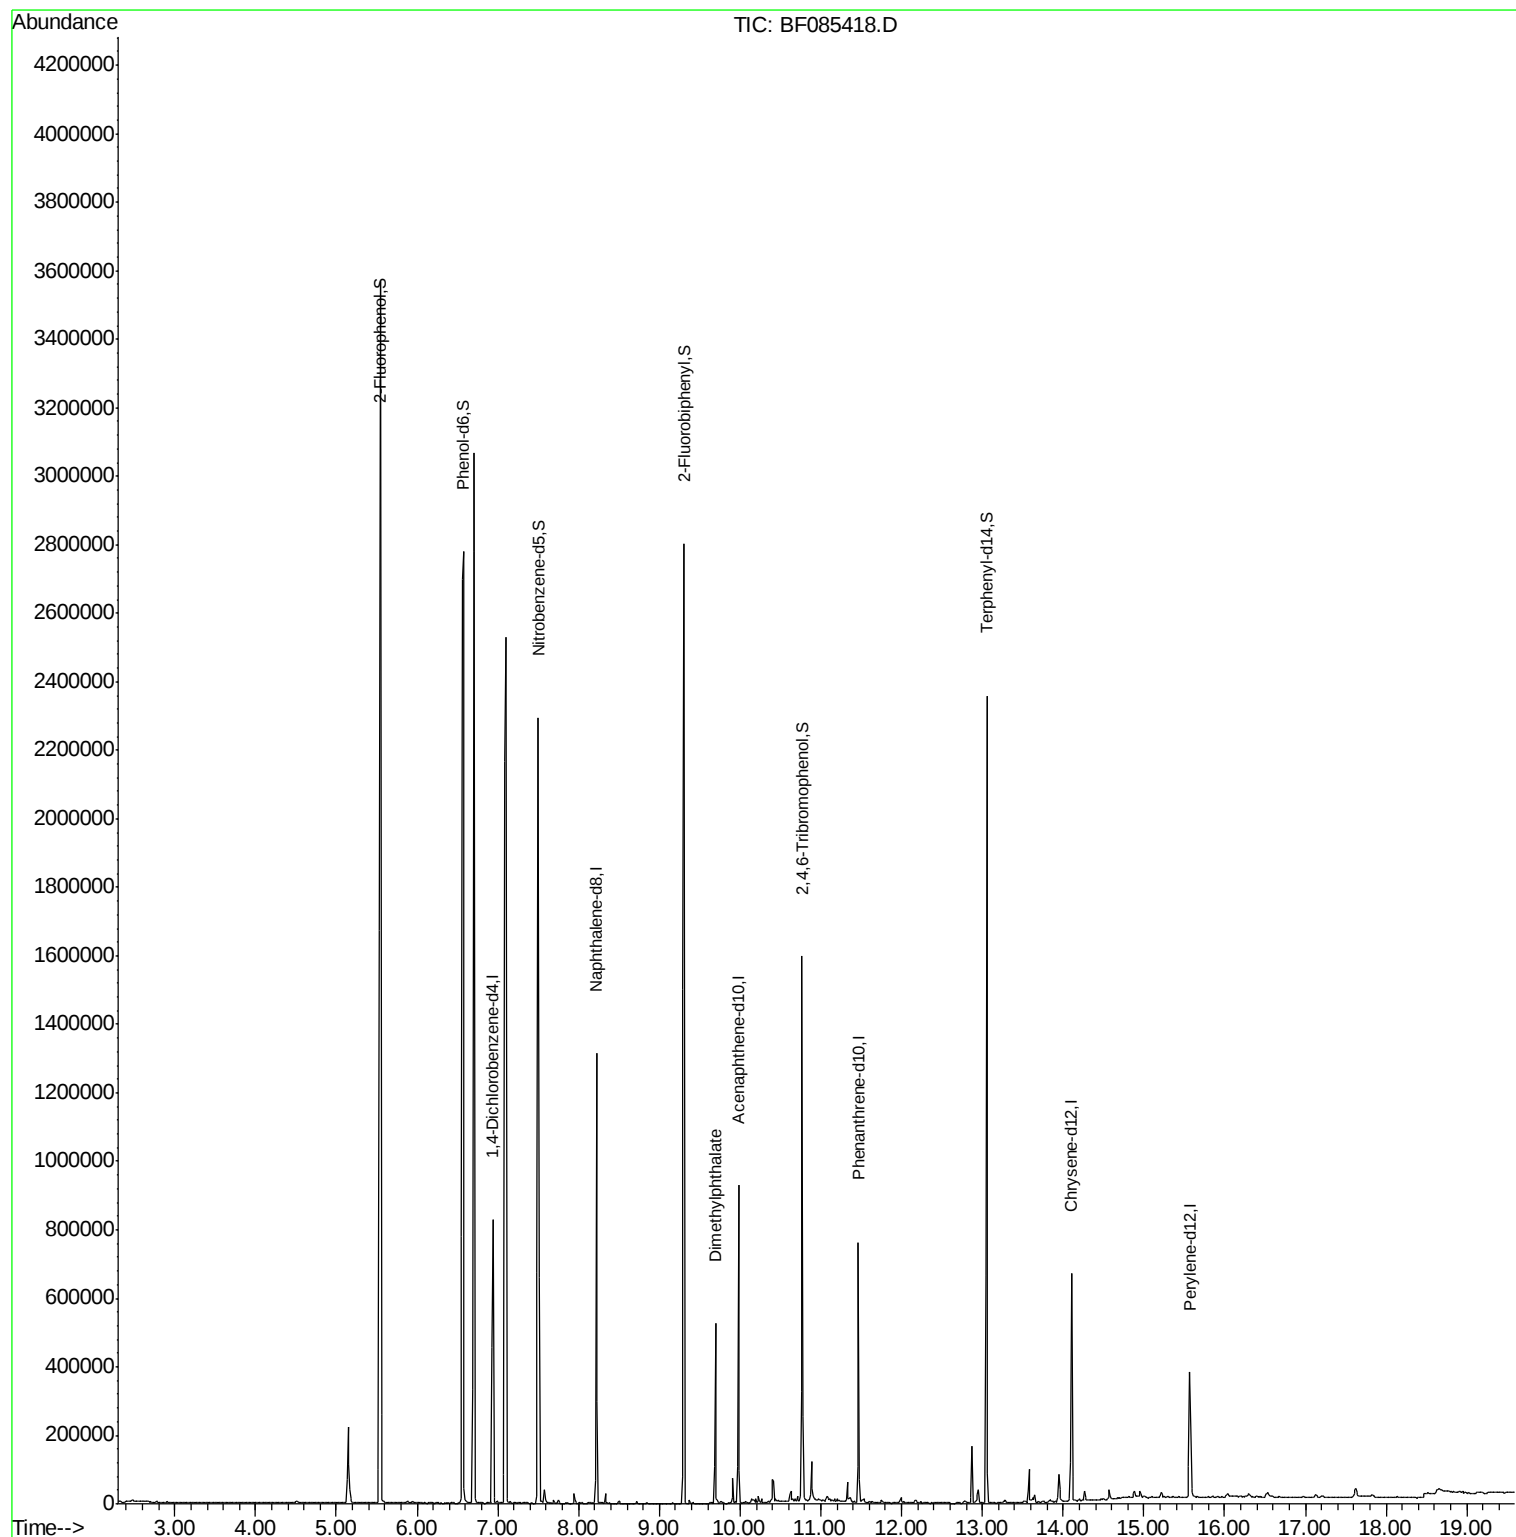


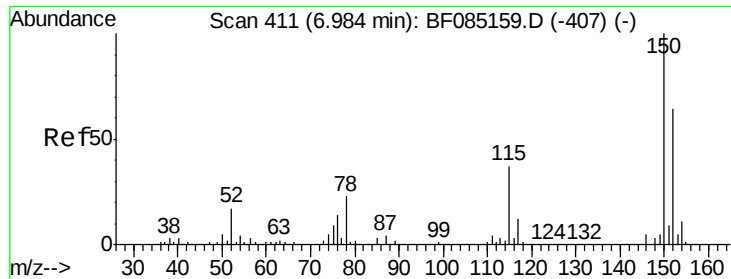




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.94 min Scan# 407
 Delta R.T. -0.05 min
 Lab File: BF085418.D
 Acq: 12 Mar 2016 14:04

Instrument :
 BNA_F
 ClientSampleId :
 SB-30-COMP

Tgt Ion:152 Resp: 151872
 Ion Ratio Lower Upper
 152 100
 150 151.2 124.6 186.8
 115 54.9 46.6 70.0

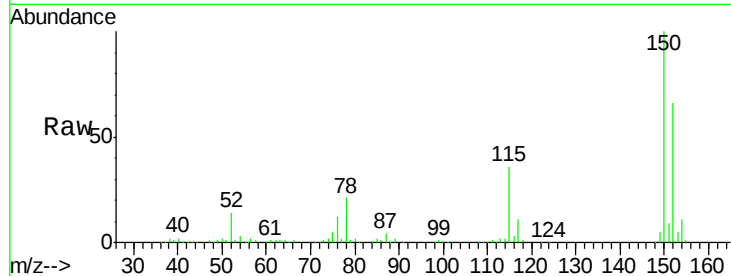


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

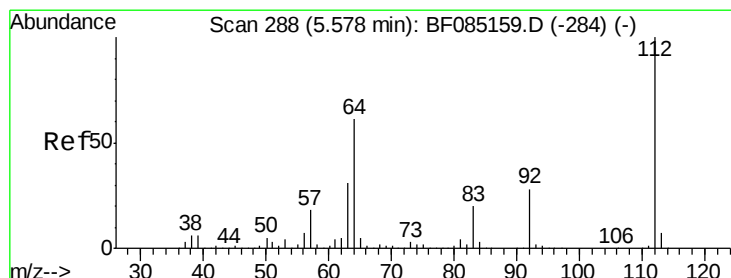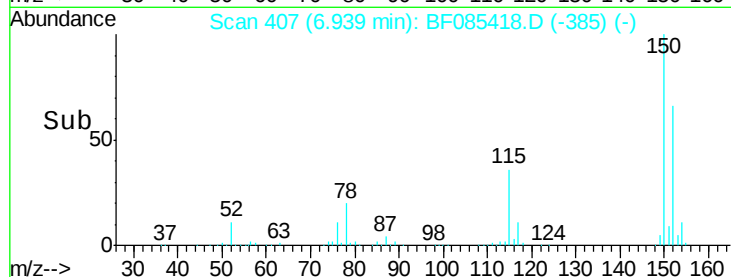
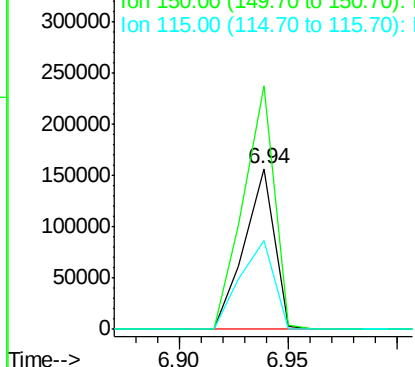



#5
 2-Fluorophenol
 Concen: 127.60 ng
 RT: 5.54 min Scan# 285
 Delta R.T. -0.03 min
 Lab File: BF085418.D
 Acq: 12 Mar 2016 14:04

Tgt Ion:112 Resp: 1155316
 Ion Ratio Lower Upper
 112 100
 64 56.2 49.0 73.4
 63 28.4 24.8 37.2

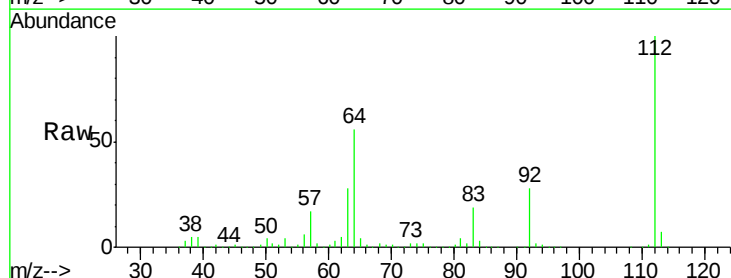

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

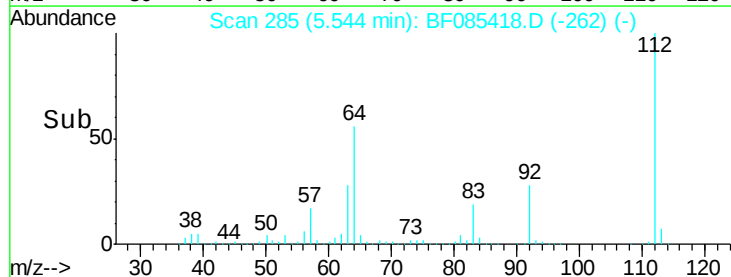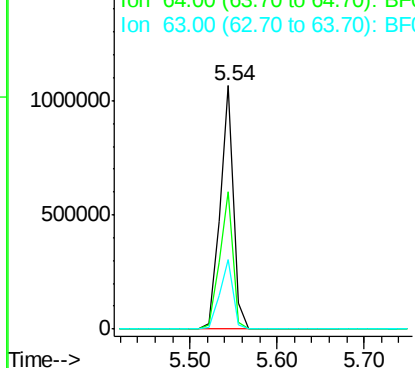

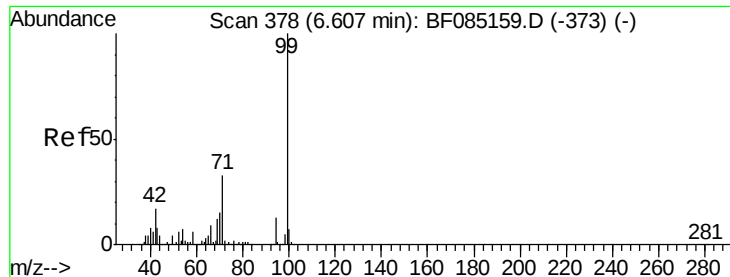

#7

Phenol-d6

Concen: 142.35 ng

RT: 6.57 min Scan# 375

Delta R.T. -0.03 min

Lab File: BF085418.D

Acq: 12 Mar 2016 14:04

Instrument :

BNA_F

ClientSampleId :

SB-30-COMP


Tgt Ion: 99 Resp: 1688612

Ion Ratio Lower Upper

99 100

42 11.9 13.6 20.4#




71 28.7 26.7 40.1

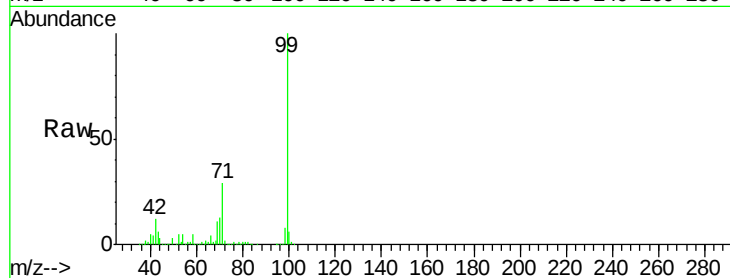

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

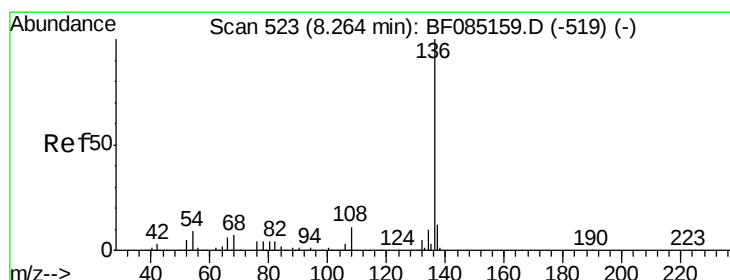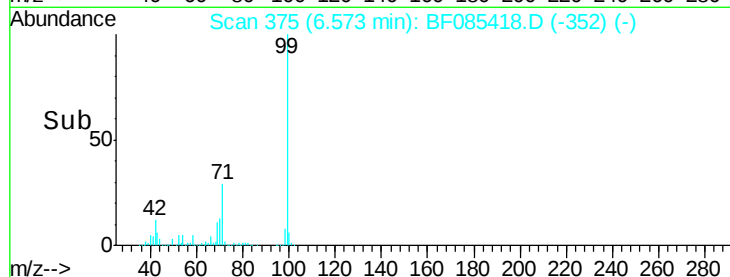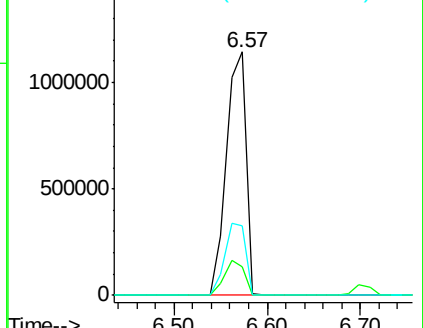

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.22 min Scan# 519

Delta R.T. -0.05 min

Lab File: BF085418.D

Acq: 12 Mar 2016 14:04

Tgt Ion: 136 Resp: 574013


Ion Ratio Lower Upper

136 100

137 11.3 9.3 13.9

54 8.3 7.4 11.2

68 6.9 6.0 9.0


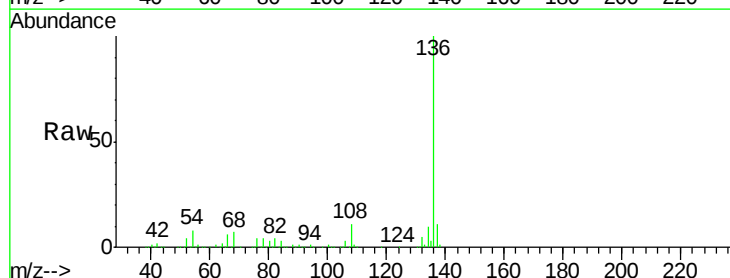



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

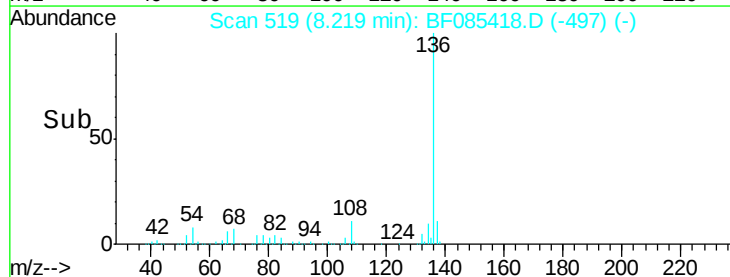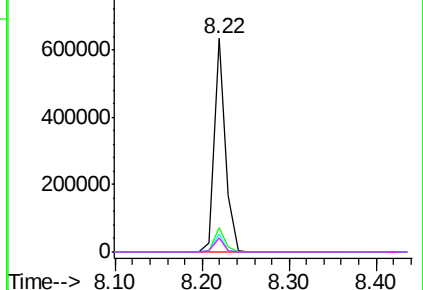


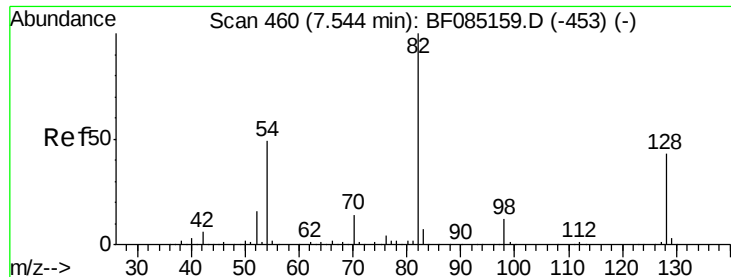




#23
 Nitrobenzene-d5
 Concen: 82.87 ng
 RT: 7.50 min Scan# 456
 Delta R.T. -0.05 min
 Lab File: BF085418.D
 Acq: 12 Mar 2016 14:04

Instrument :
 BNA_F
 ClientSampleId :
 SB-30-COMP

Tgt Ion: 82 Resp: 888892
 Ion Ratio Lower Upper
 82 100
 128 44.1 34.5 51.7
 54 46.7 39.3 58.9

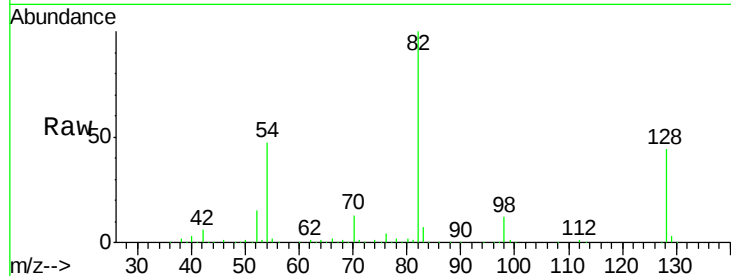


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

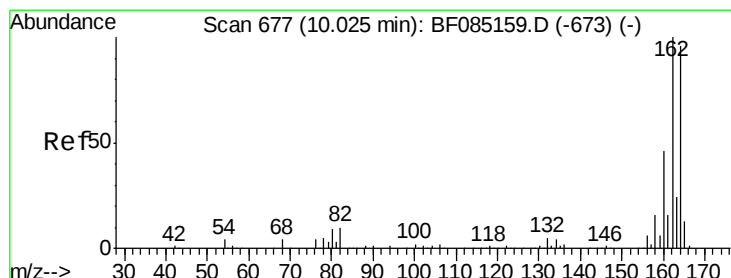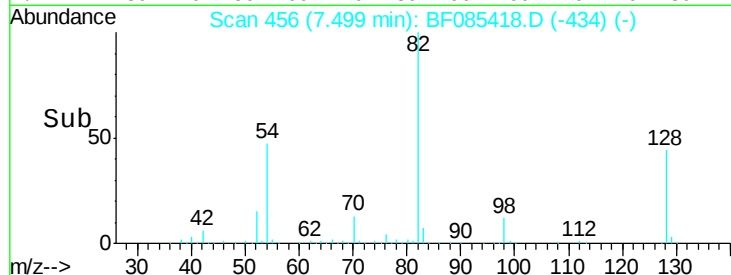
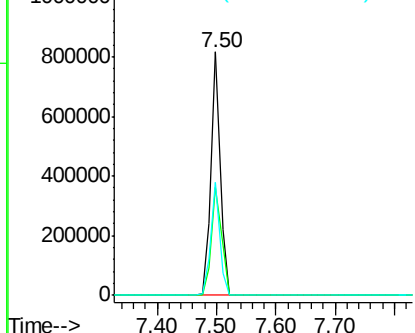



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.98 min Scan# 673
 Delta R.T. -0.05 min
 Lab File: BF085418.D
 Acq: 12 Mar 2016 14:04

Tgt Ion: 164 Resp: 168207
 Ion Ratio Lower Upper
 164 100
 162 105.0 83.3 124.9
 160 45.8 37.9 56.9

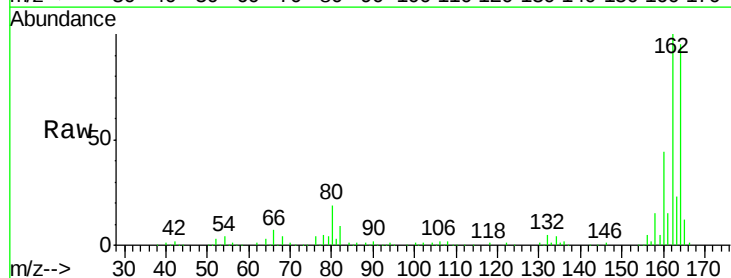

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

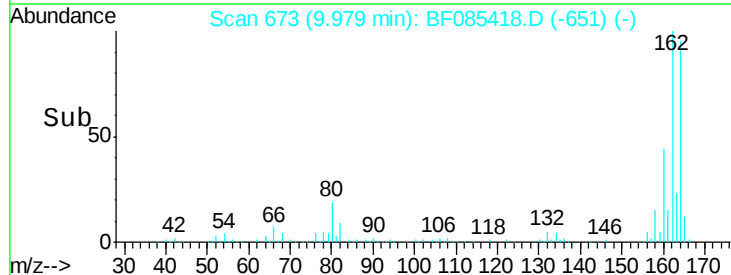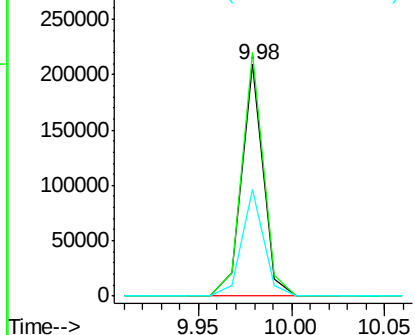


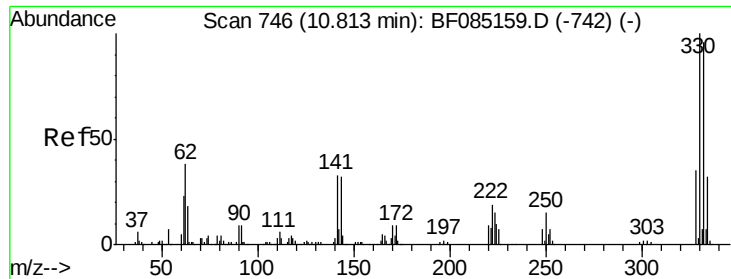




#41
 2,4,6-Tribromophenol
 Concen: 125.28 ng
 RT: 10.77 min Scan# 742
 Delta R.T. -0.05 min
 Lab File: BF085418.D
 Acq: 12 Mar 2016 14:04

Instrument :
 BNA_F
 ClientSampleId :
 SB-30-COMP

Tgt Ion	Ratio	Lower	Upper
330	100		
332	98.6	77.1	115.7
141	40.0	35.0	52.6

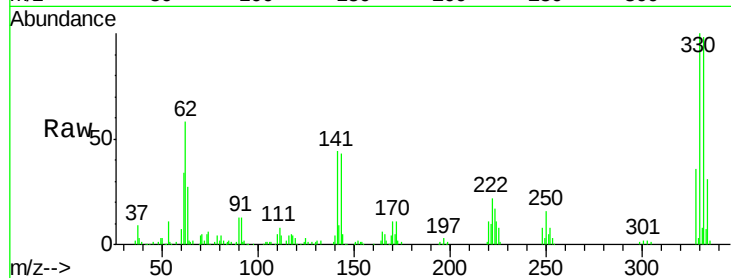


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

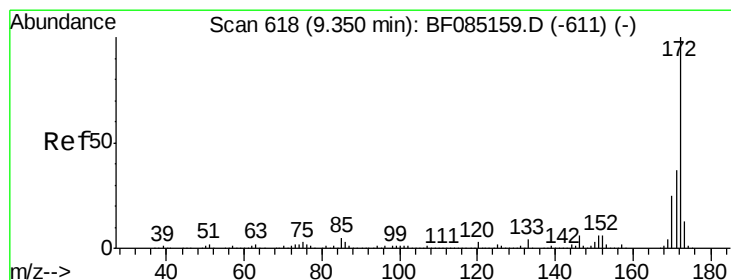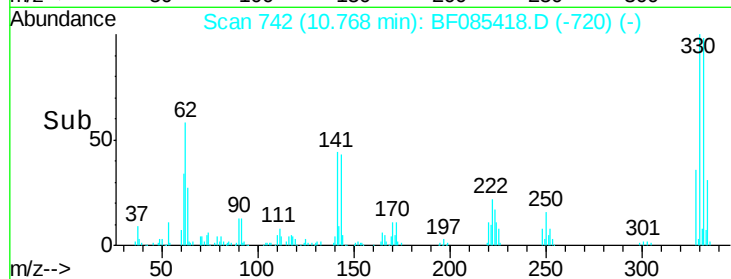
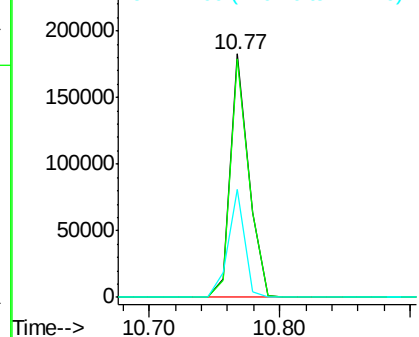



#44
 2-Fluorobiphenyl
 Concen: 94.69 ng
 RT: 9.30 min Scan# 614
 Delta R.T. -0.05 min
 Lab File: BF085418.D
 Acq: 12 Mar 2016 14:04

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	29.3	43.9
170	24.4	20.0	30.0

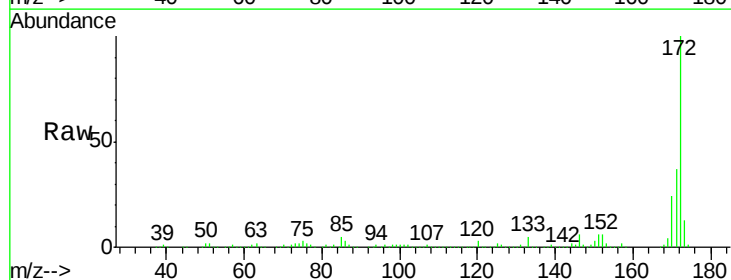

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

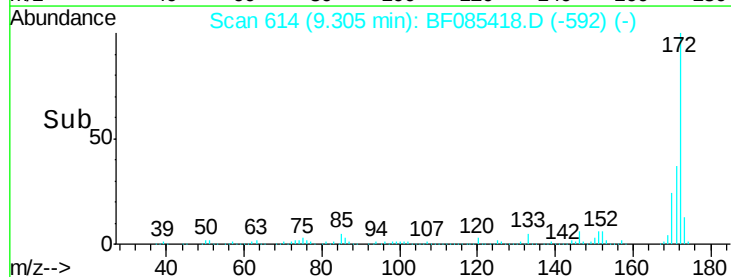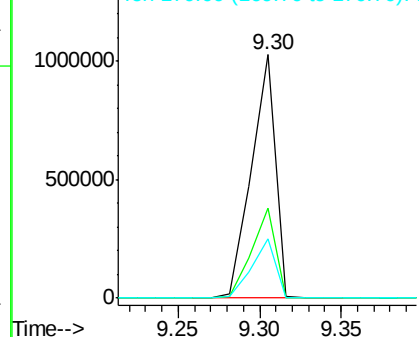

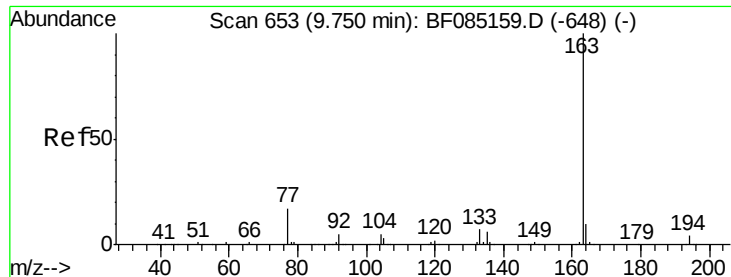

#49

Dimethylphthalate

Concen: 16.39 ng

RT: 9.69 min Scan# 648

Delta R.T. -0.06 min

Lab File: BF085418.D

Acq: 12 Mar 2016 14:04

Instrument :

BNA_F

ClientSampleId :

SB-30-COMP


Tgt Ion:163 Resp: 211577

Ion Ratio Lower Upper

163 100

194 3.6 3.1 4.7




164 9.6 8.2 12.4

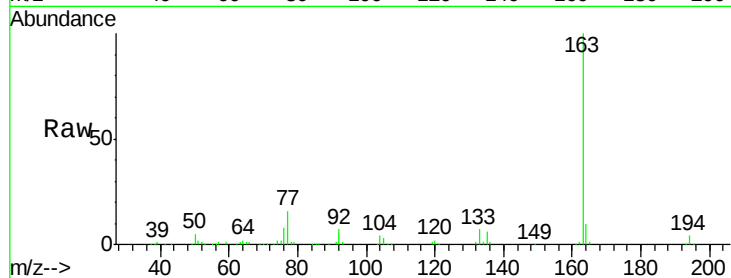

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

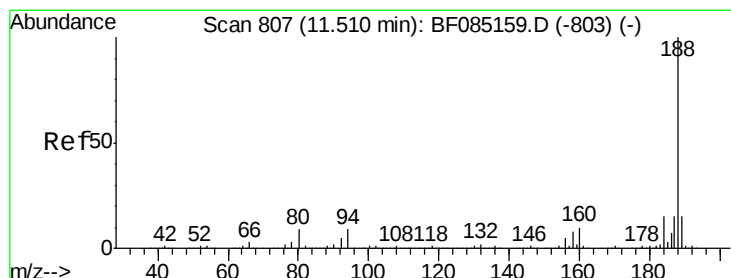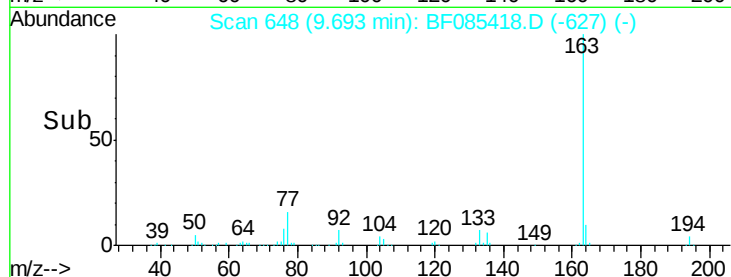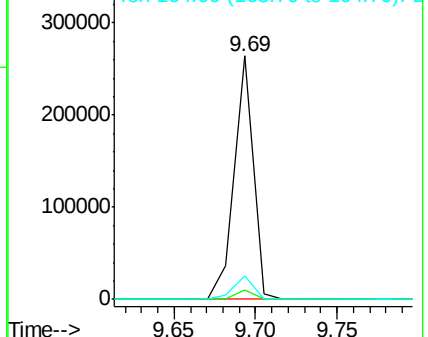

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.46 min Scan# 803

Delta R.T. -0.05 min

Lab File: BF085418.D

Acq: 12 Mar 2016 14:04


Tgt Ion:188 Resp: 261331

Ion Ratio Lower Upper

188 100

94 9.1 7.0 10.6



80 9.7 7.4 11.0

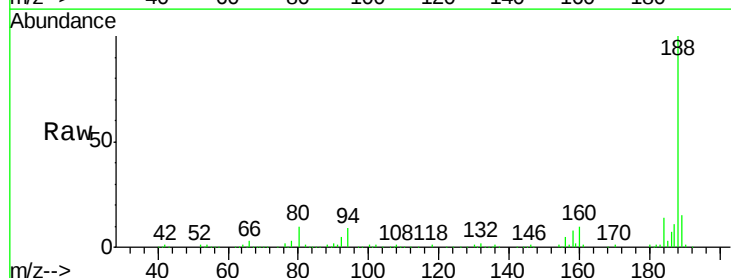


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

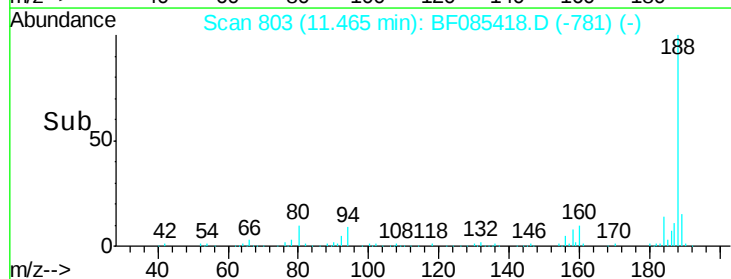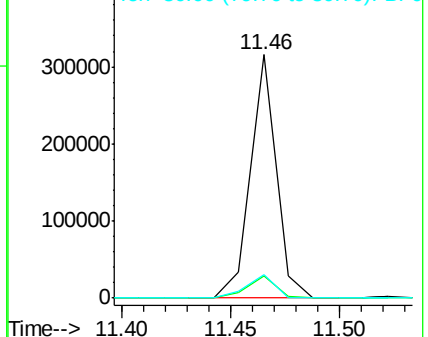

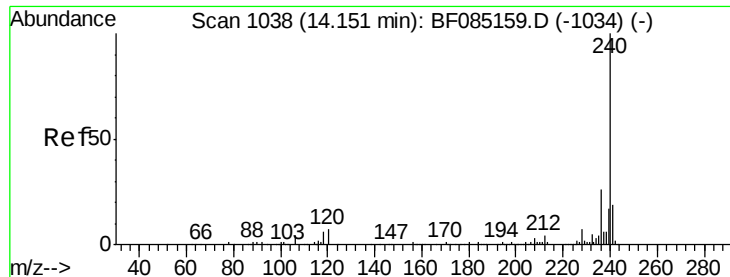

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.11 min Scan# 1034

Delta R.T. -0.05 min

Lab File: BF085418.D

Acq: 12 Mar 2016 14:04

Instrument :

BNA_F

ClientSampleId :

SB-30-COMP


Tgt Ion:240 Resp: 213356

Ion Ratio Lower Upper

240 100

120 12.1 5.3 7.9#




236 25.9 20.7 31.1

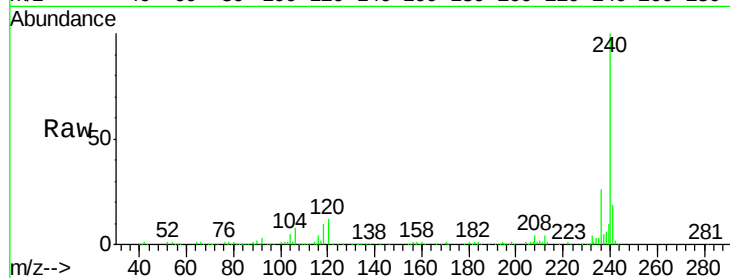

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

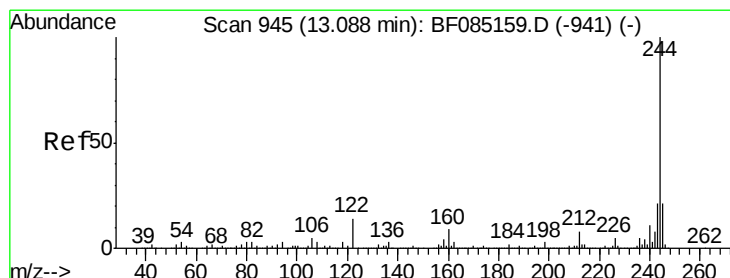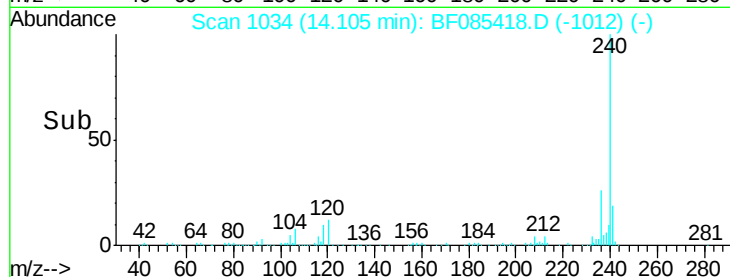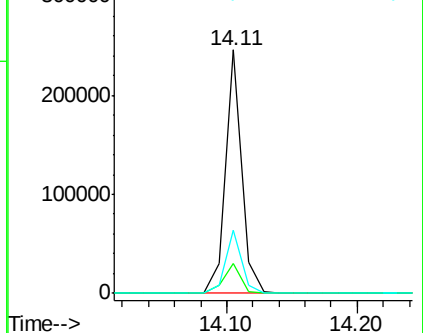

#78

Terphenyl-d14

Concen: 77.68 ng

RT: 13.05 min Scan# 942

Delta R.T. -0.03 min

Lab File: BF085418.D

Acq: 12 Mar 2016 14:04


Tgt Ion:244 Resp: 713950

Ion Ratio Lower Upper

244 100

212 7.5 6.4 9.6



122 11.0 11.4 17.2#

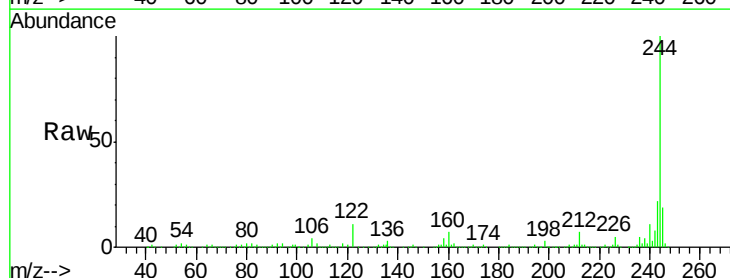


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

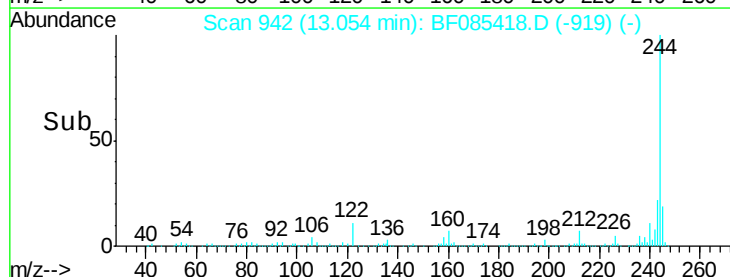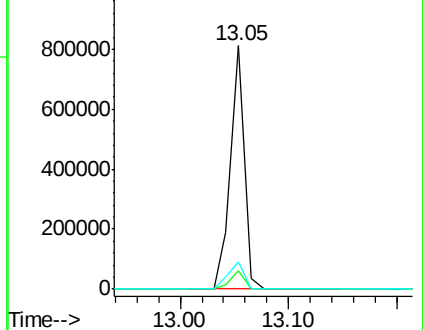


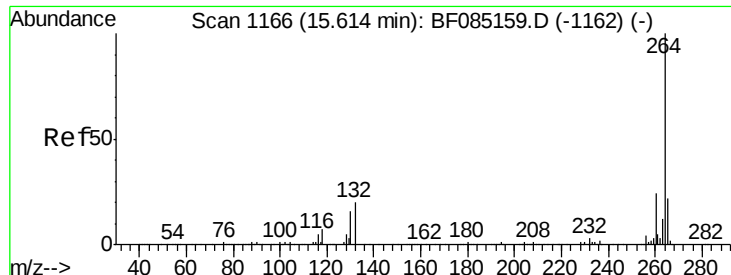

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.57 min Scan# 1162
Delta R.T. -0.05 min
Lab File: BF085418.D
Acq: 12 Mar 2016 14:04

Instrument :
BNA_F
ClientSampleId :
SB-30-COMP

Tgt Ion: 264 Resp: 171379
Ion Ratio Lower Upper
264 100
260 23.2 19.2 28.8
265 21.4 17.3 25.9

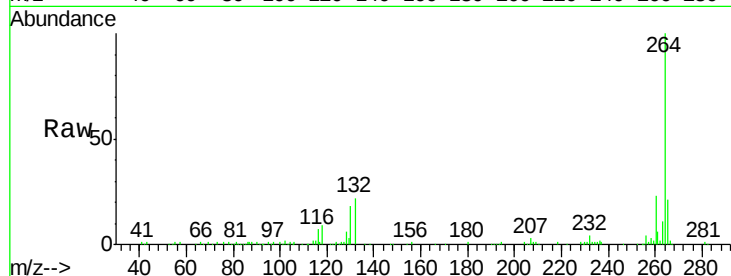

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

