

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031116\
 Data File : BF085378.D
 Acq On : 11 Mar 2016 18:05
 Operator : UM/SJ
 Sample : PB88818BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB88818BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.933	141	144	146	rBV4	80216	112947	2.80%	0.338%
2	3.967	146	147	150	rVV2	82704	83080	2.06%	0.249%
3	4.036	150	153	155	rVB2	67789	136961	3.39%	0.410%
4	5.144	247	250	258	rVB	158974	237272	5.88%	0.710%
5	5.544	282	285	287	rBV	2831744	3658518	90.68%	10.952%
6	6.562	371	374	376	rBV	3283304	3733222	92.53%	11.176%
7	6.699	383	386	388	rBV	3576196	3375499	83.67%	10.105%
8	6.927	404	406	409	rBV	770461	894359	22.17%	2.677%
9	7.087	418	420	423	rBV	2869243	2729270	67.65%	8.170%
10	7.499	453	456	458	rBV	2310005	2523914	62.56%	7.556%
11	8.219	516	519	521	rBV	1456439	1249212	30.96%	3.740%
12	9.293	610	613	616	rBV	3177018	4034466	100.00%	12.078%
13	9.979	670	673	675	rBV	1380435	1314402	32.58%	3.935%
14	10.768	739	742	744	rBV	2463889	2475977	61.37%	7.412%
15	11.465	800	803	805	rBV	1398564	1320692	32.74%	3.954%
16	13.054	939	942	944	rBV	3915343	3950128	97.91%	11.825%
17	14.105	1031	1034	1036	rBV	743759	881315	21.84%	2.638%
18	15.568	1159	1162	1165	rBV	537497	693328	17.19%	2.076%


Sum of corrected areas: 33404562

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031116\
Data File : BF085378.D
Acq On : 11 Mar 2016 18:05
Operator : UM/SJ
Sample : PB88818BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88818BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

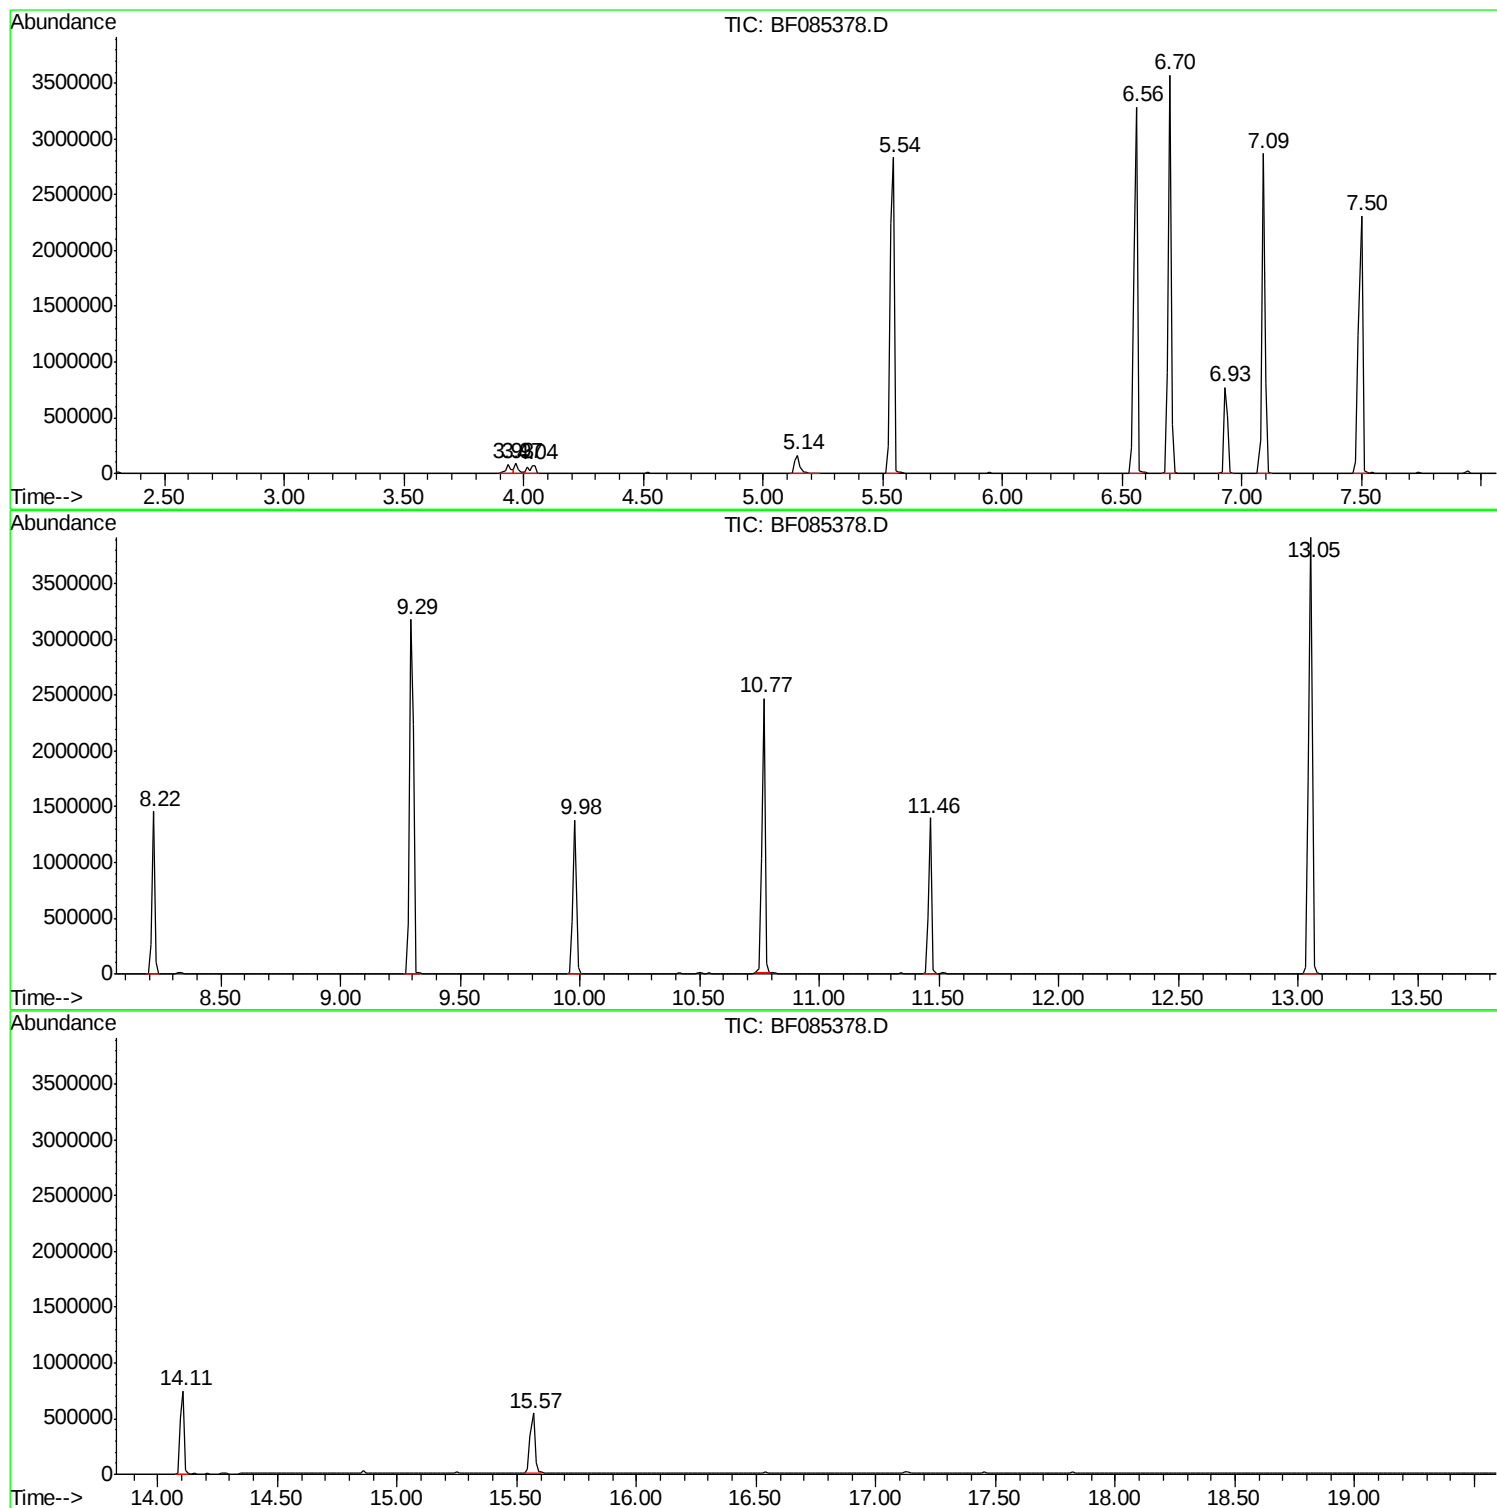

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031116\
Data File : BF085378.D
Acq On : 11 Mar 2016 18:05
Operator : UM/SJ
Sample : PB88818BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88818BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.14	5.31 ng	237272	1,4-Dichlorobenzene-d4	6.93

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25
3		Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17
4		(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9
5		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

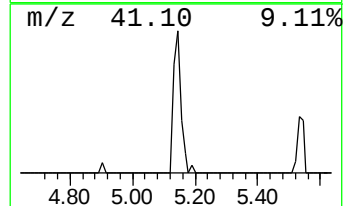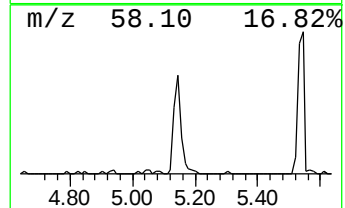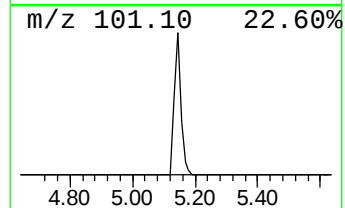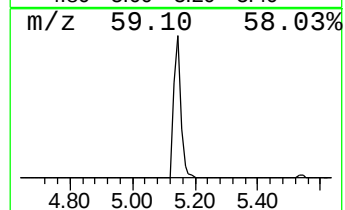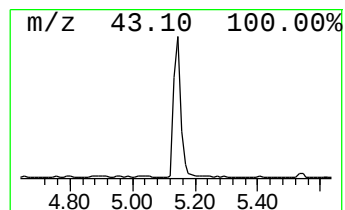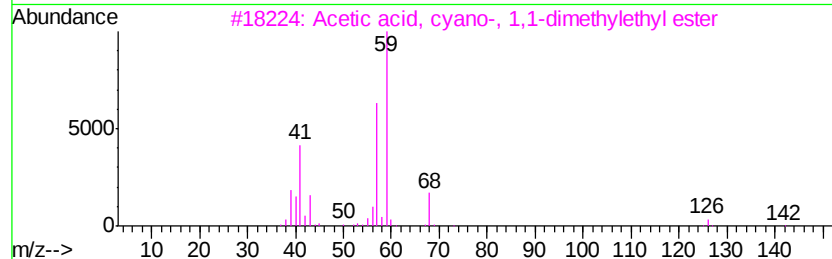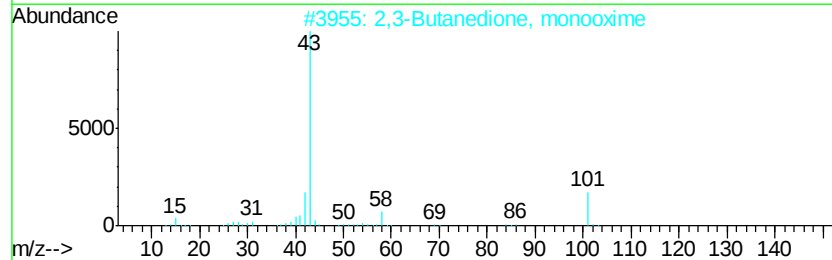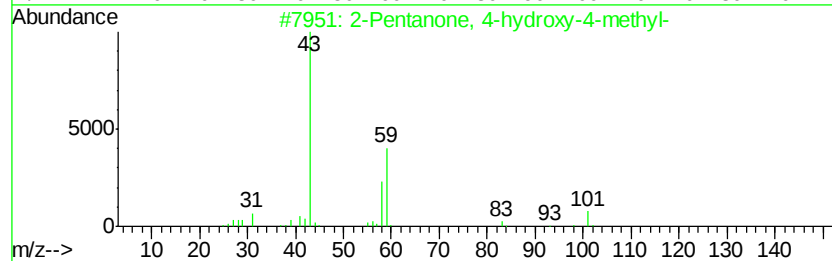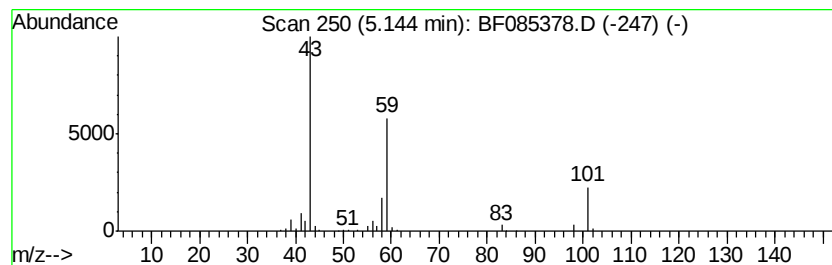

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031116\
Data File : BF085378.D
Acq On : 11 Mar 2016 18:05
Operator : UM/SJ
Sample : PB88818BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88818BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown6.70 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.70	75.48 ng	3375500	1,4-Dichlorobenzene-d4	6.93

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

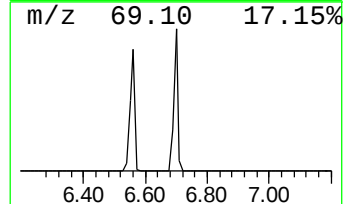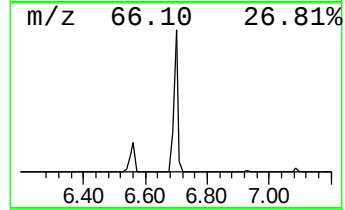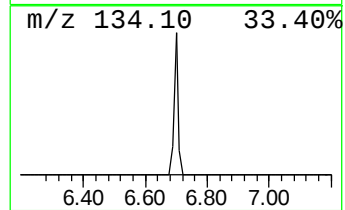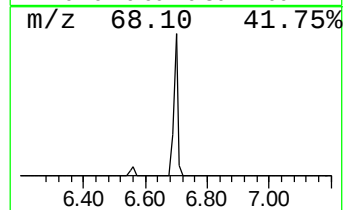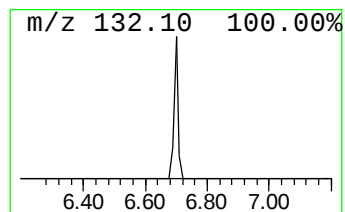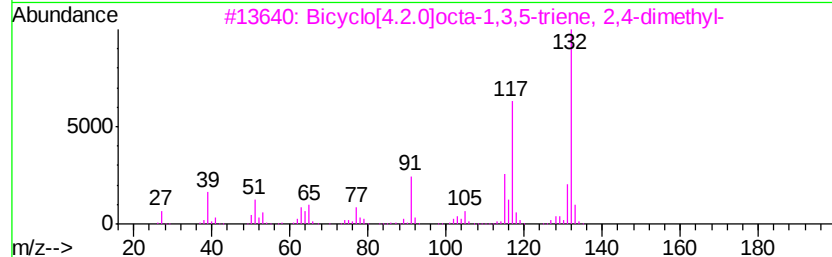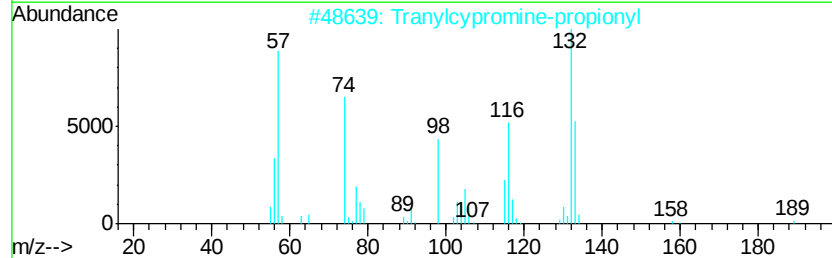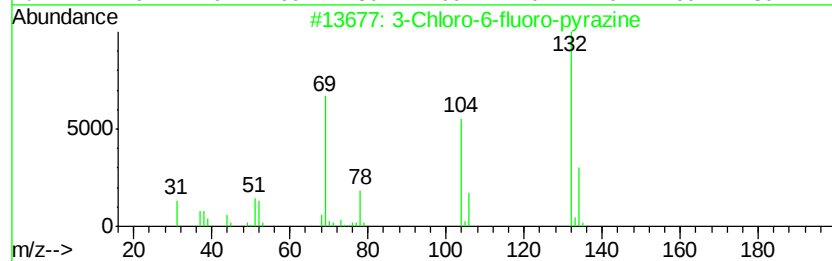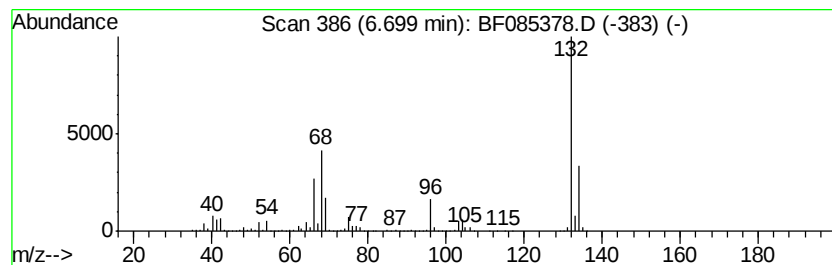

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031116\
Data File : BF085378.D
Acq On : 11 Mar 2016 18:05
Operator : UM/SJ
Sample : PB88818BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88818BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.14	5.3	ng	237272	1	6.93	894359	20.0
unknown6.70	6.70	75.5	ng	3375500	1	6.93	894359	20.0