


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031116\
 Data File : BF085368.D
 Acq On : 11 Mar 2016 13:19
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 04 00:54:58 2016

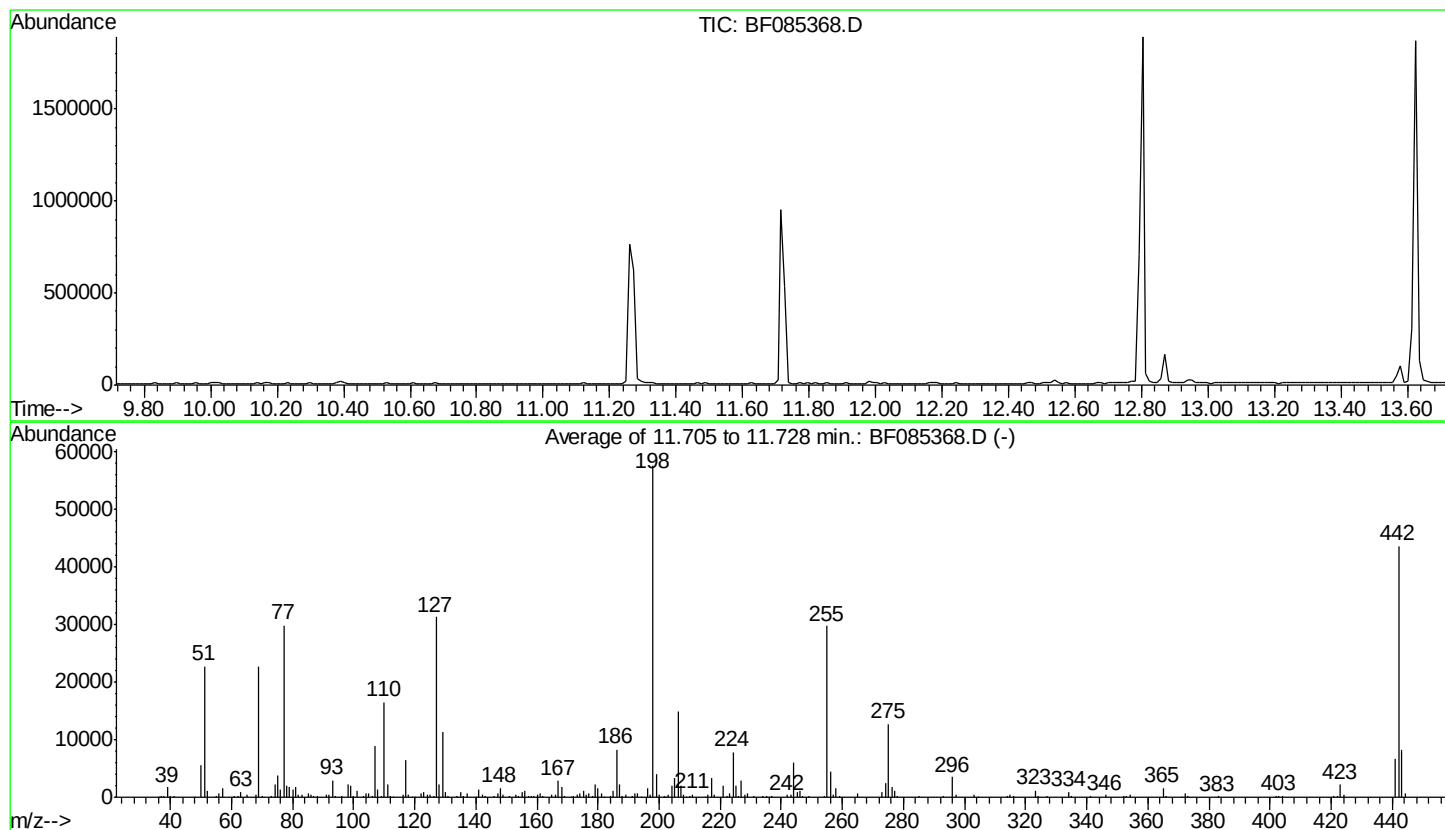

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	22698	PASS
68	69	0.00	2	1.5	346	PASS
69	198	0.00	100	39.6	22786	PASS
70	69	0.00	2	0.7	152	PASS
127	198	10	80	54.3	31289	PASS
197	198	0.00	2	0.7	419	PASS
198	198	100	100	100.0	57597	PASS
199	198	5	9	6.8	3907	PASS
275	198	10	60	22.2	12770	PASS
365	198	1	100	2.8	1627	PASS
441	442	0.01	24	15.5	6752	PASS
442	198	50	100	75.8	43685	PASS
443	442	15	24	18.8	8204	PASS