


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031116\
 Data File : BF085393.D
 Acq On : 12 Mar 2016 2:28
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 04 00:54:58 2016

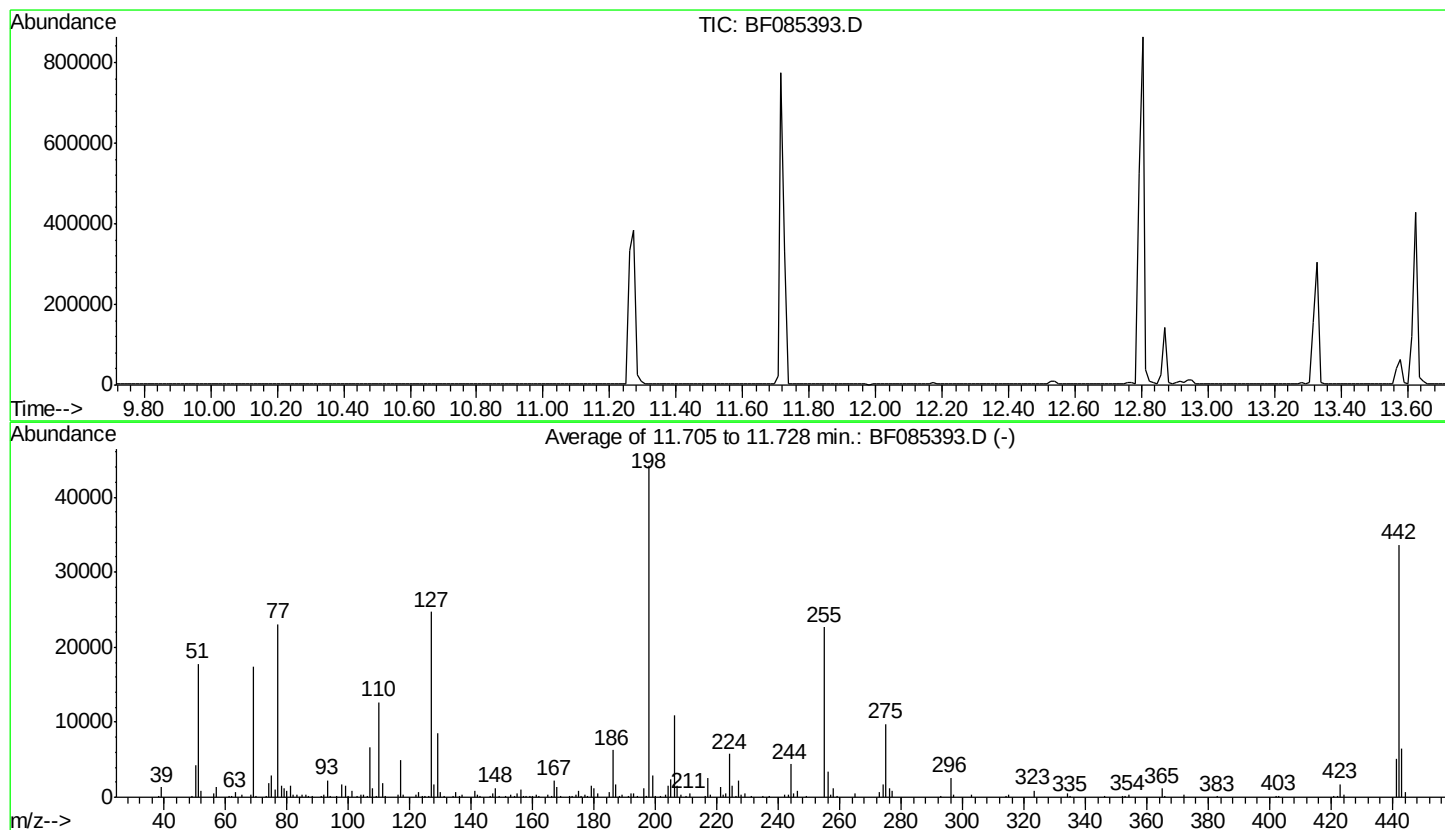

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	17756	PASS
68	69	0.00	2	1.7	287	PASS
69	198	0.00	100	39.3	17368	PASS
70	69	0.00	2	0.6	100	PASS
127	198	10	80	56.0	24737	PASS
197	198	0.00	2	0.5	226	PASS
198	198	100	100	100.0	44196	PASS
199	198	5	9	6.5	2894	PASS
275	198	10	60	22.2	9809	PASS
365	198	1	100	2.7	1185	PASS
441	442	0.01	24	15.0	5064	PASS
442	198	50	100	76.2	33665	PASS
443	442	15	24	19.1	6442	PASS