


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031117\
 Data File : BF093564.D
 Acq On : 11 Mar 2017 12:53
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 13 15:05:08 2017

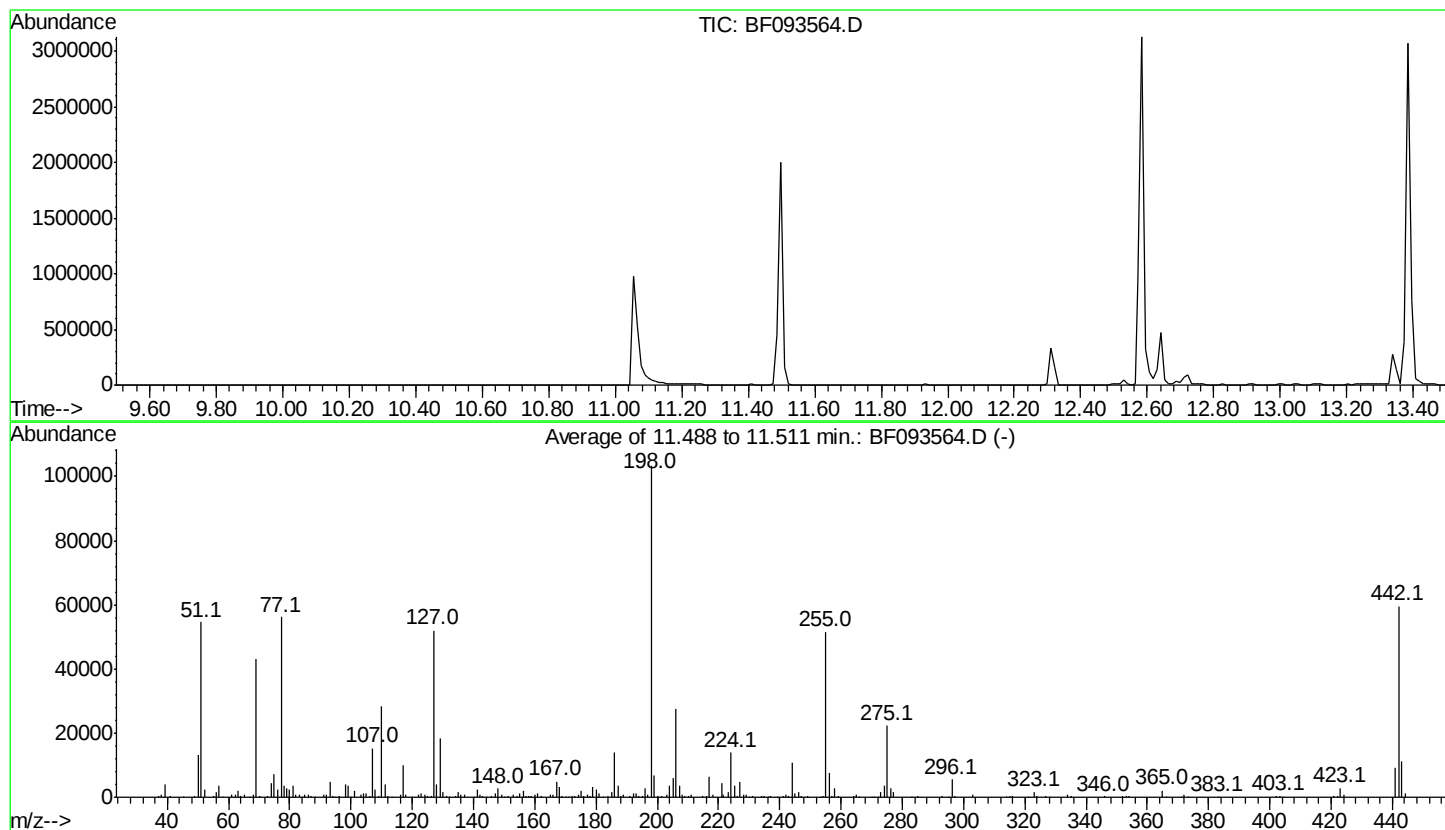

AutoFind: Scans 840, 841, 842; Background Corrected with Scan 837

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.9	54647	PASS
68	69	0.00	2	1.7	744	PASS
69	198	0.00	100	41.7	43118	PASS
70	69	0.00	2	0.6	248	PASS
127	198	10	80	50.3	51968	PASS
197	198	0.00	2	0.9	882	PASS
198	198	100	100	100.0	103367	PASS
199	198	5	9	6.7	6969	PASS
275	198	10	60	21.6	22317	PASS
365	198	1	100	2.0	2063	PASS
441	442	0.01	24	15.5	9266	PASS
442	198	50	100	57.7	59650	PASS
443	442	15	24	18.9	11274	PASS