


Data Path : Z:\HPCHEM1\BNA_F\Data\BF031117\
 Data File : BF093586.D
 Acq On : 12 Mar 2017 3:04
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 13 15:05:08 2017

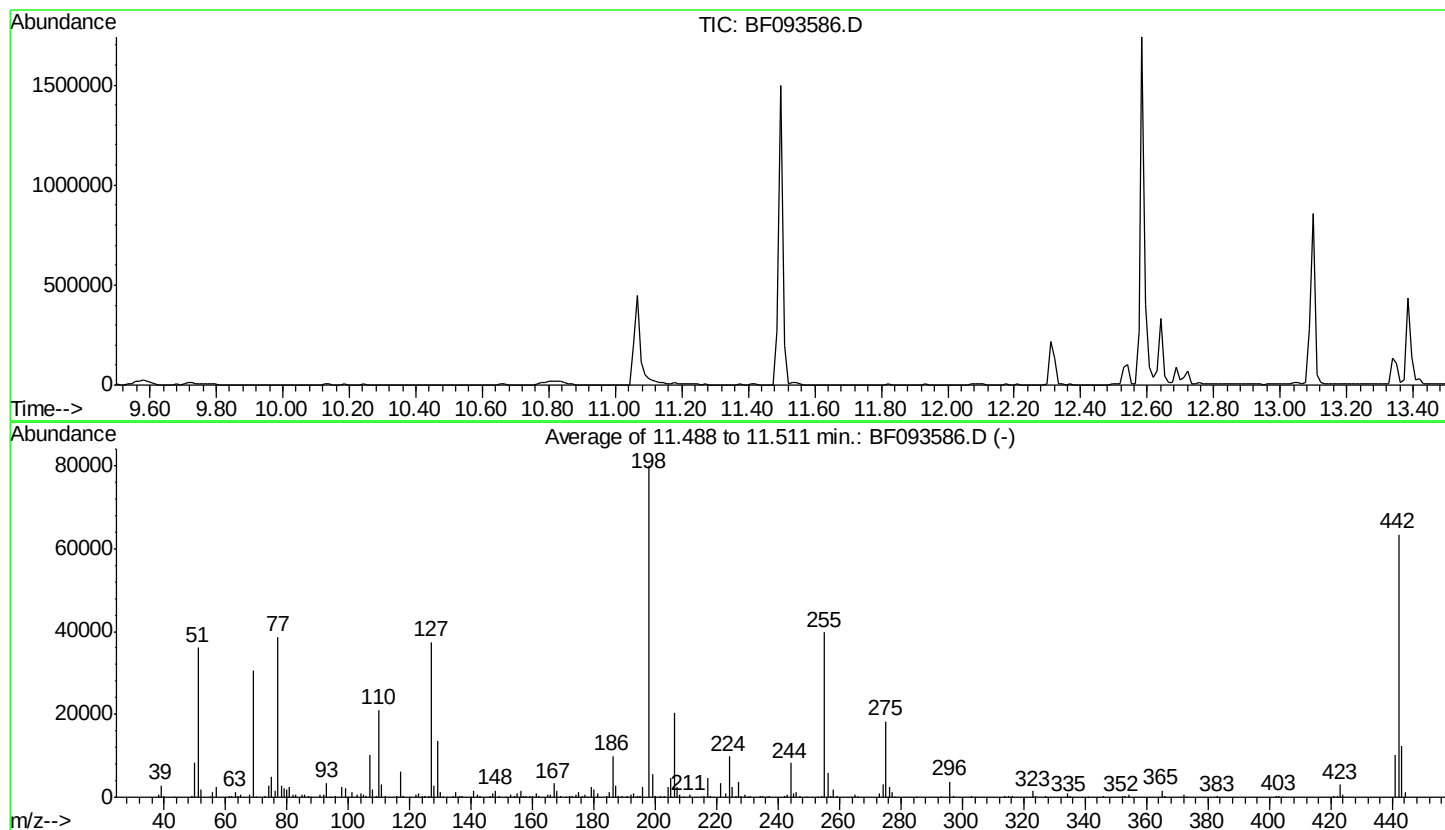

AutoFind: Scans 840, 841, 842; Background Corrected with Scan 837

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	36085	PASS
68	69	0.00	2	1.9	581	PASS
69	198	0.00	100	38.2	30566	PASS
70	69	0.00	2	0.4	119	PASS
127	198	10	80	46.8	37459	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80013	PASS
199	198	5	9	6.9	5499	PASS
275	198	10	60	22.8	18246	PASS
365	198	1	100	1.9	1553	PASS
441	442	0.01	24	16.2	10260	PASS
442	198	50	100	79.2	63395	PASS
443	442	15	24	19.7	12501	PASS