


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031120\
 Data File : BF119347.D
 Acq On : 11 Mar 2020 14:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 06 23:38:46 2020

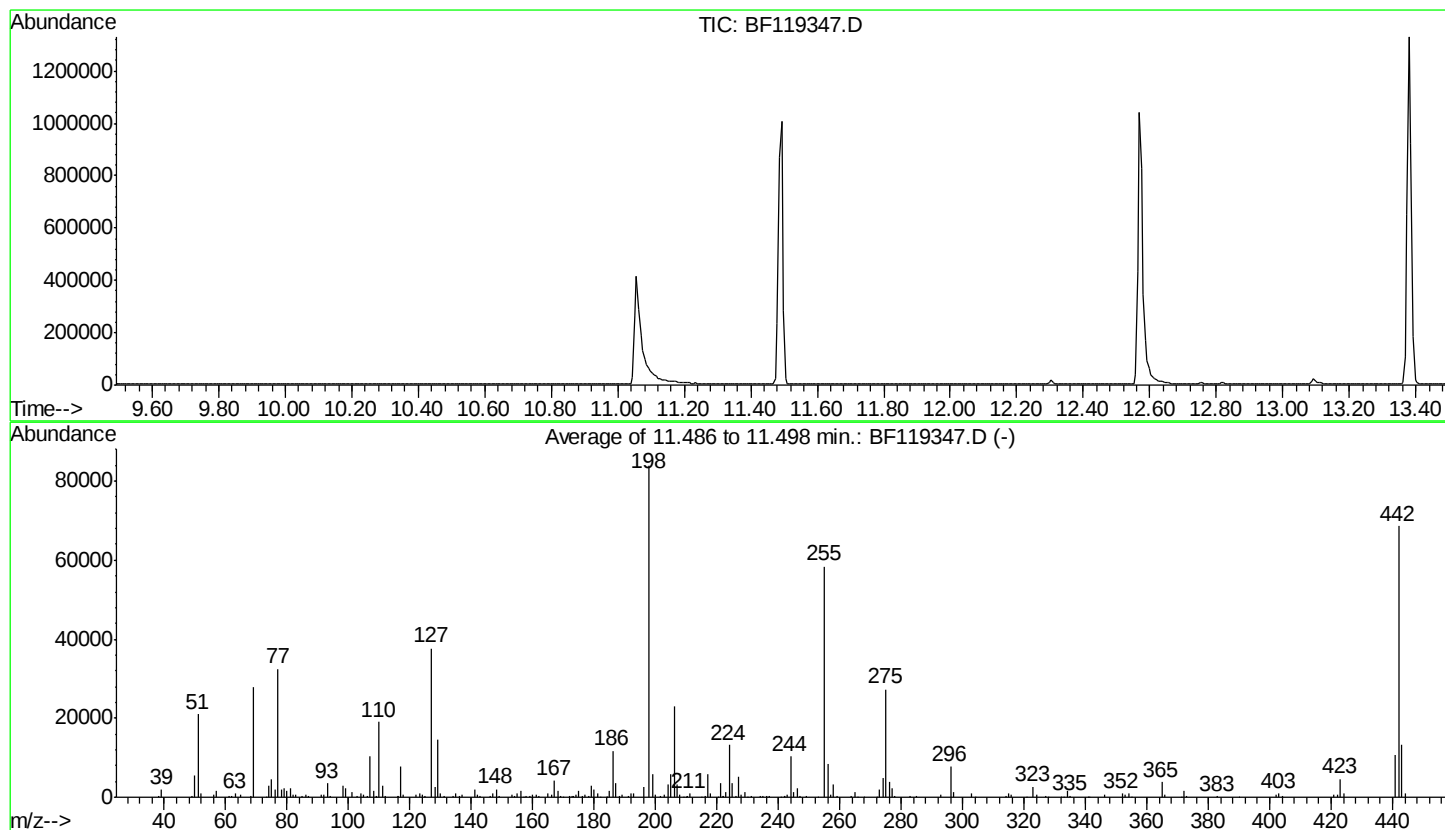

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.1	21048	PASS
68	69	0.00	2	0.9	242	PASS
69	198	0.00	100	33.1	27815	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.8	37631	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83930	PASS
199	198	5	9	6.9	5781	PASS
275	198	10	60	32.6	27333	PASS
365	198	1	100	4.5	3774	PASS
441	198	0.01	100	12.8	10777	PASS
442	198	50	100	81.7	68592	PASS
443	442	15	24	19.3	13220	PASS