
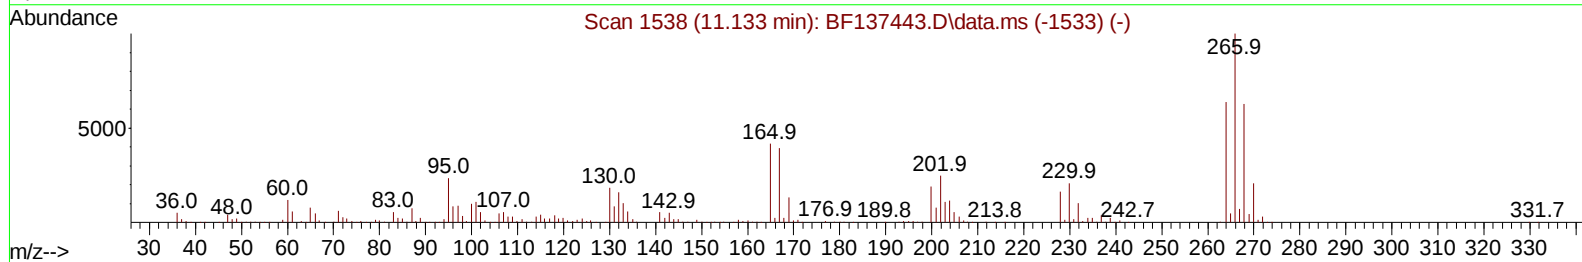
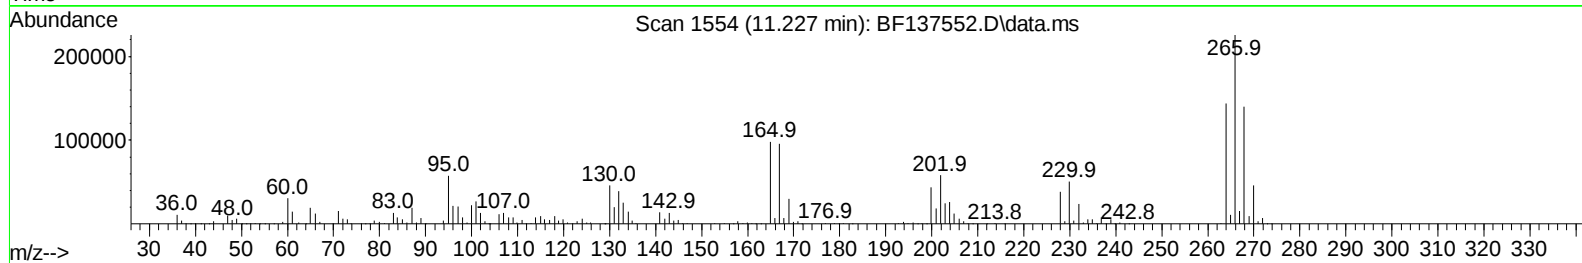


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031124\
Data File : BF137552.D
Acq On : 11 Mar 2024 12:39
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 12 02:47:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 12 02:00:03 2024
Response via : Initial Calibration

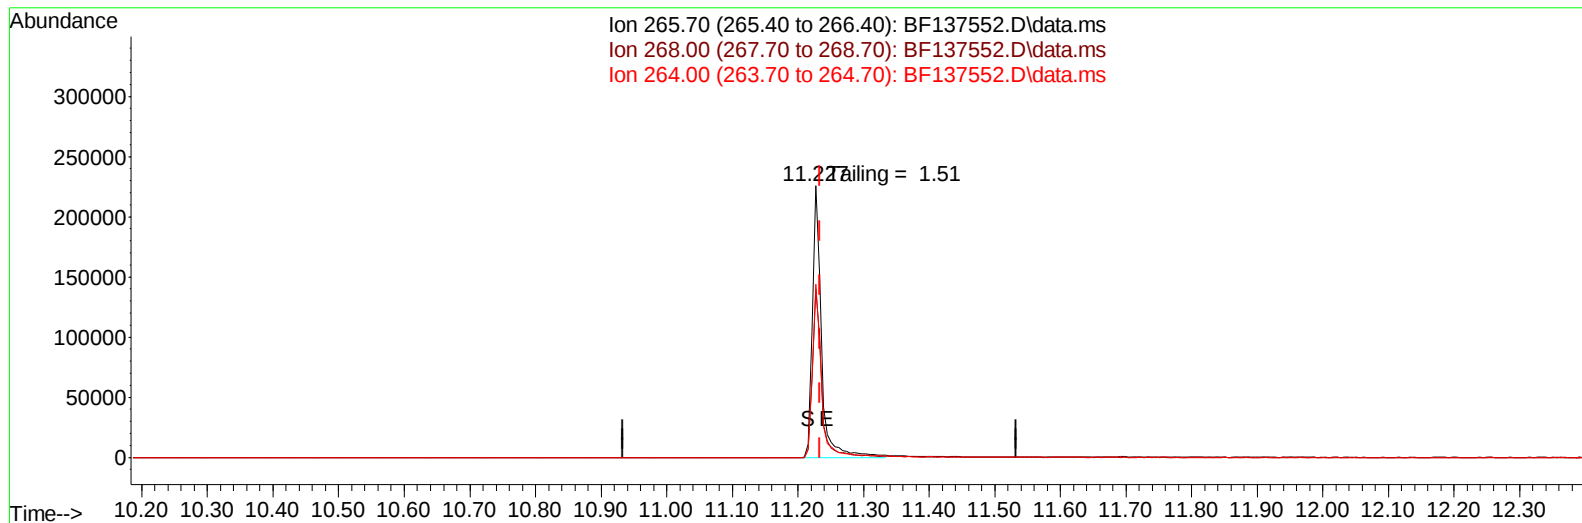

TIC: BF137552.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.006) 30390.24 ng

response 223525

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.00
264.00	63.60	63.67
0.00	0.00	0.00

