
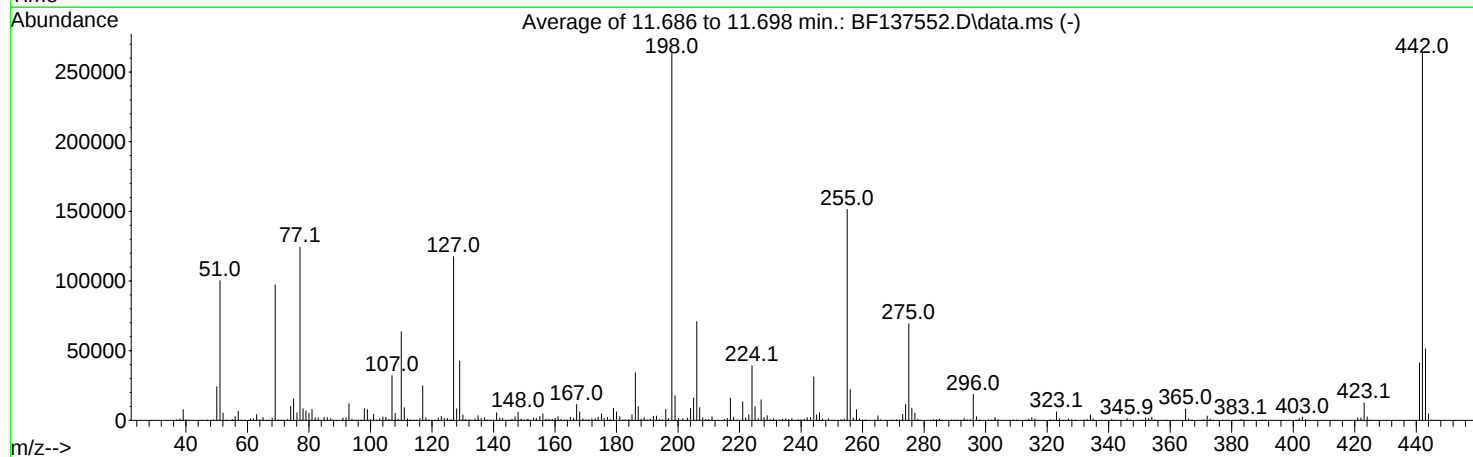


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031124\
Data File : BF137552.D
Acq On : 11 Mar 2024 12:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 12 02:00:03 2024

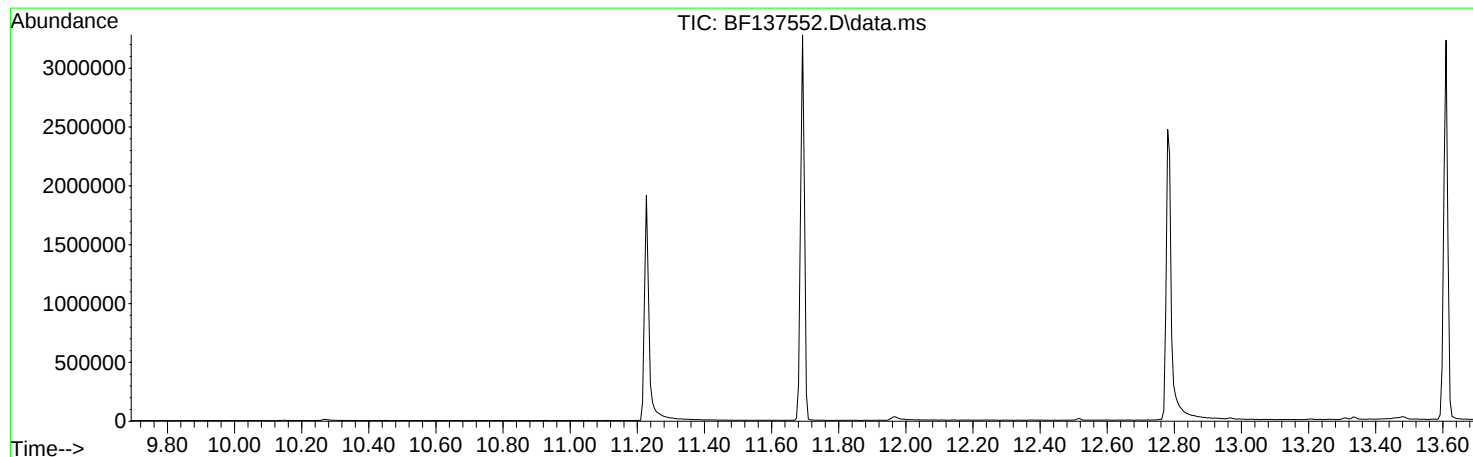




AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	100203	PASS
68	69	0.00	2	1.6	1581	PASS
69	198	0.00	100	37.0	97320	PASS
70	69	0.00	2	0.5	522	PASS
127	198	10	80	44.7	117637	PASS
197	198	0.00	2	0.5	1223	PASS
198	198	100	100	100.0	263339	PASS
199	198	5	9	6.7	17717	PASS
275	198	10	60	26.3	69224	PASS
365	198	1	100	3.1	8131	PASS
441	198	0.01	100	15.6	41179	PASS
442	442	50	100	100.0	263992	PASS
443	442	15	24	19.4	51331	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031124\
Data File : BF137552.D
Acq On : 11 Mar 2024 12:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 12 02:47:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 12 02:00:03 2024
Response via : Initial Calibration

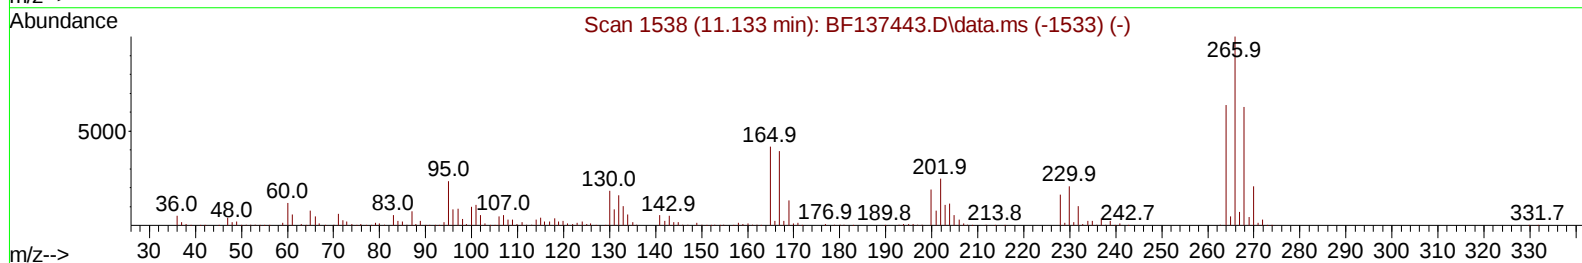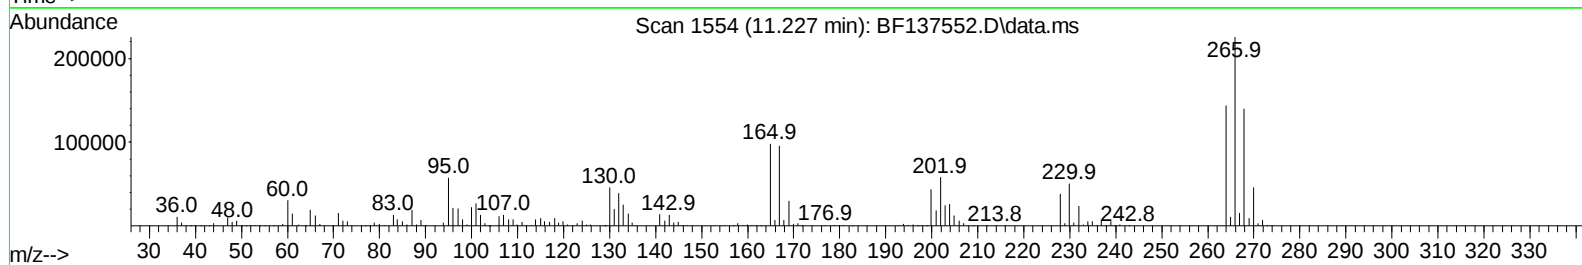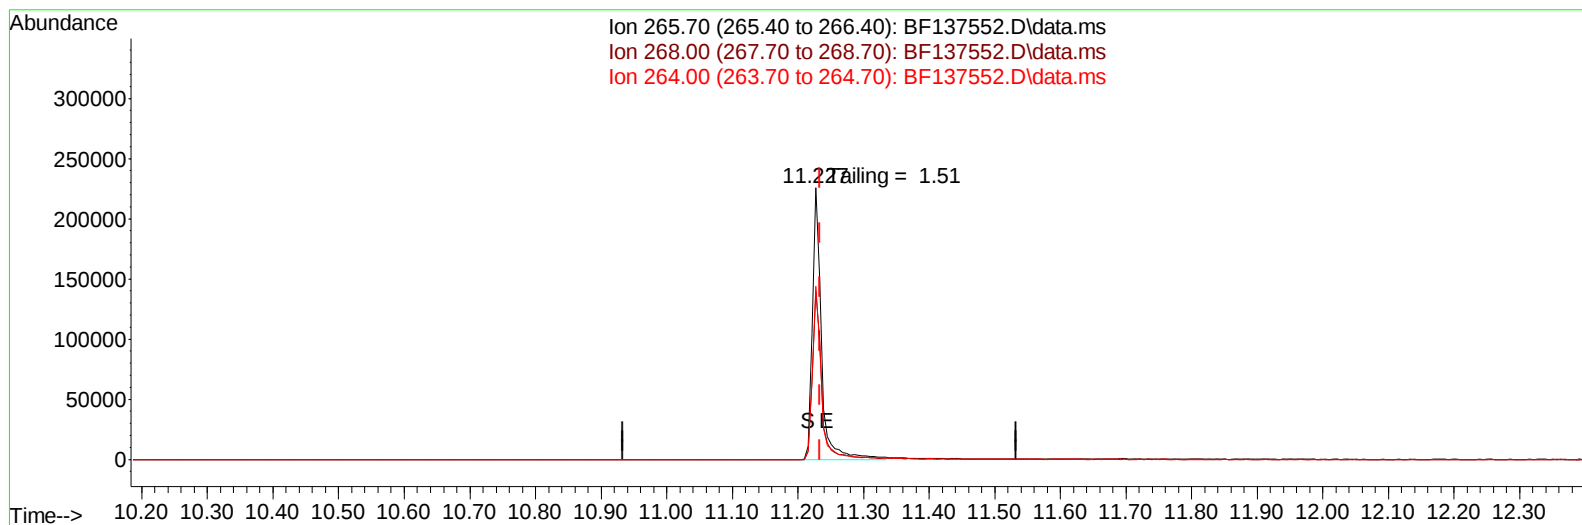

TIC: BF137552.D\data.ms



(70) Pentachlorophenol (C)

11.227min (-0.006) 30390.24 ng

response 223525

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.00
264.00	63.60	63.67
0.00	0.00	0.00

Instrument :
BNA_F
ClientSampleId :
DFTPP

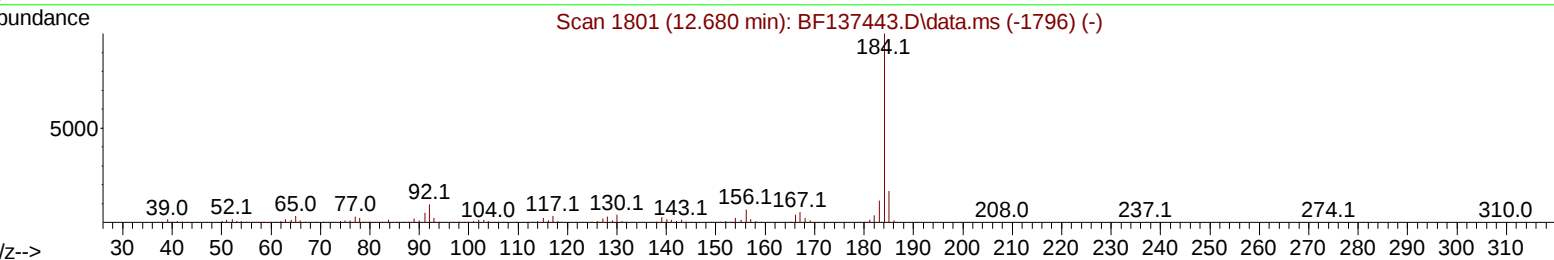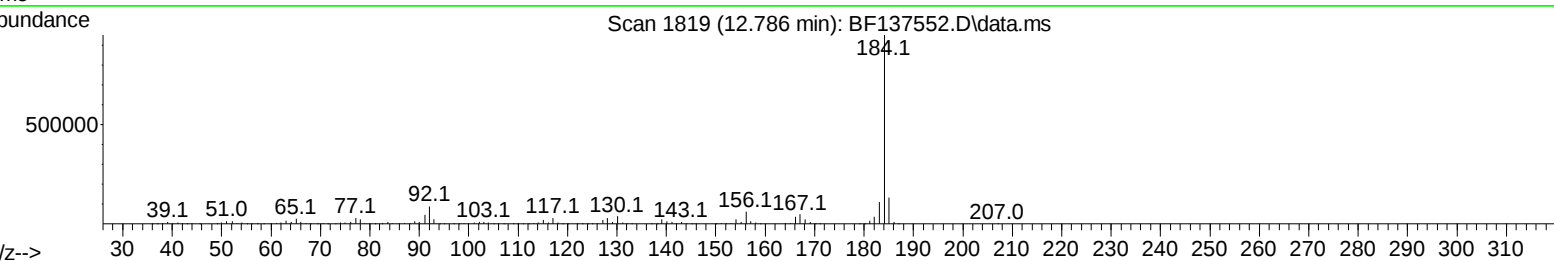

TIC: BF137552.D\data.ms

(77) Benzidine

12.786min (-0.000) 0.00 ng

response **1122364**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	13.89
183.00	11.60	11.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/11/2024	BNA_F	<u>BF137552.D</u>
Compound Name	Response	Retention Time
DDT	515818	13.61
DDD	7442	13.333
DDE	1145	12.968
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8587	524405	1.64

Instrument :
BNA_F
ClientSampleId :
DFTPP