

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031125\
 Data File : BF141913.D
 Acq On : 11 Mar 2025 13:20
 Operator : RC/JU
 Sample : PB167078BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB167078BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141913.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.263	22	29	35	rVB	72007	124097	1.29%	0.269%
2	5.504	573	580	586	rBV	3592499	5118809	53.07%	11.115%
3	6.498	742	749	755	rBV	3394558	5115295	53.03%	11.107%
4	6.875	808	813	819	rBV	901759	1169180	12.12%	2.539%
5	7.439	901	909	914	rBV	2412402	3518582	36.48%	7.640%
6	8.157	1025	1031	1053	rBV	1178045	1577508	16.36%	3.425%
7	9.233	1207	1214	1219	rBV	5387839	7444674	77.18%	16.165%
8	9.910	1322	1329	1349	rVB	1488785	1955132	20.27%	4.245%
9	10.704	1454	1464	1469	rBV	4024789	5541572	57.45%	12.033%
10	11.398	1576	1582	1589	rBV	1719501	2172336	22.52%	4.717%
11	12.986	1846	1852	1858	rBV	6946321	9645239	100.00%	20.944%
12	14.033	2025	2030	2040	rBV	1204590	1543894	16.01%	3.352%
13	15.504	2274	2280	2295	rBV	705436	1126839	11.68%	2.447%




Sum of corrected areas: 46053157

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031125\
Data File : BF141913.D
Acq On : 11 Mar 2025 13:20
Operator : RC/JU
Sample : PB167078BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167078BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

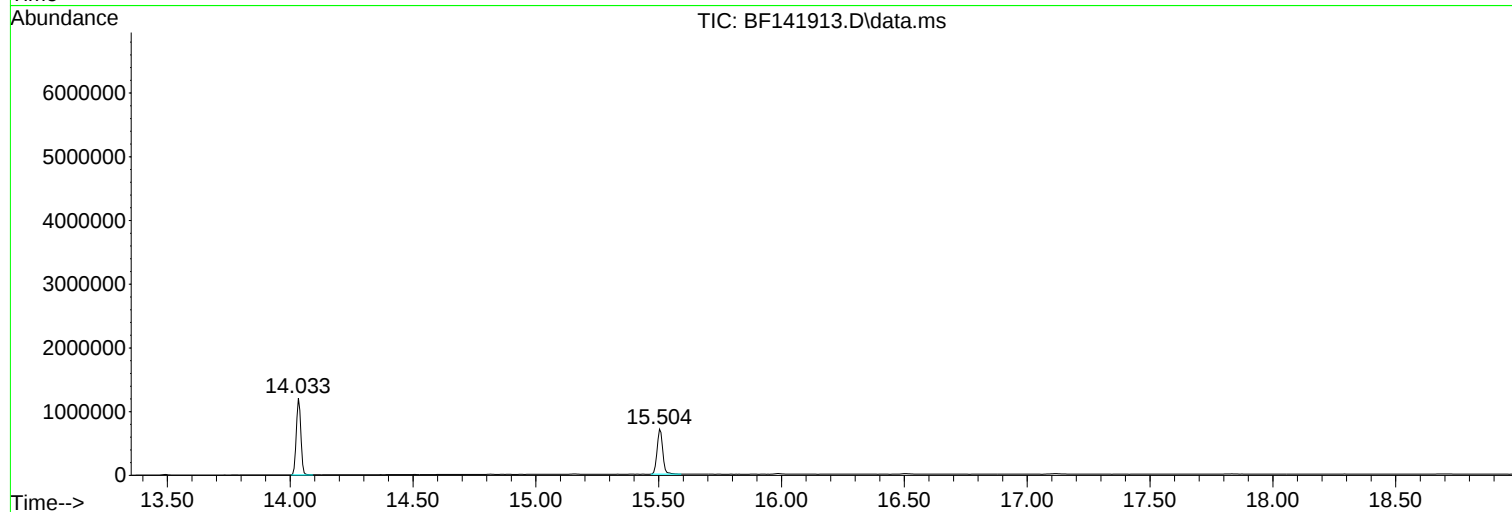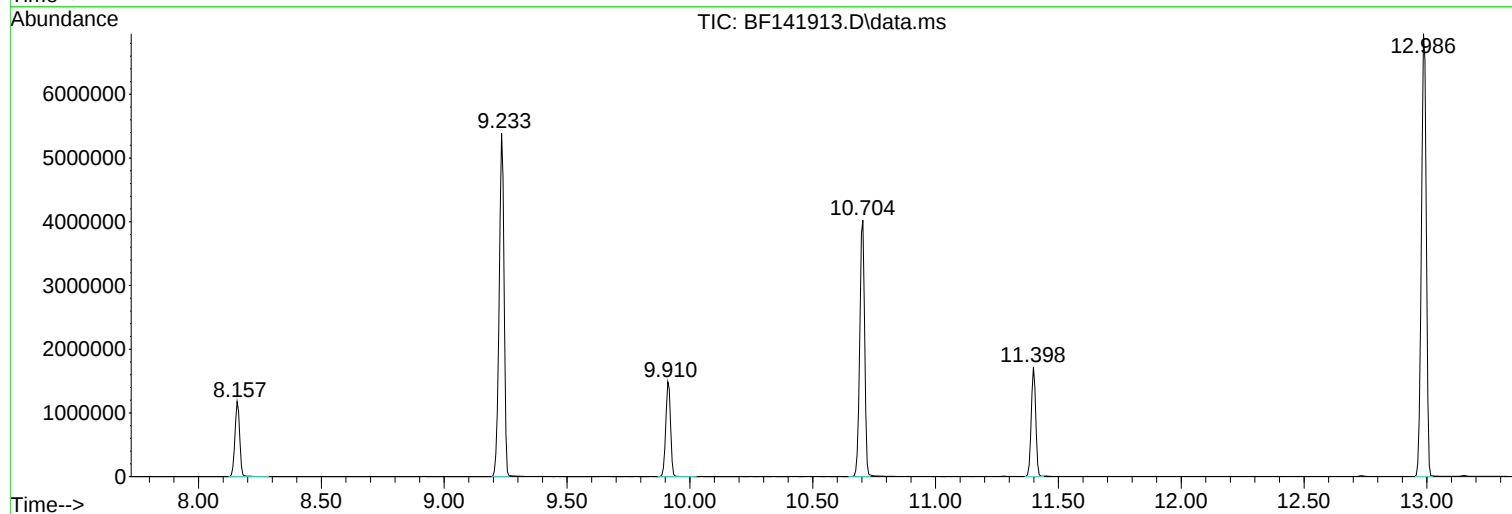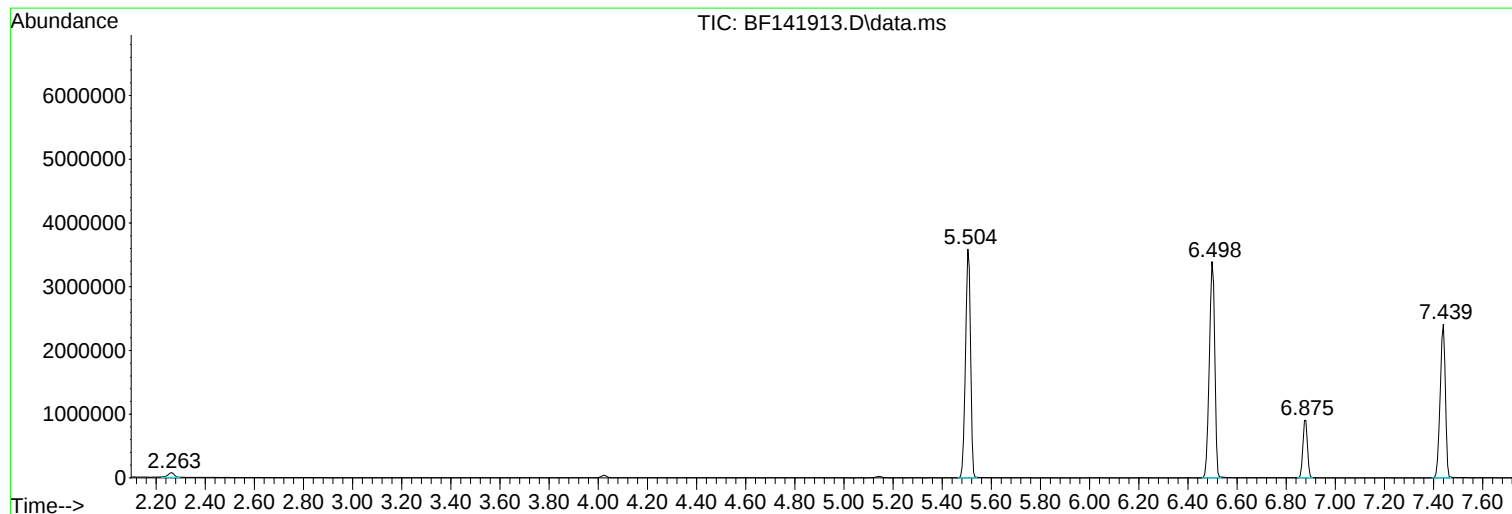

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031125\
Data File : BF141913.D
Acq On : 11 Mar 2025 13:20
Operator : RC/JU
Sample : PB167078BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167078BL








Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.263	2.12 ng	124097	1,4-Dichlorobenzene-d4	6.881

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	36
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

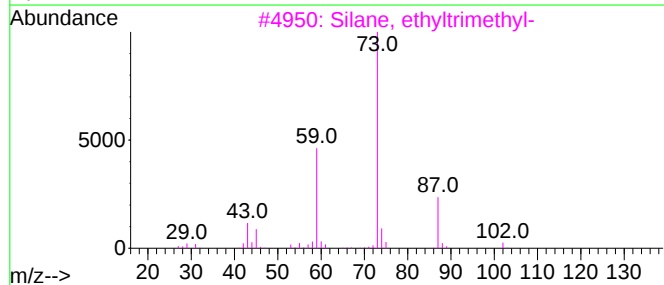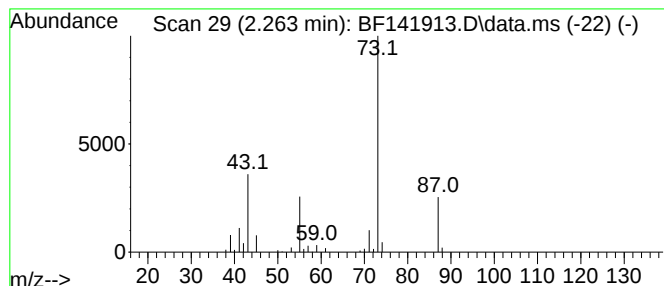

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031125\
Data File : BF141913.D
Acq On : 11 Mar 2025 13:20
Operator : RC/JU
Sample : PB167078BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167078BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.263	2.1	ng	124097	1	6.881	1169180	20.0