


Data Path : Z:\HPCHEM1\BNA_F\Data\BF031215\
 Data File : BF077725.D
 Acq On : 12 Mar 2015 12:00
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 12 14:10:27 2015

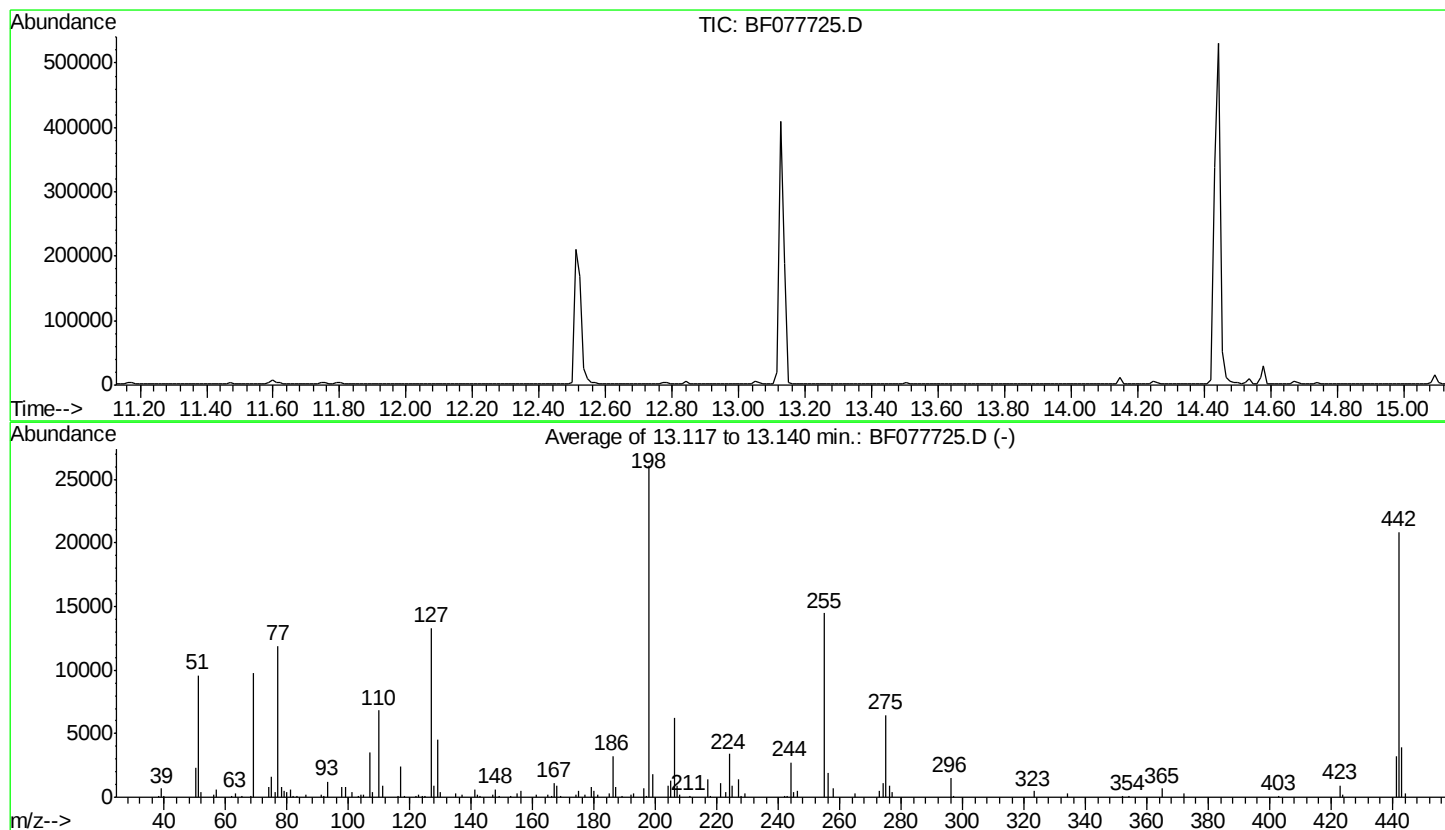

AutoFind: Scans 1070, 1071, 1072; Background Corrected with Scan 1067

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	9610	PASS
68	69	0.00	2	1.4	137	PASS
69	198	0.00	100	37.6	9811	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.1	13323	PASS
197	198	0.00	2	0.5	127	PASS
198	198	100	100	100.0	26084	PASS
199	198	5	9	6.9	1803	PASS
275	198	10	60	24.8	6458	PASS
365	198	1	100	2.6	691	PASS
441	442	0.01	24	15.5	3238	PASS
442	198	50	100	79.9	20845	PASS
443	442	15	24	18.7	3907	PASS