

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031218\
 Data File : BF103591.D
 Acq On : 12 Mar 2018 19:29
 Operator : SJ/JU
 Sample : J1867-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CPS043071

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.098	508	512	523	rBV	18155	49013	1.19%	0.176%
2	5.492	576	579	607	rBV	434716	1534177	37.23%	5.511%
3	6.516	749	753	769	rBV	302004	928060	22.52%	3.334%
4	6.634	769	773	795	rVB	2109332	3298549	80.04%	11.849%
5	6.857	808	811	833	rVB	441179	750681	18.22%	2.696%
6	7.010	833	837	863	rBV	2461017	3009179	73.02%	10.809%
7	7.428	904	908	933	rBV	1920639	2869164	69.62%	10.306%
8	8.139	1026	1029	1061	rBV	597190	1090408	26.46%	3.917%
9	9.216	1208	1212	1221	rBV	3628118	4120943	100.00%	14.803%
10	9.810	1309	1313	1318	rBV	66168	56717	1.38%	0.204%
11	9.898	1324	1328	1349	rBV	1003472	1108394	26.90%	3.981%
12	10.310	1395	1398	1401	rVB	84277	69813	1.69%	0.251%
13	10.698	1460	1464	1476	rBV	1894279	2519329	61.13%	9.050%
14	10.780	1476	1478	1489	rVB	77938	111213	2.70%	0.399%
15	11.398	1579	1583	1600	rBV	868798	1097001	26.62%	3.940%
16	12.980	1847	1852	1865	rBV	2784410	3404207	82.61%	12.228%
17	14.057	2031	2035	2049	rBV	772912	991155	24.05%	3.560%
18	15.562	2286	2291	2307	rBV	469273	831218	20.17%	2.986%


Sum of corrected areas: 27839221

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031218\
Data File : BF103591.D
Acq On : 12 Mar 2018 19:29
Operator : SJ/JU
Sample : J1867-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CPS043071

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

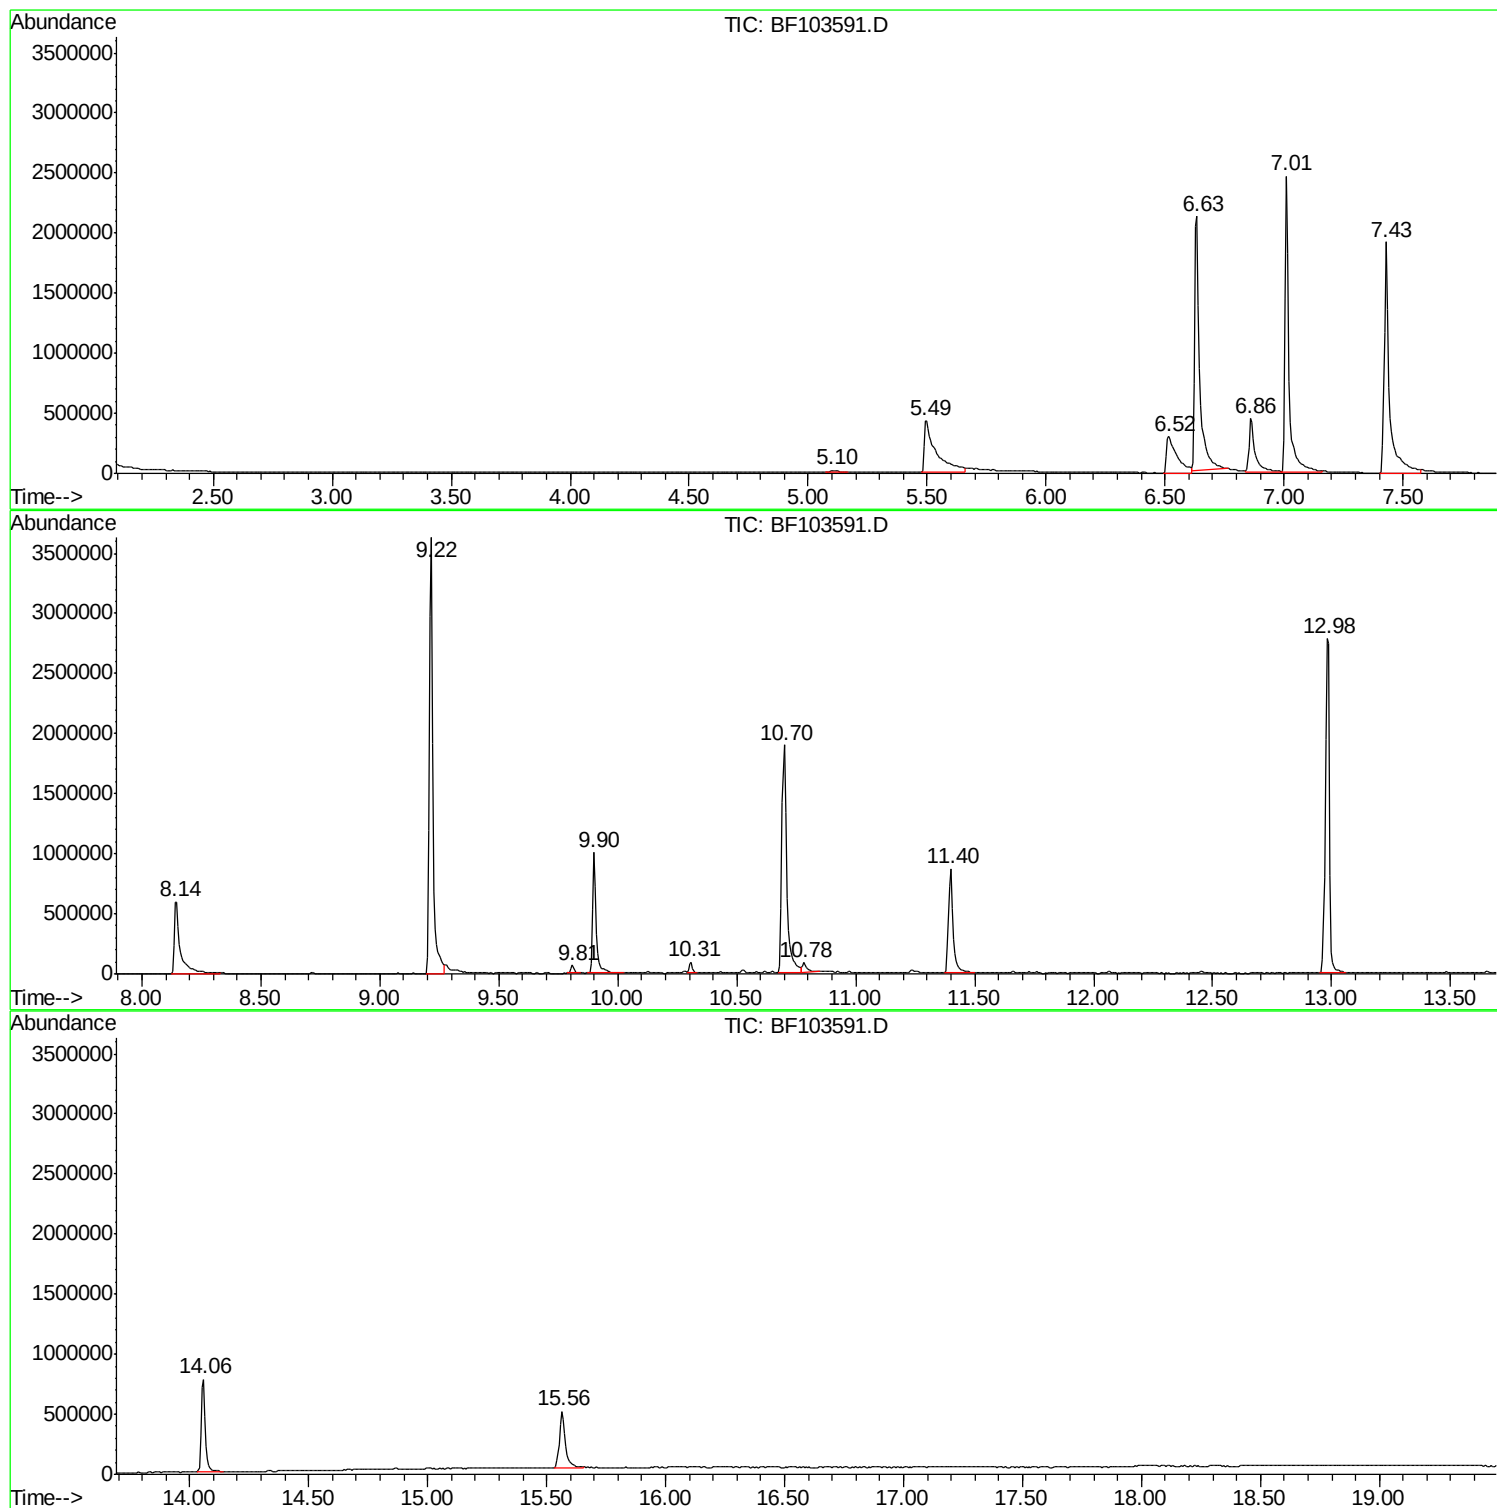

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031218\
Data File : BF103591.D
Acq On : 12 Mar 2018 19:29
Operator : SJ/JU
Sample : J1867-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CPS043071










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.63 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.63	87.88 ng	3298550	1,4-Dichlorobenzene-d4	6.86

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9

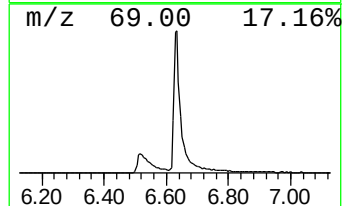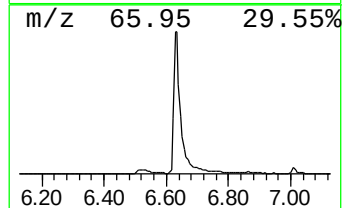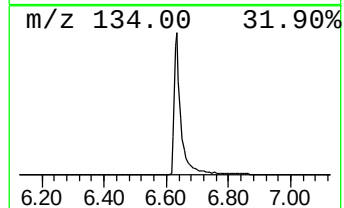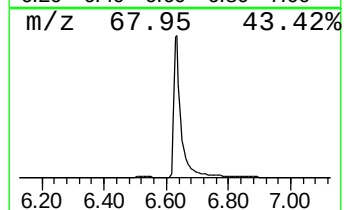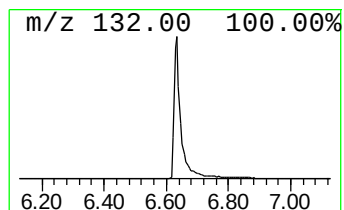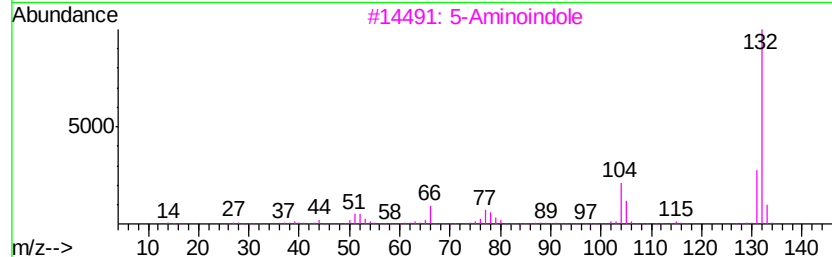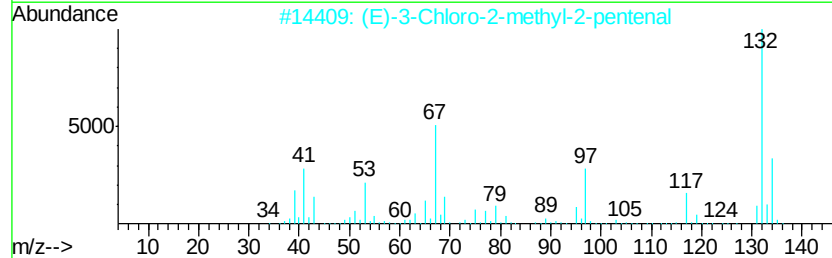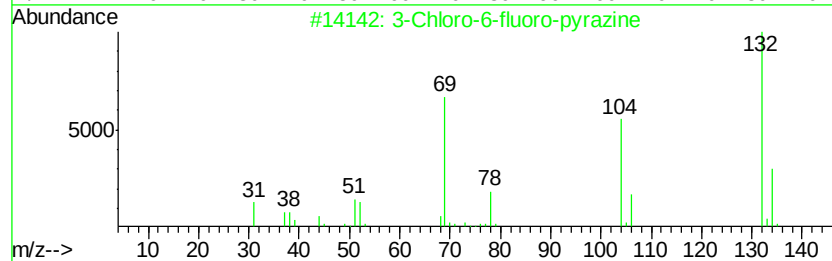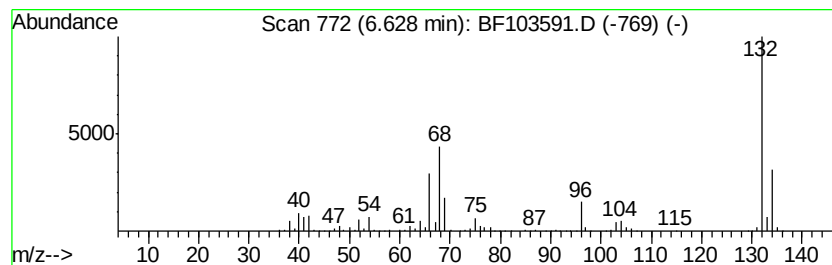

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031218\
Data File : BF103591.D
Acq On : 12 Mar 2018 19:29
Operator : SJ/JU
Sample : J1867-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CPS043071










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Tridecane, 1-iodo- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.78	2.03 ng	111213	Phenanthrene-d10	11.40

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Tridecane, 1-iodo-	310	C13H27I	035599-77-0	86
2		Dodecane, 1-iodo-	296	C12H25I	004292-19-7	86
3		Tetratetracontane	619	C44H90	007098-22-8	86
4		Octacosane	394	C28H58	000630-02-4	86
5		Pentadecane	212	C15H32	000629-62-9	86

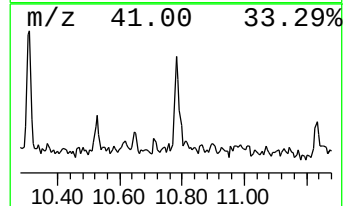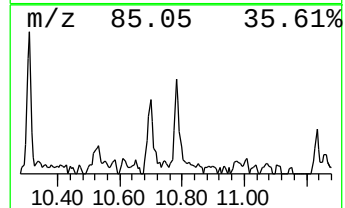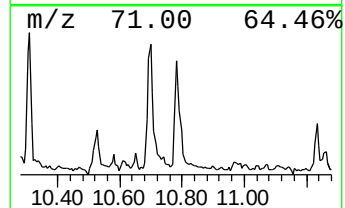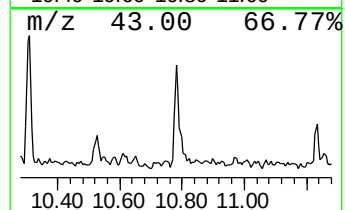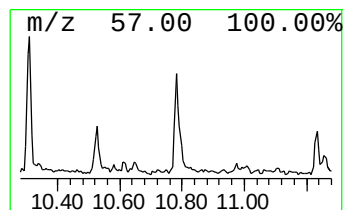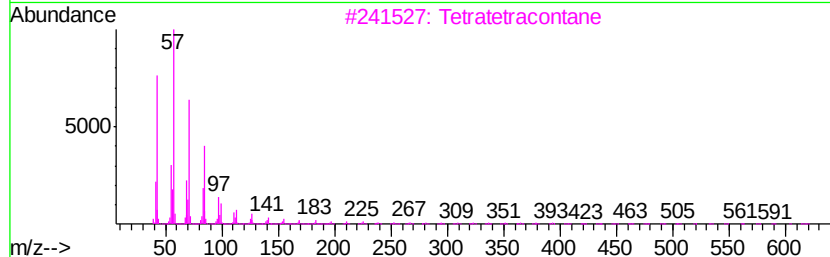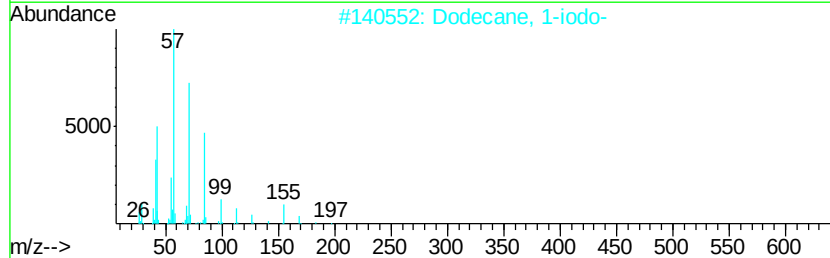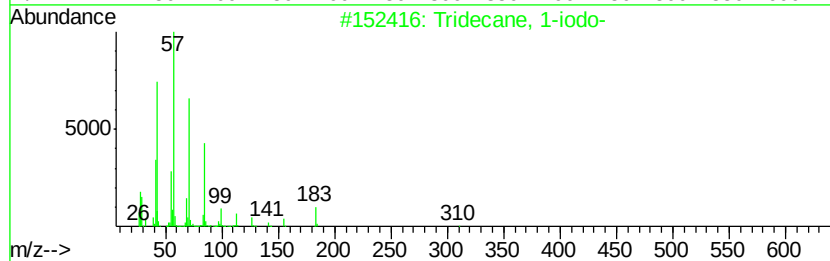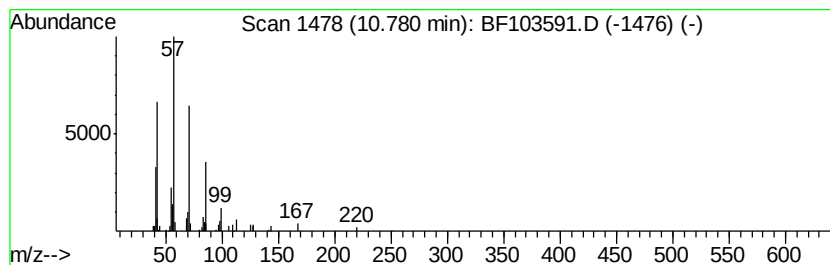

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031218\
Data File : BF103591.D
Acq On : 12 Mar 2018 19:29
Operator : SJ/JU
Sample : J1867-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CPS043071

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.63	6.63	87.9	ng	3298550	1	6.86	750681	20.0
Tridecane, 1-iodo-	10.78	2.0	ng	111213	4	11.40	1097000	20.0