


Data Path : Z:\HPCHEM1\BNA F\Data\BF031218\
 Data File : BF103570.D
 Acq On : 12 Mar 2018 9:53
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 09 11:47:13 2018

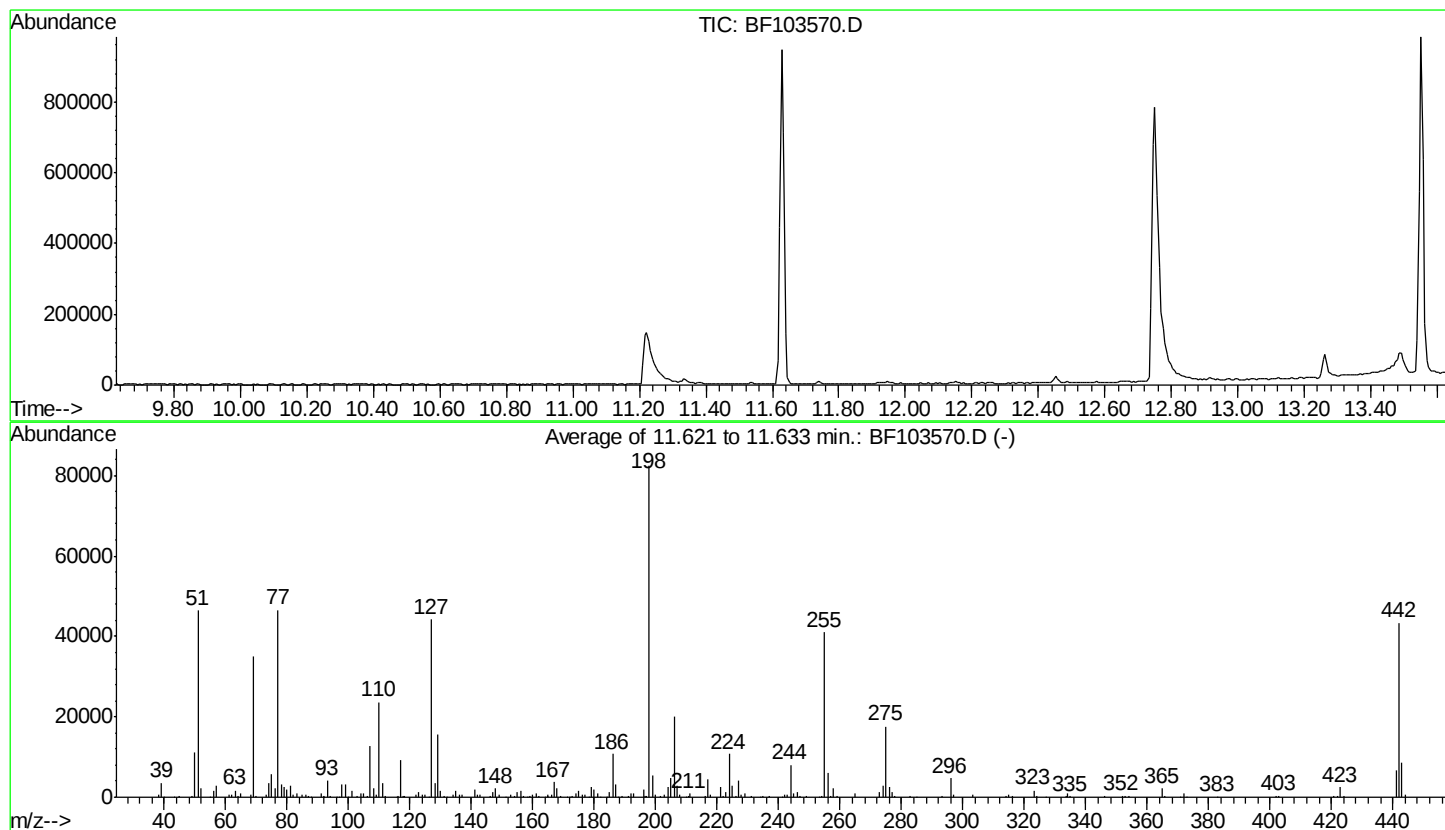

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.3	46453	PASS
68	69	0.00	2	1.7	584	PASS
69	198	0.00	100	42.4	34938	PASS
70	69	0.00	2	1.0	346	PASS
127	198	10	80	53.6	44218	PASS
197	198	0.00	2	0.4	353	PASS
198	198	100	100	100.0	82485	PASS
199	198	5	9	6.6	5472	PASS
275	198	10	60	21.3	17584	PASS
365	198	1	100	2.5	2092	PASS
441	443	0.01	100	77.7	6673	PASS
442	198	50	100	52.6	43364	PASS
443	442	15	24	19.8	8585	PASS