


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF031219\  
 Data File : BF112998.D  
 Acq On : 12 Mar 2019 12:30  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF022719.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Mar 13 03:42:55 2019

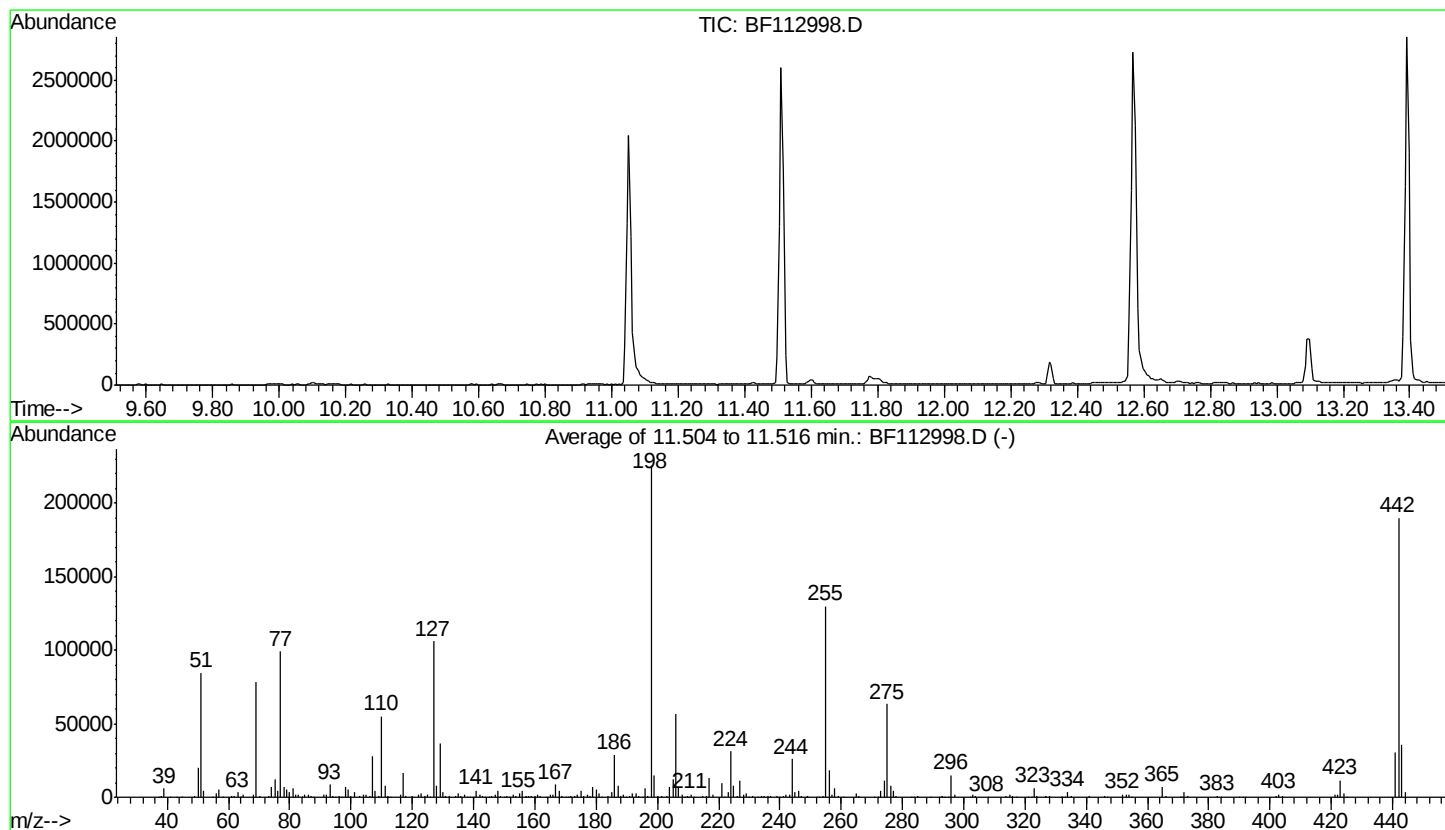

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 37.5      | 84658   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 1339    | PASS             |
| 69          | 198          | 0.00         | 100          | 34.9      | 78720   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 508     | PASS             |
| 127         | 198          | 10           | 80           | 47.0      | 105970  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 1037    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 225664  | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 14861   | PASS             |
| 275         | 198          | 10           | 60           | 28.1      | 63445   | PASS             |
| 365         | 198          | 1            | 100          | 3.1       | 7090    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.5      | 30377   | PASS             |
| 442         | 198          | 50           | 100          | 84.3      | 190138  | PASS             |
| 443         | 442          | 15           | 24           | 18.8      | 35683   | PASS             |