
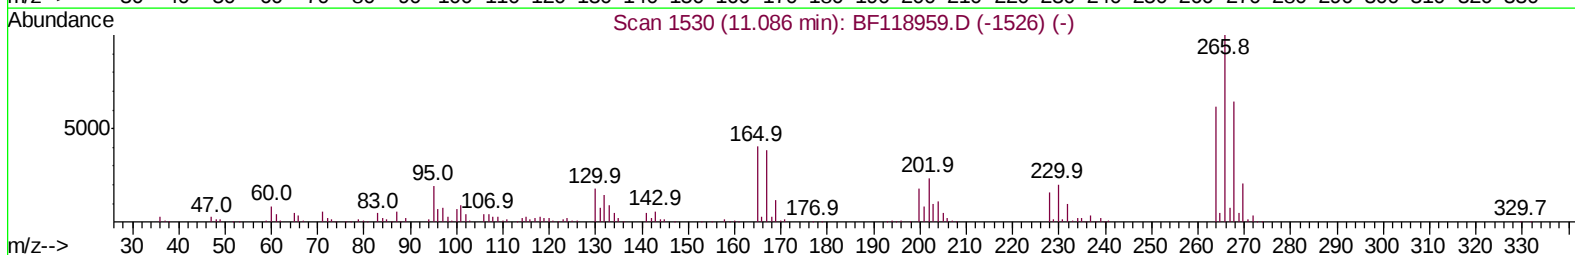
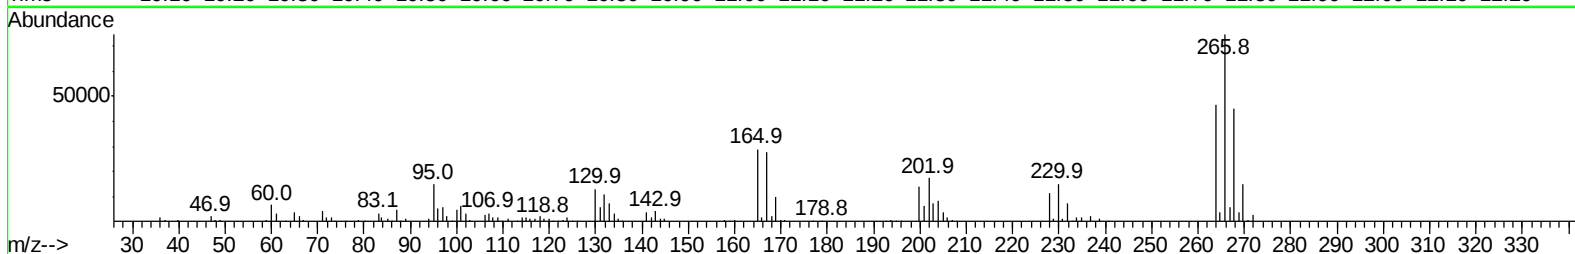


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF031220\
Data File : BF119370.D
Acq On : 12 Mar 2020 9:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 07:59:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 06 23:38:46 2020
Response via : Initial Calibration

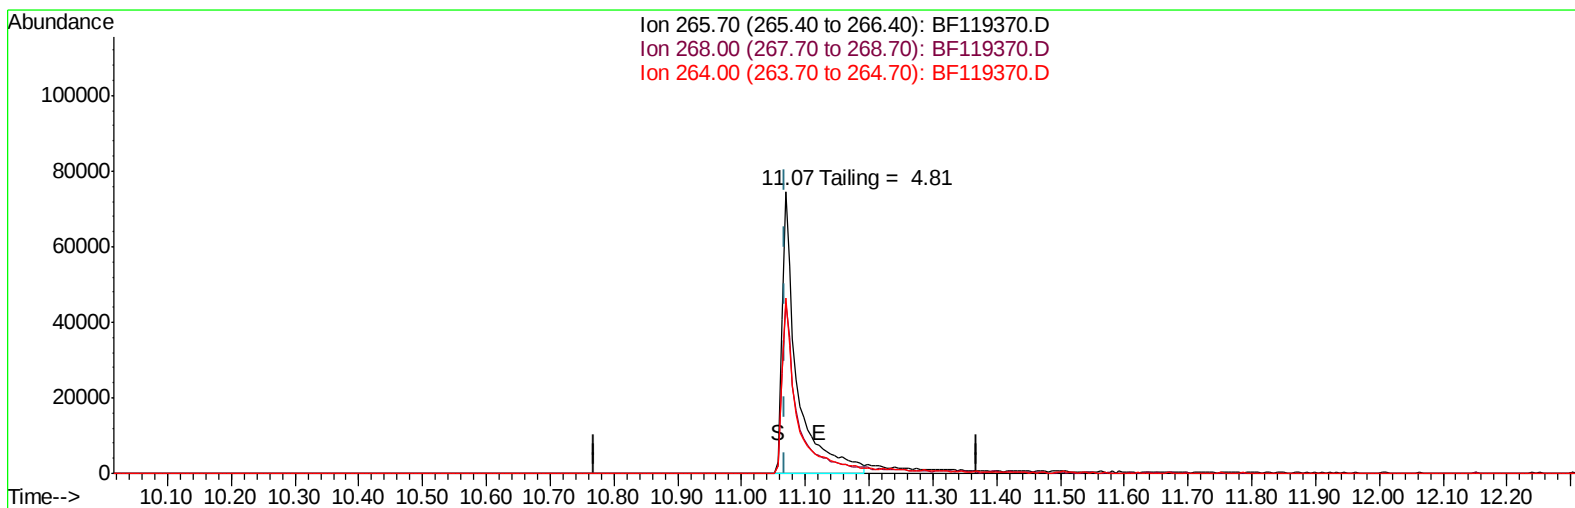

TIC: BF119370.D

(70) Pentachlorophenol (C)




11.069min (+0.000) 54829.82ng

response 134475

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	60.59
264.00	63.70	62.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF031220\
Data File : BF119370.D
Acq On : 12 Mar 2020 9:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 07:59:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 06 23:38:46 2020
Response via : Initial Calibration

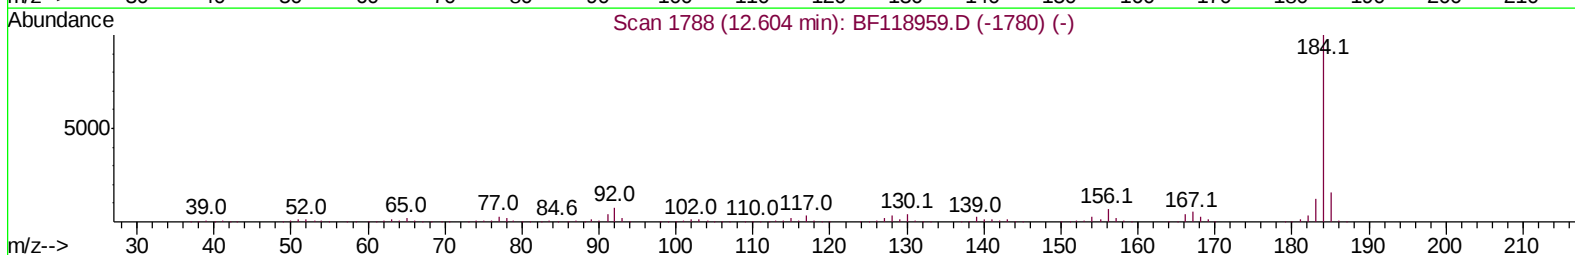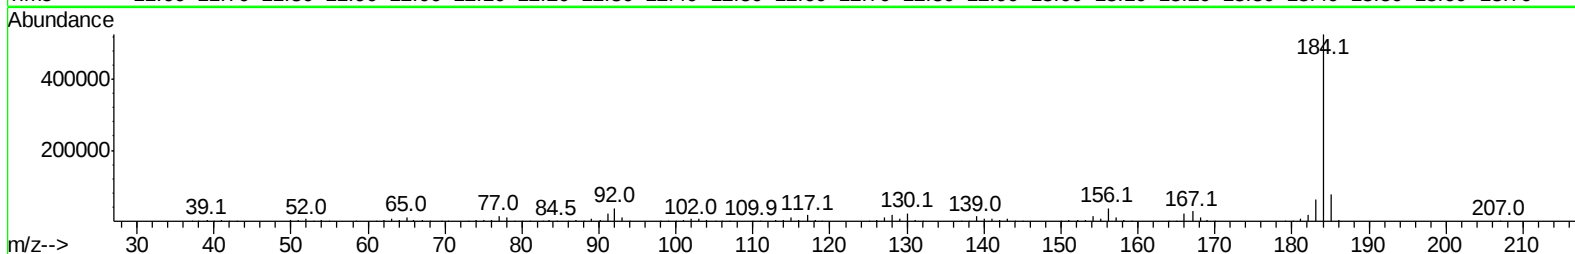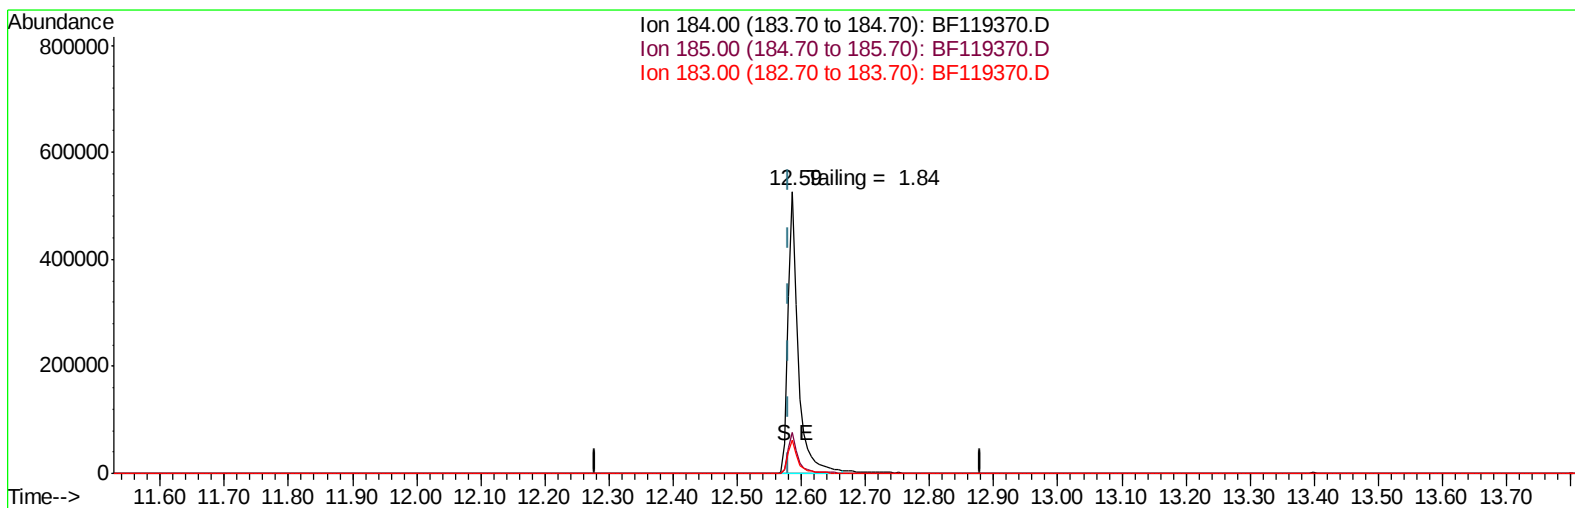

TIC: BF119370.D

(77) Benzidine

12.586min (+0.006) 114262.84ng

response 585519

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.38
183.00	12.40	12.01
0.00	0.00	0.00