
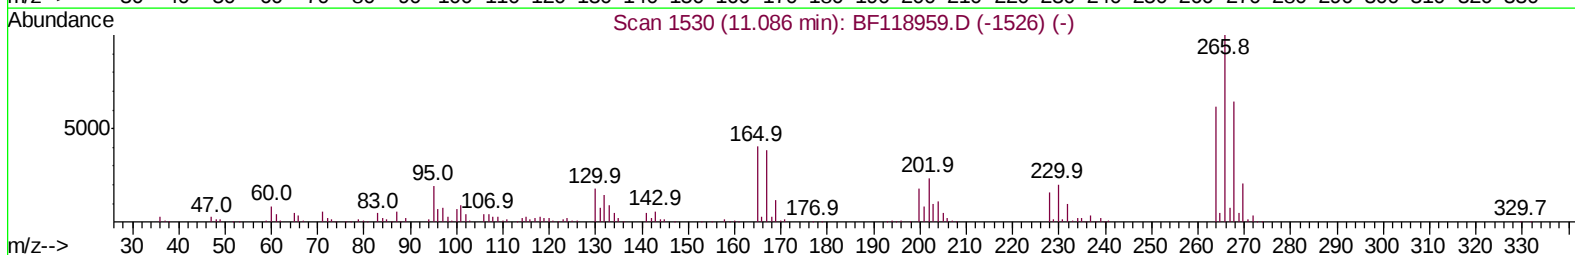
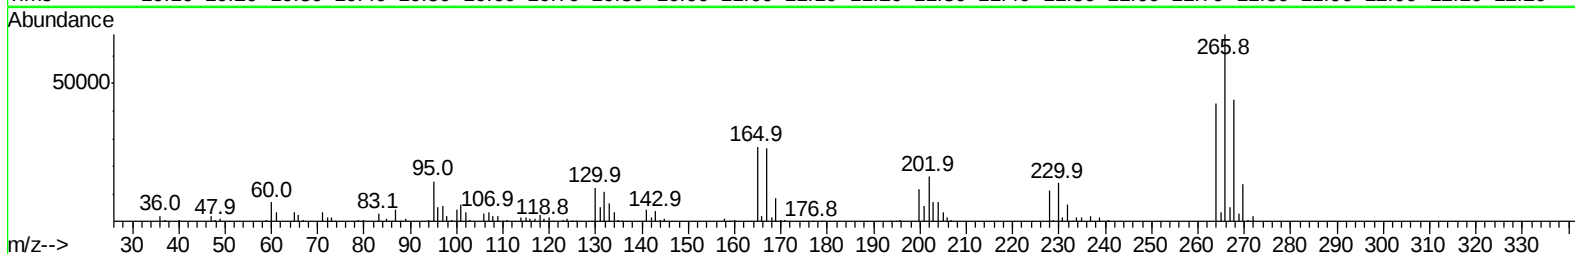


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF031220\
Data File : BF119382.D
Acq On : 12 Mar 2020 15:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 08:00:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 06 23:38:46 2020
Response via : Initial Calibration

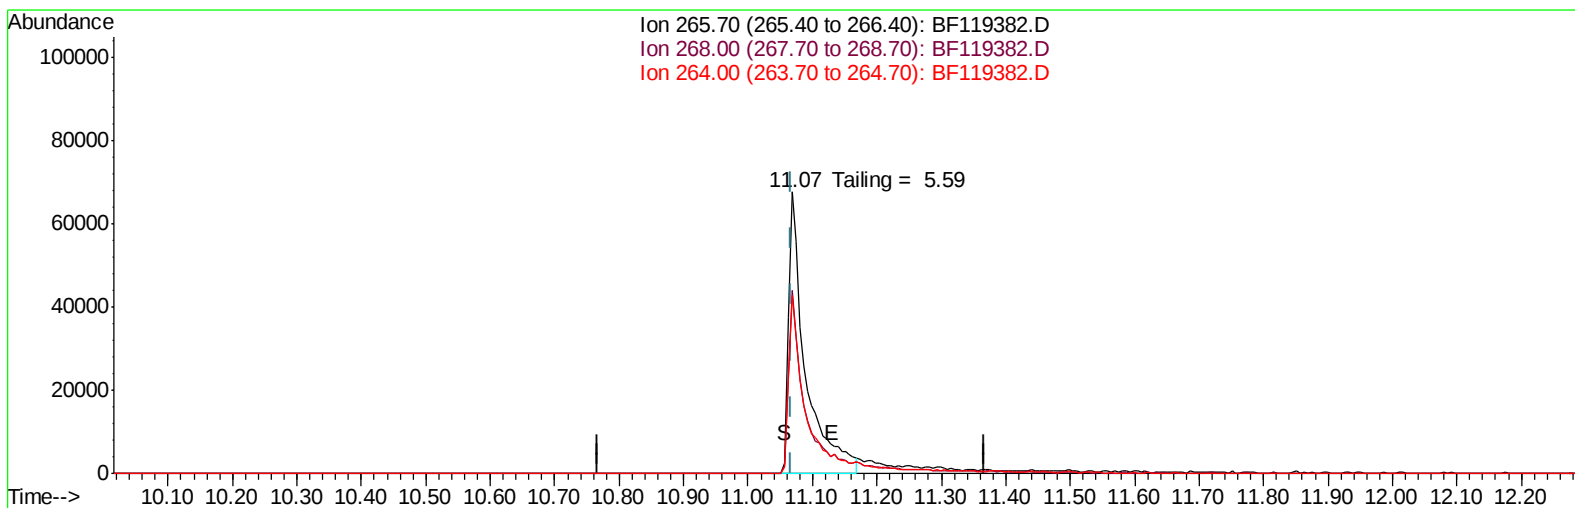

TIC: BF119382.D

(70) Pentachlorophenol (C)




11.069min (+0.000) 58034.74ng

response 136346

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	65.13
264.00	63.70	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF031220\
Data File : BF119382.D
Acq On : 12 Mar 2020 15:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 08:00:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 06 23:38:46 2020
Response via : Initial Calibration

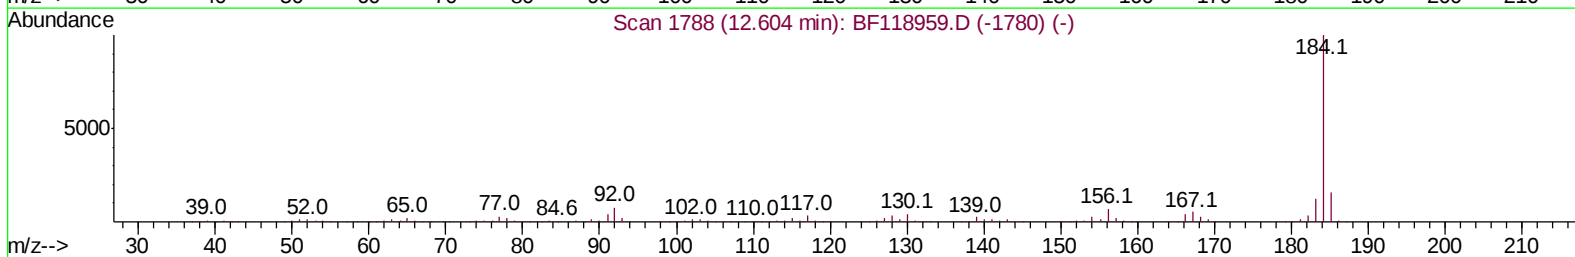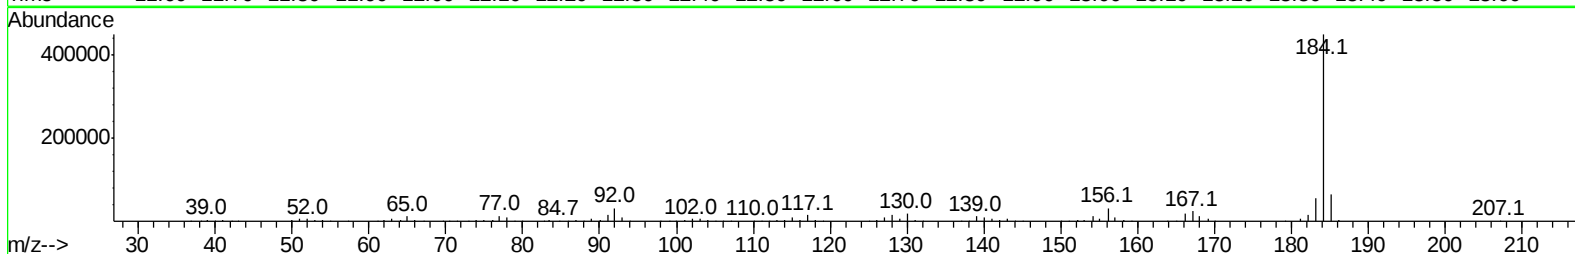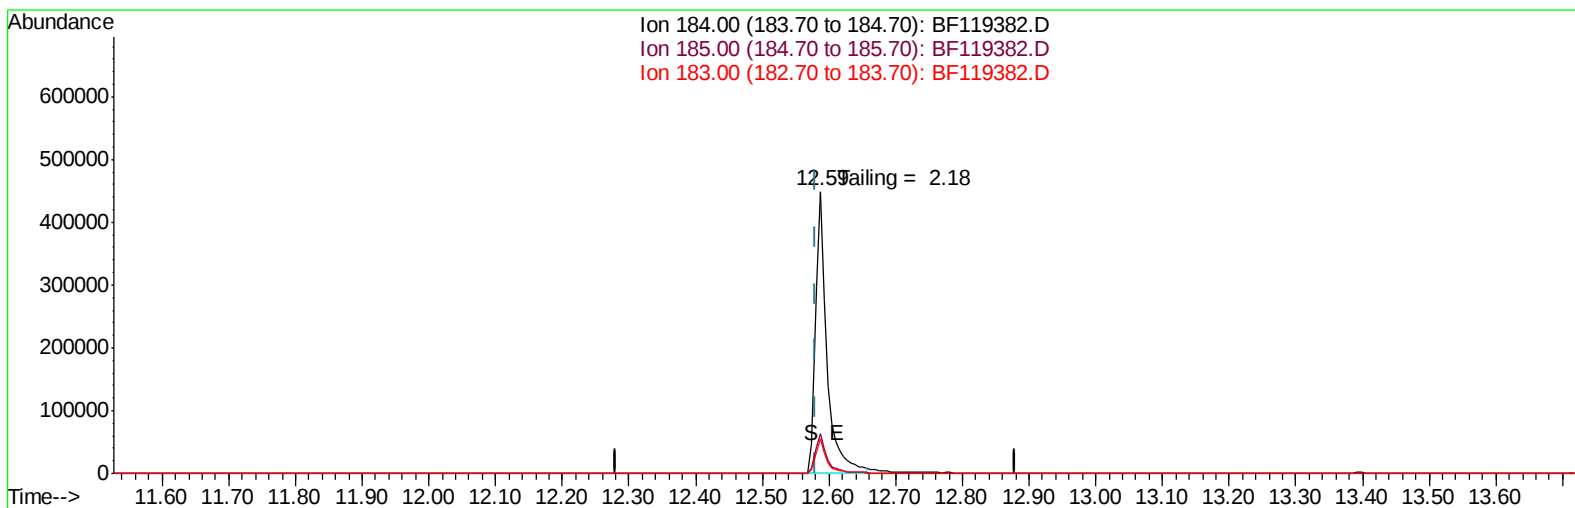

TIC: BF119382.D

(77) Benzidine




12.586min (+0.006) 0.00ng

response 538387

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.31
183.00	12.40	12.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF031220\
Data File : BF119382.D
Acq On : 12 Mar 2020 15:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 08:00:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 06 23:38:46 2020
Response via : Initial Calibration

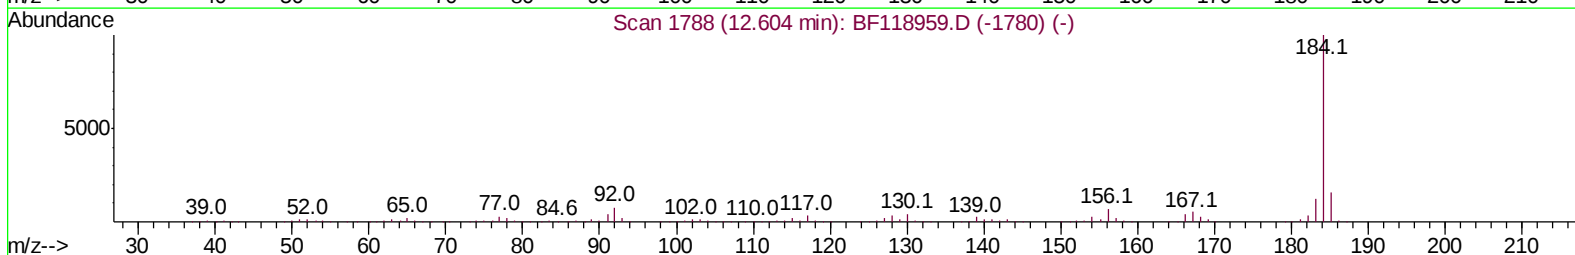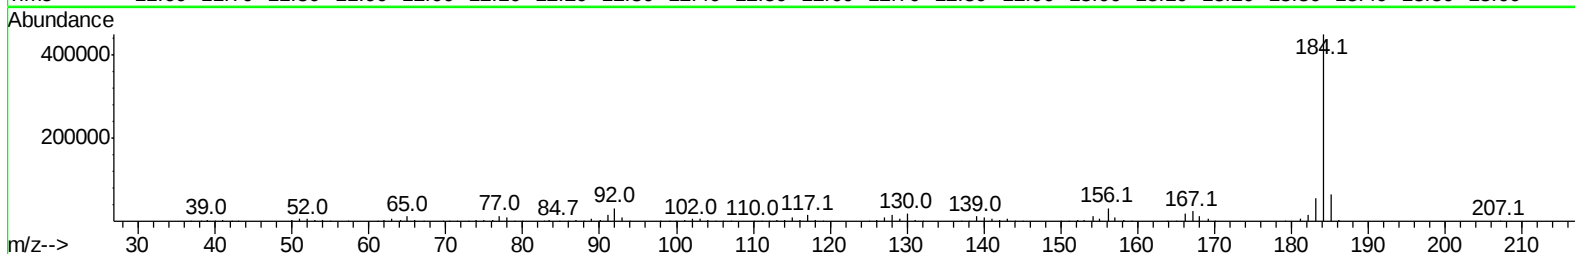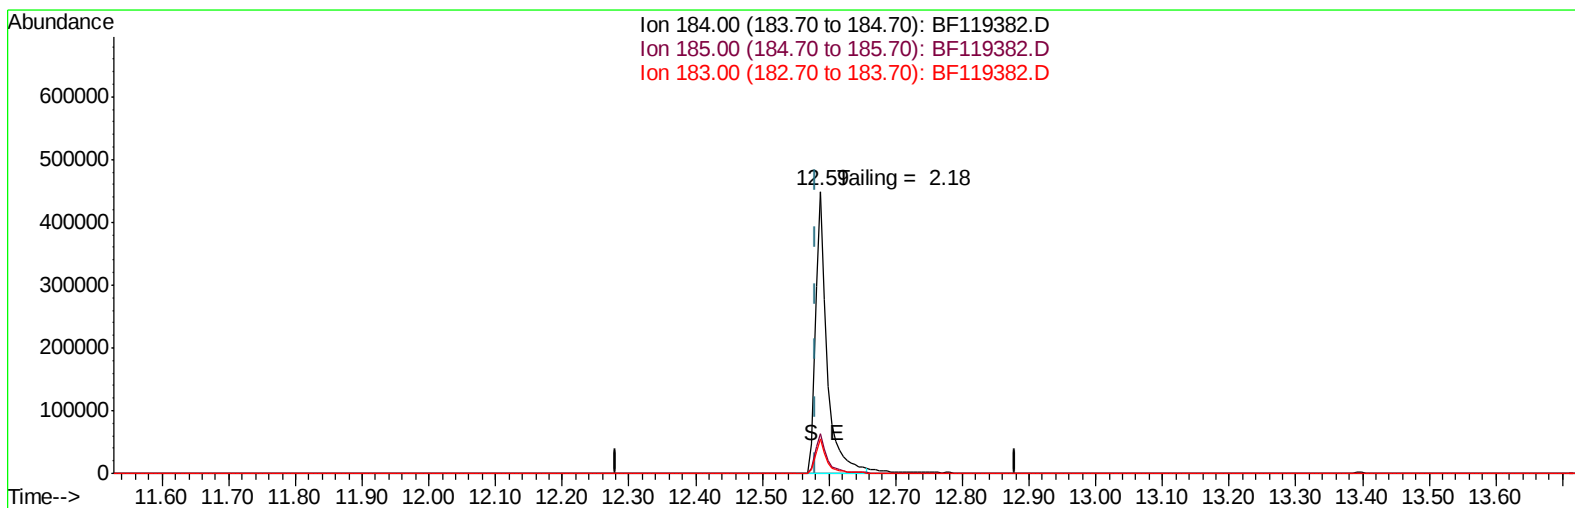

TIC: BF119382.D

(77) Benzidine

12.586min (+0.006) 0.00ng

response 538387

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.31
183.00	12.40	12.15
0.00	0.00	0.00