


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031220\
 Data File : BF119370.D
 Acq On : 12 Mar 2020 9:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 06 23:38:46 2020

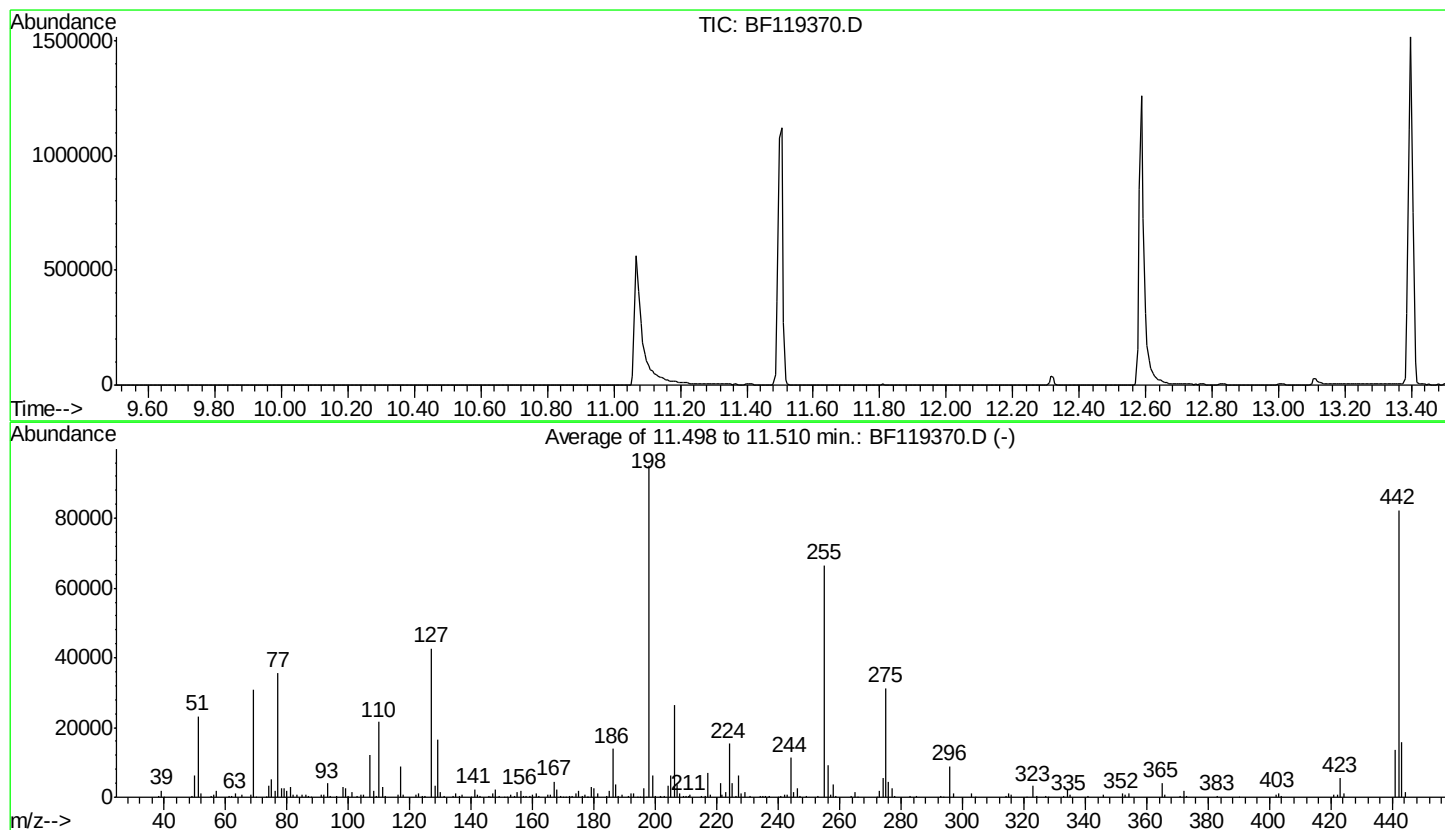

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	23217	PASS
68	69	0.00	2	2.0	608	PASS
69	198	0.00	100	32.5	30874	PASS
70	69	0.00	2	0.3	104	PASS
127	198	10	80	44.9	42687	PASS
197	198	0.00	2	0.2	166	PASS
198	198	100	100	100.0	95117	PASS
199	198	5	9	6.6	6316	PASS
275	198	10	60	32.9	31256	PASS
365	198	1	100	4.4	4199	PASS
441	198	0.01	100	14.4	13698	PASS
442	198	50	100	86.5	82306	PASS
443	442	15	24	19.3	15851	PASS