


Data Path : Z:\HPCHEM1\BNA_F\Data\BF031315\
 Data File : BF077735.D
 Acq On : 13 Mar 2015 11:43
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 13 14:04:45 2015

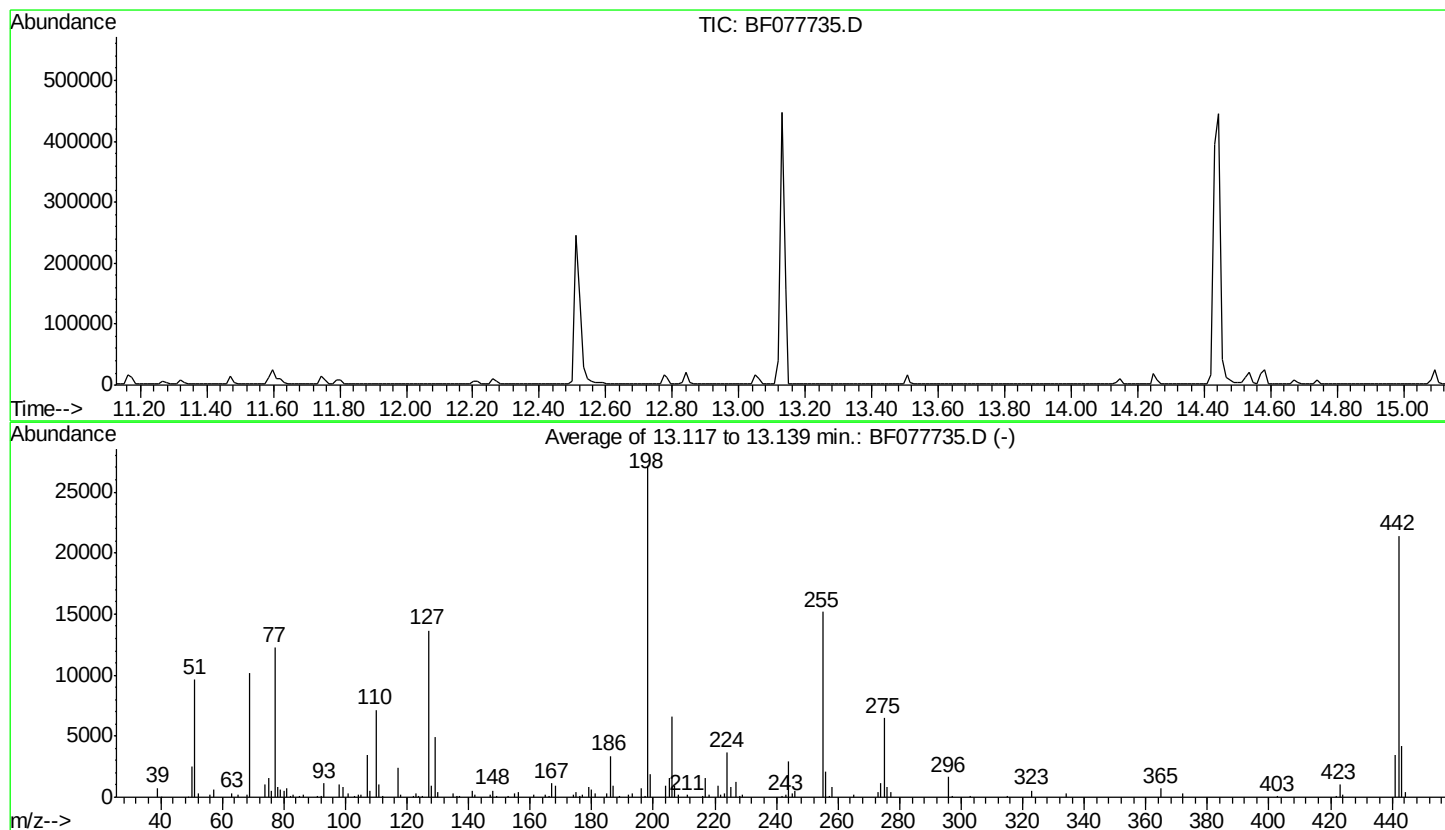

AutoFind: Scans 1070, 1071, 1072; Background Corrected with Scan 1067

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	9616	PASS
68	69	0.00	2	1.7	167	PASS
69	198	0.00	100	37.3	10121	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.3	13662	PASS
197	198	0.00	2	0.5	146	PASS
198	198	100	100	100.0	27150	PASS
199	198	5	9	6.8	1848	PASS
275	198	10	60	23.9	6480	PASS
365	198	1	100	2.6	712	PASS
441	442	0.01	24	16.1	3438	PASS
442	198	50	100	78.9	21415	PASS
443	442	15	24	19.7	4217	PASS