

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031317\
 Data File : BF093626.D
 Acq On : 14 Mar 2017 00:12
 Operator : SJ/MA
 Sample : PB97546BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB97546BL

Quant Time: Mar 14 01:07:15 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 13 15:05:08 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.71	152	176698	20.00	ng	-0.01
21) Naphthalene-d8	8.00	136	712923	20.00	ng	-0.01
38) Acenaphthene-d10	9.76	164	328483	20.00	ng	0.00
63) Phenanthrene-d10	11.25	188	640542	20.00	ng	0.00
75) Chrysene-d12	13.90	240	506232	20.00	ng	0.01
86) Perylene-d12	15.31	264	350365	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	1520467	143.21	ng	0.00
7) Phenol-d6	6.37	99	1806659	134.95	ng	-0.01
23) Nitrobenzene-d5	7.28	82	1134119	88.26	ng	-0.02
41) 2,4,6-Tribromophenol	10.56	330	323917	151.35	ng	0.01
44) 2-Fluorobiphenyl	9.09	172	1838282	104.09	ng	0.00
78) Terphenyl-d14	12.84	244	1447603	74.35	ng	0.01
Target Compounds						
9) Benzaldehyde	6.37	77	2625	Below Cal	#	17
19) n-Nitroso-di-n-propylamine	7.28	70	153046	16.63	ng	# 84
25) Isophorone	7.28	82	1101617	42.52	ng	# 65
50) 2,6-Dinitrotoluene	9.76	165	43023	9.00	ng	# 32
56) 2,4-Dinitrotoluene	9.76	165	43017	7.33	ng	# 21
66) 4-Bromophenyl-phenylether	10.55	248	23225	3.43	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031317\
Data File : BF093626.D
Acq On : 14 Mar 2017 00:12
Operator : SJ/MA
Sample : PB97546BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB97546BL

Quant Time: Mar 14 01:07:15 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 13 15:05:08 2017
Response via : Initial Calibration

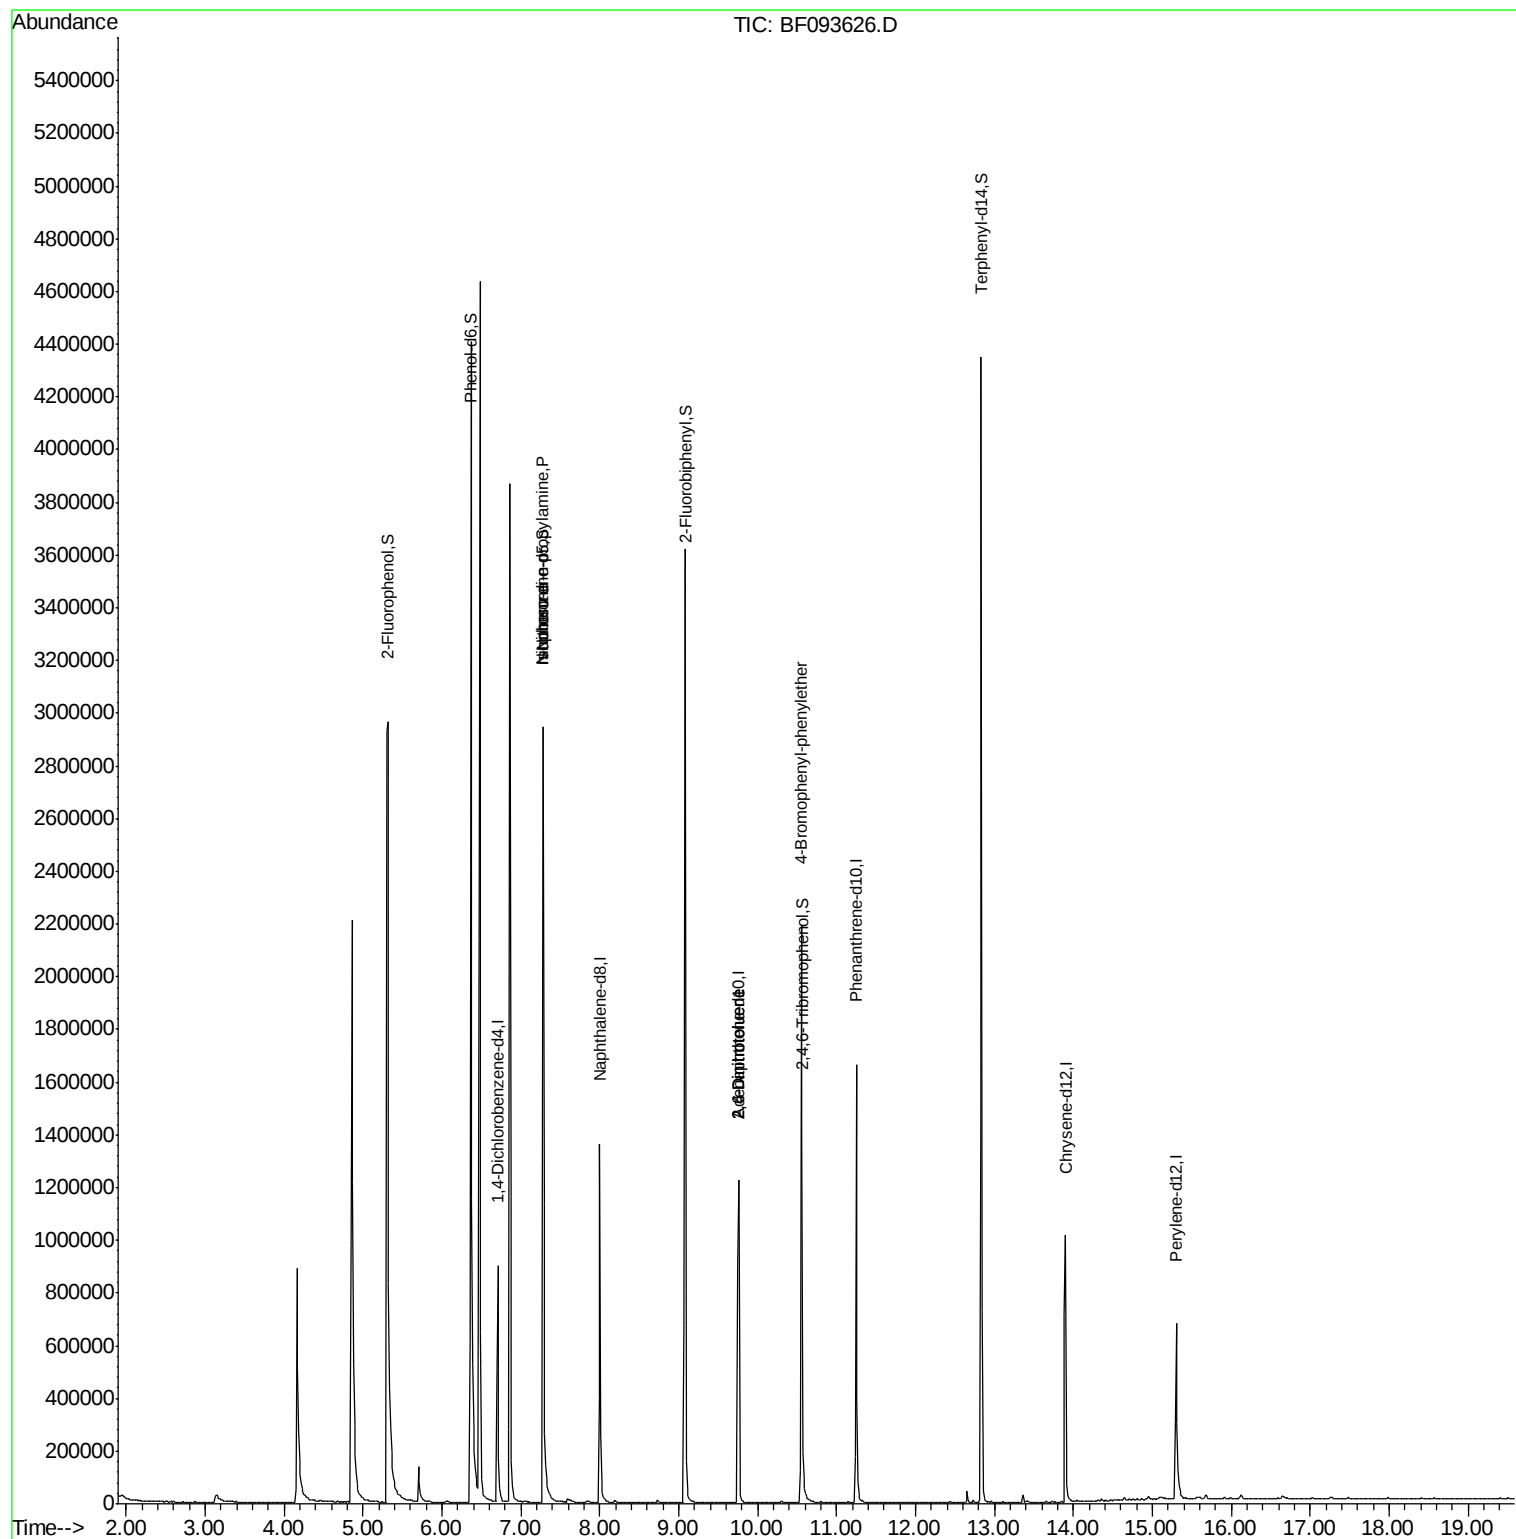

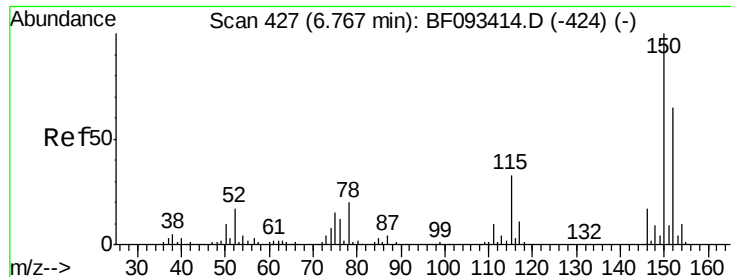


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.71 min Scan# 422
 Delta R.T. -0.01 min
 Lab File: BF093626.D
 Acq: 14 Mar 2017 00:12

Instrument :
 BNA_F
 ClientSampleId :
 PB97546BL

Tgt Ion:152 Resp: 176698
 Ion Ratio Lower Upper
 152 100
 150 154.3 124.9 187.3
 115 57.0 46.0 69.0

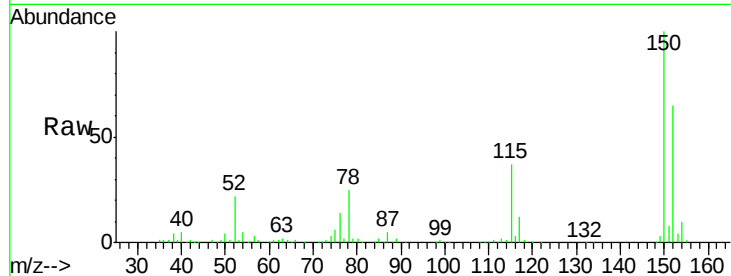


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

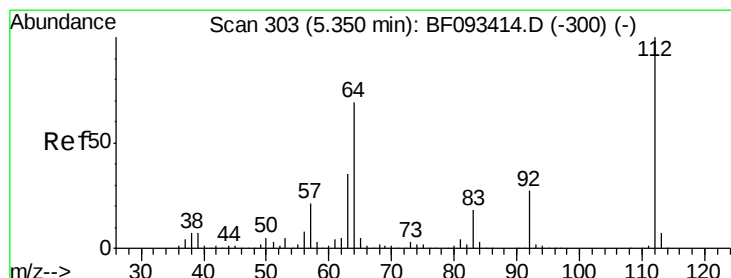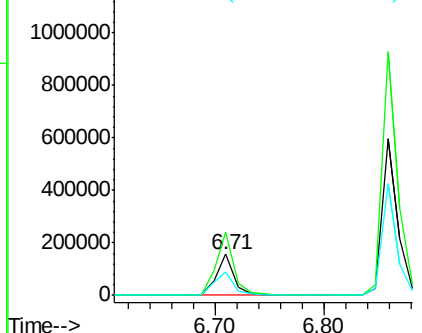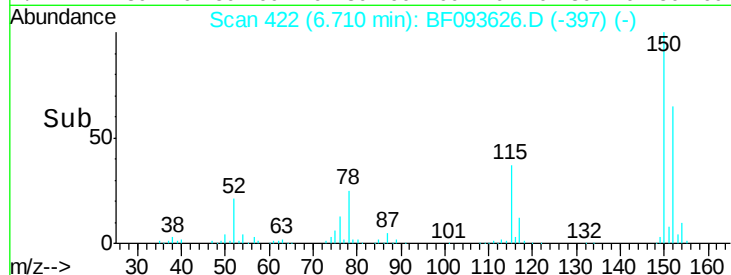



#5




2-Fluorophenol
 Concen: 143.21 ng
 RT: 5.32 min Scan# 300
 Delta R.T. -0.00 min
 Lab File: BF093626.D
 Acq: 14 Mar 2017 00:12

Tgt Ion:112 Resp: 1520467
 Ion Ratio Lower Upper
 112 100
 64 57.5 46.1 69.1
 63 30.0 23.8 35.6

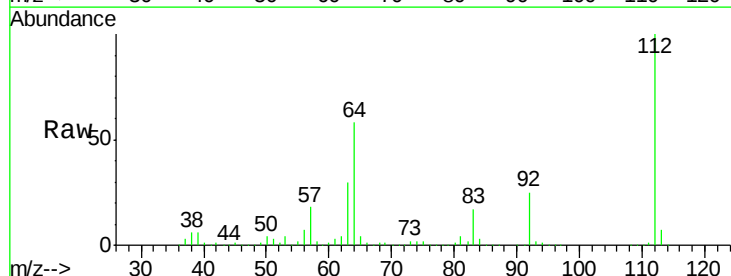

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

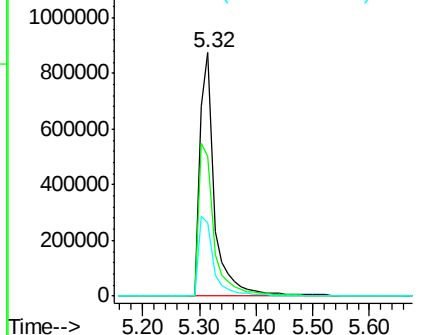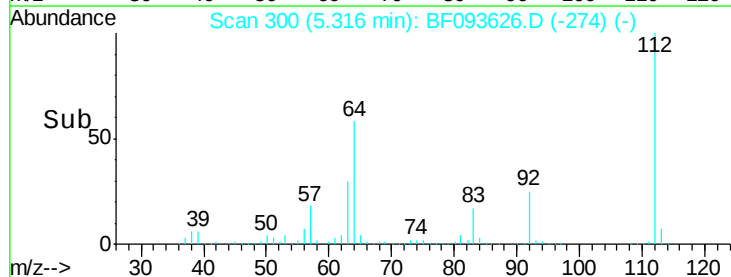

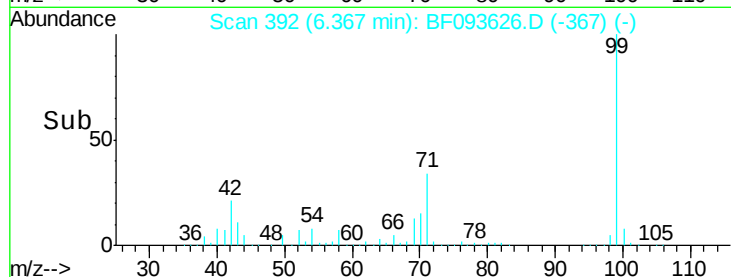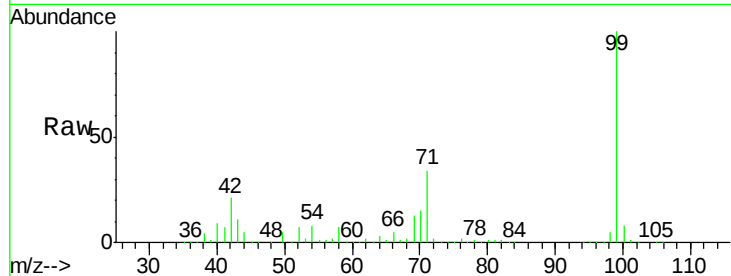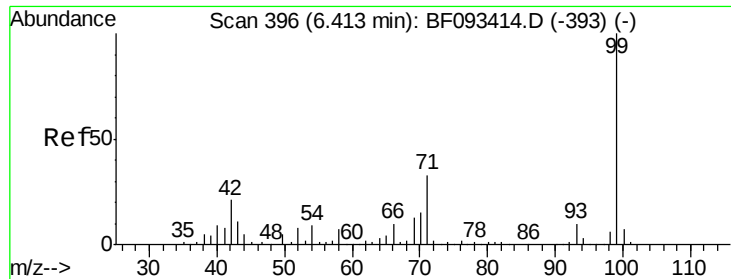

#7

Phenol-d6

Concen: 134.95 ng

RT: 6.37 min Scan# 392

Delta R.T. -0.01 min

Lab File: BF093626.D

Acq: 14 Mar 2017 00:12

Instrument :

BNA_F

ClientSampleId :

PB97546BL





Tgt Ion: 99 Resp: 1806659

Ion Ratio Lower Upper

99 100

42 21.4 15.6 23.4

71 34.4 27.5 41.3

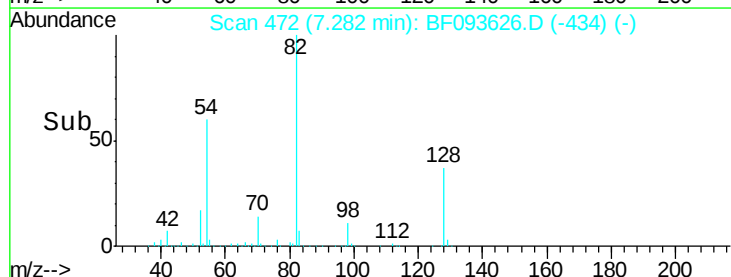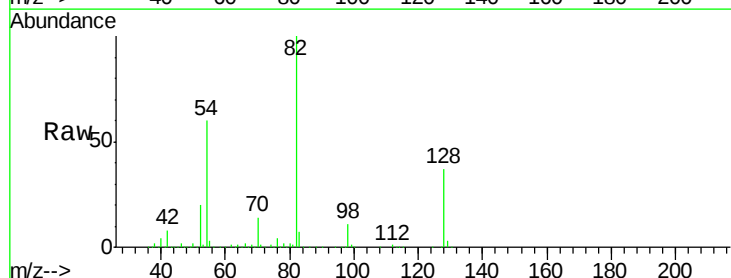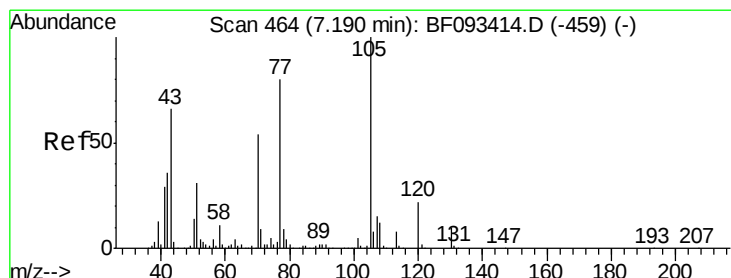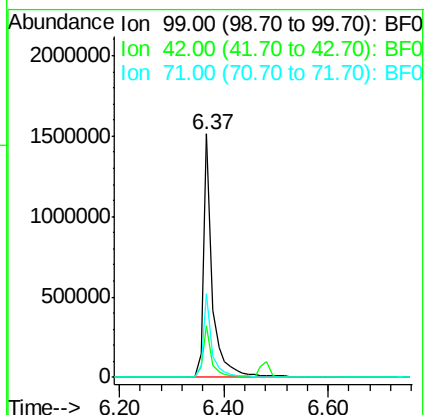

#19

n-Nitroso-di-n-propylamine

Concen: 16.63 ng

RT: 7.28 min Scan# 472

Delta R.T. 0.14 min

Lab File: BF093626.D

Acq: 14 Mar 2017 00:12

Tgt Ion: 70 Resp: 153046


Ion Ratio Lower Upper


70 100

42 55.1 49.4 74.0

101 0.0 7.4 11.2#

130 1.8 14.2 21.4#




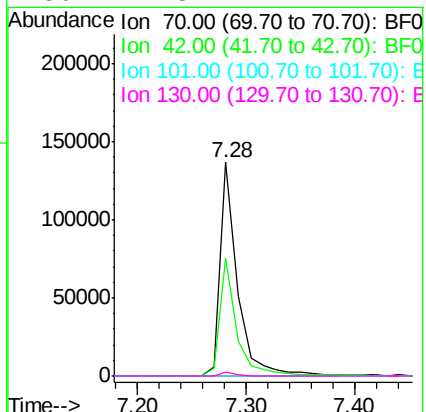


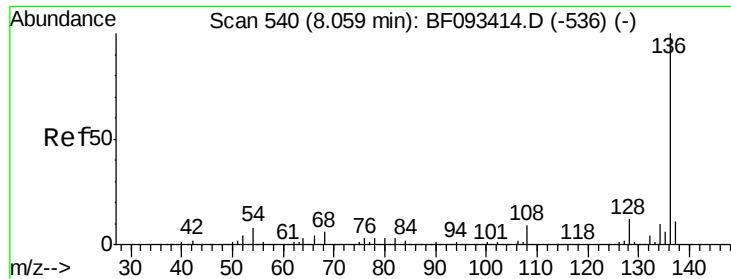

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.00 min Scan# 535
Delta R.T. -0.01 min
Lab File: BF093626.D
Acq: 14 Mar 2017 00:12




Instrument :
BNA_F
ClientSampleId :
PB97546BL


Tgt Ion:	136	Resp:	712923
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.4	12.6
54	9.2	4.5	6.7#
68	6.8	3.6	5.4#

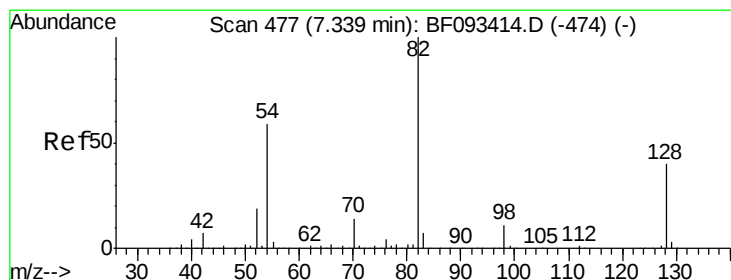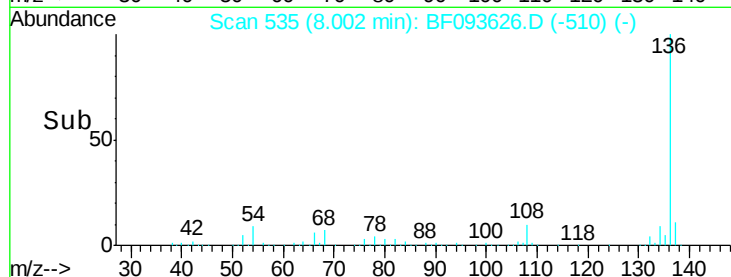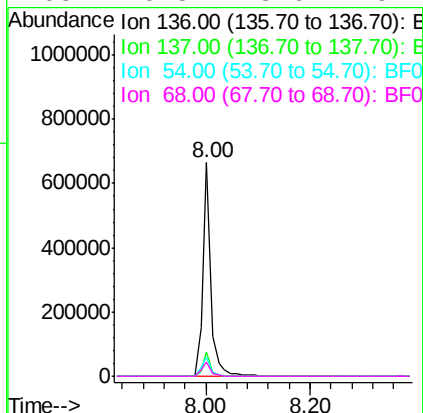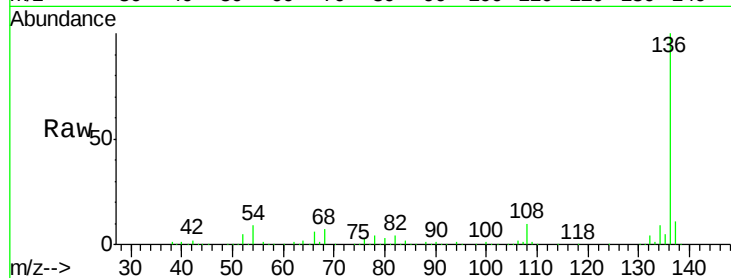

#23
Nitrobenzene-d5
Concen: 88.26 ng
RT: 7.28 min Scan# 472
Delta R.T. -0.02 min
Lab File: BF093626.D
Acq: 14 Mar 2017 00:12

Tgt Ion:	82	Resp:	1134119
Ion	Ratio	Lower	Upper
82	100		
128	37.2	34.6	52.0
54	60.3	39.5	59.3#


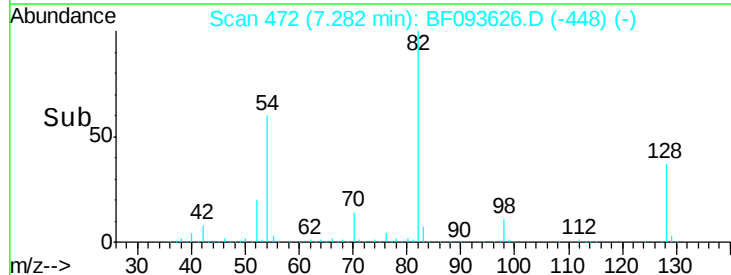
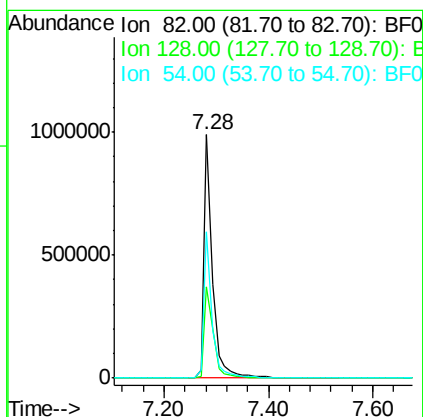
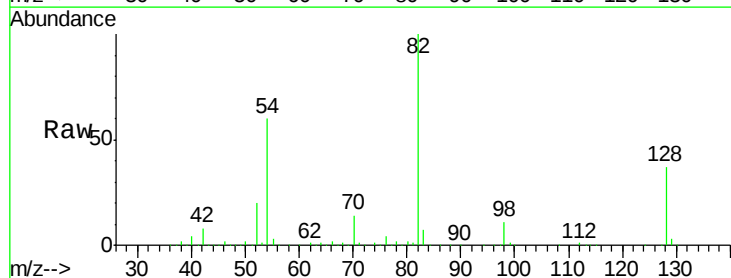


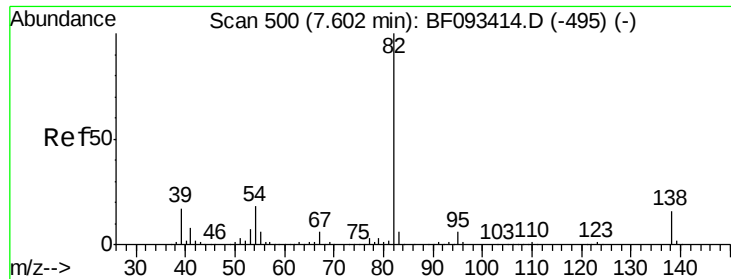

#25
Isophorone
Concen: 42.52 ng
RT: 7.28 min Scan# 472
Delta R.T. -0.27 min
Lab File: BF093626.D
Acq: 14 Mar 2017 00:12




Instrument :
BNA_F
ClientSampleId :
PB97546BL


Tgt Ion: 82 Resp: 1101617
Ion Ratio Lower Upper
82 100
95 0.0 5.6 8.4#
138 0.0 14.6 22.0#

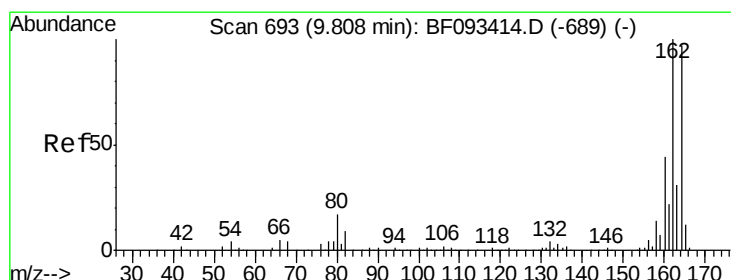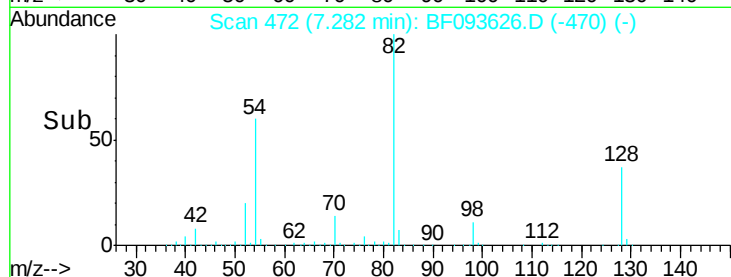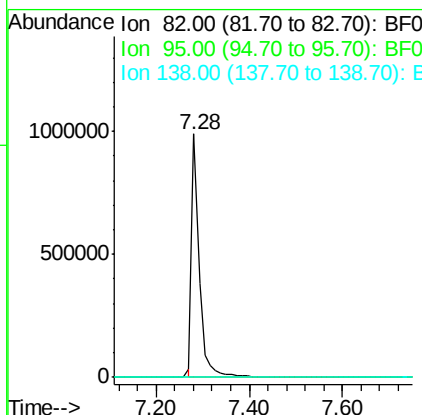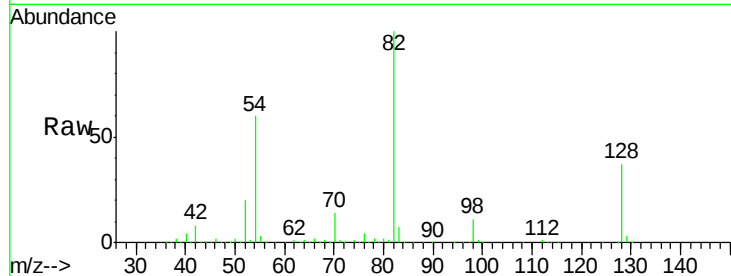

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.76 min Scan# 689
Delta R.T. -0.00 min
Lab File: BF093626.D
Acq: 14 Mar 2017 00:12

Tgt Ion: 164 Resp: 328483
Ion Ratio Lower Upper
164 100
162 105.9 80.2 120.2
160 46.4 36.9 55.3

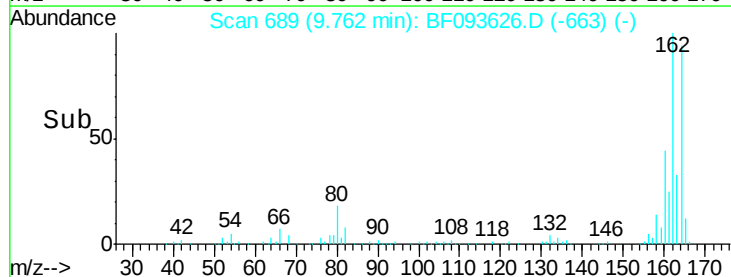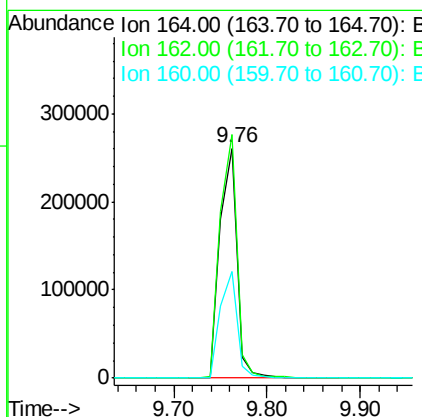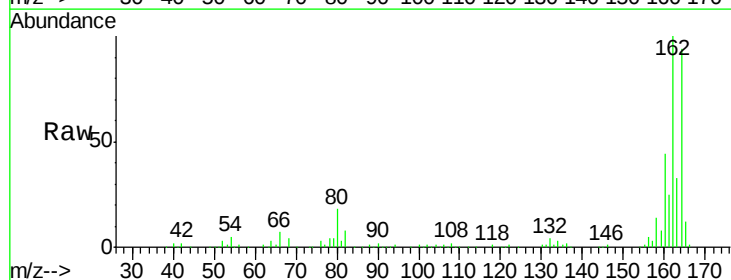


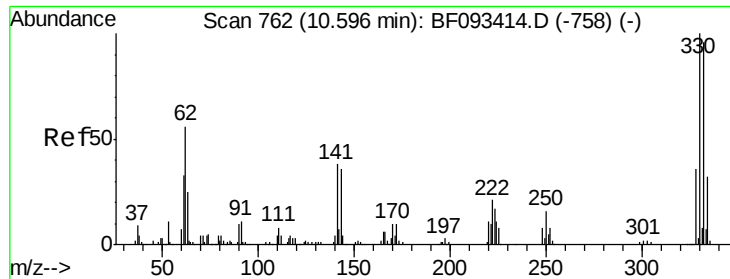




#41
 2,4,6-Tribromophenol
 Concen: 151.35 ng
 RT: 10.56 min Scan# 759
 Delta R.T. 0.01 min
 Lab File: BF093626.D
 Acq: 14 Mar 2017 00:12

Instrument :
 BNA_F
 ClientSampleId :
 PB97546BL

Tgt Ion:330 Resp: 323917
 Ion Ratio Lower Upper
 330 100
 332 97.3 77.4 116.2
 141 39.3 34.1 51.1

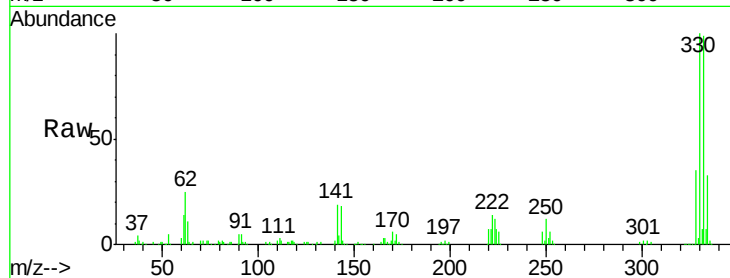


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

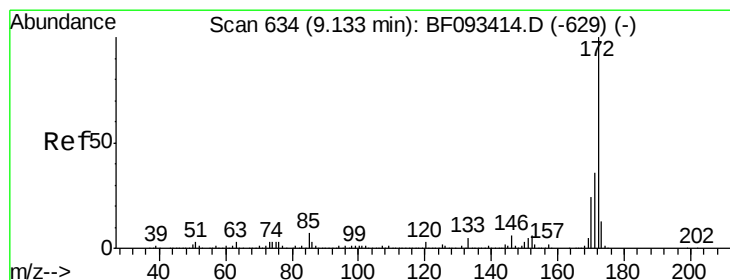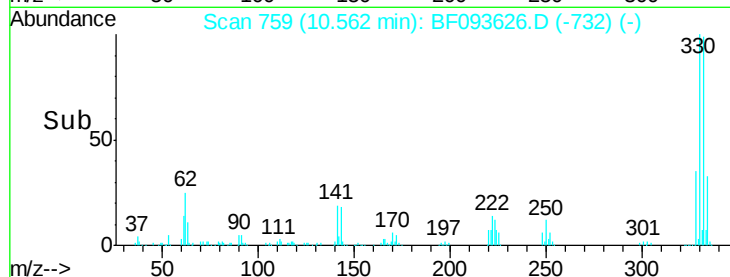
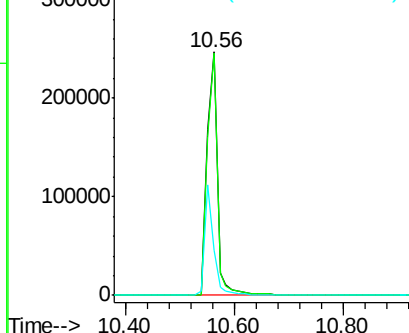



#44
 2-Fluorobiphenyl
 Concen: 104.09 ng
 RT: 9.09 min Scan# 630
 Delta R.T. -0.00 min
 Lab File: BF093626.D
 Acq: 14 Mar 2017 00:12

Tgt Ion:172 Resp: 1838282
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.4 44.0
 170 24.6 20.2 30.4

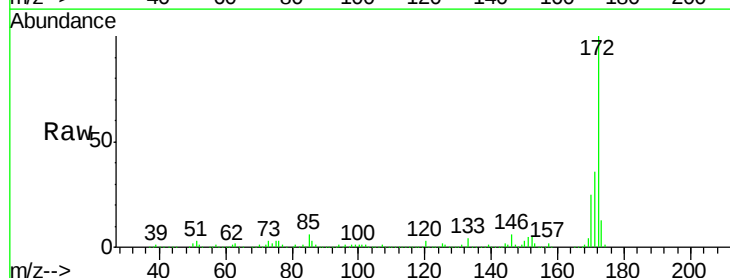

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



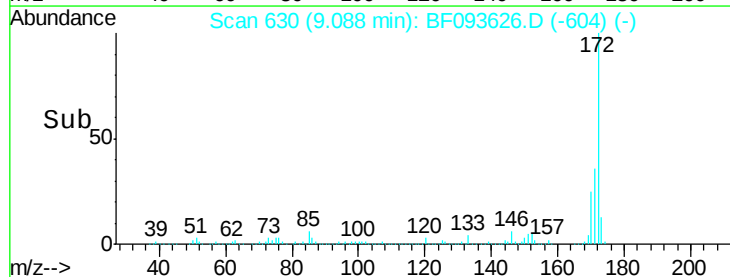
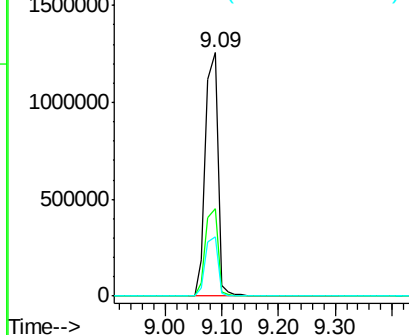


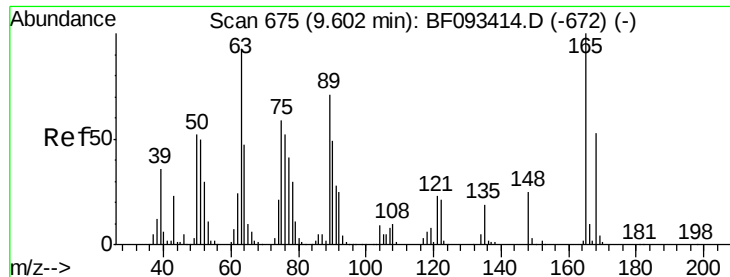

#50
 2,6-Dinitrotoluene
 Concen: 9.00 ng
 RT: 9.76 min Scan# 689
 Delta R.T. 0.19 min
 Lab File: BF093626.D
 Acq: 14 Mar 2017 00:12




Instrument :
 BNA_F
 ClientSampleId :
 PB97546BL


Tgt Ion:165 Resp: 43023
 Ion Ratio Lower Upper
 165 100
 63 2.0 36.2 54.4#
 89 2.4 40.2 60.4#

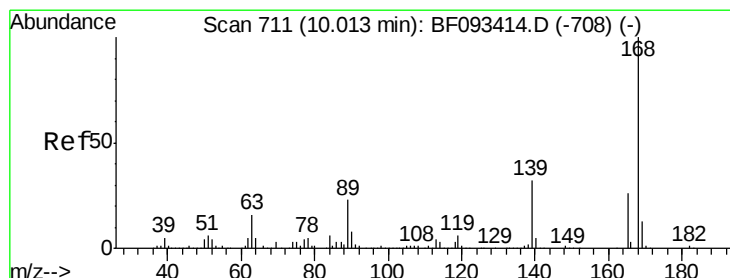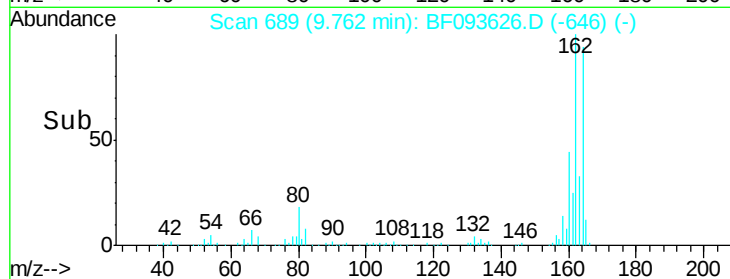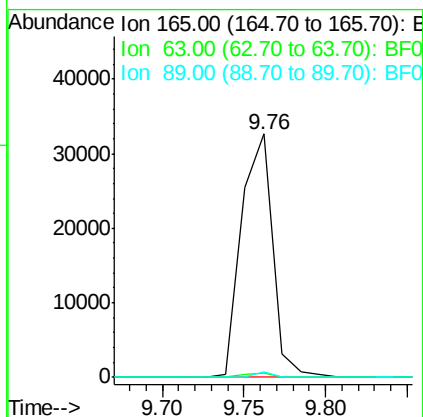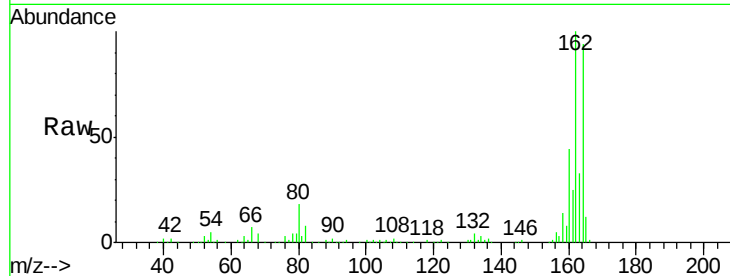

#56
 2,4-Dinitrotoluene
 Concen: 7.33 ng
 RT: 9.76 min Scan# 689
 Delta R.T. -0.22 min
 Lab File: BF093626.D
 Acq: 14 Mar 2017 00:12

Tgt Ion:165 Resp: 43017
 Ion Ratio Lower Upper
 165 100
 63 2.0 40.2 60.4#
 89 2.4 62.5 93.7#
 182 0.0 1.8 2.8#

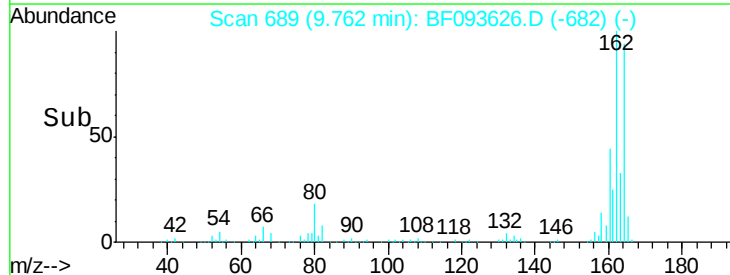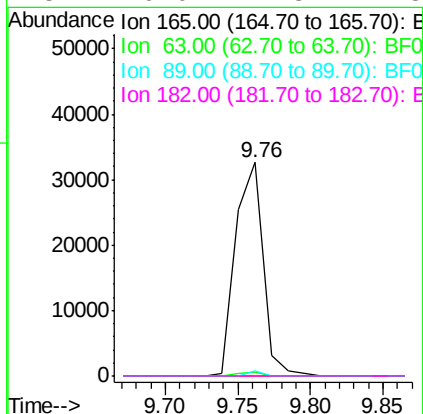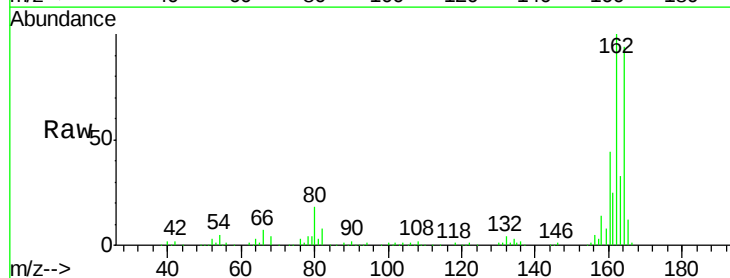


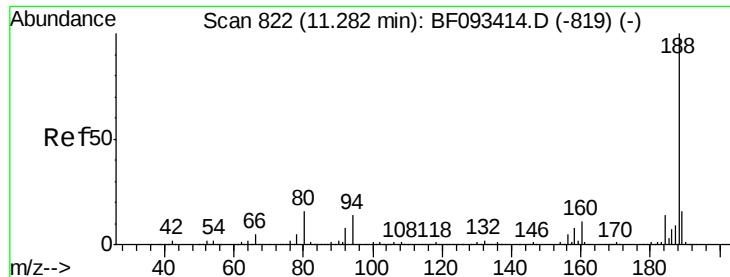




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.25 min Scan# 819
Delta R.T. -0.00 min
Lab File: BF093626.D
Acq: 14 Mar 2017 00:12

Instrument :
BNA_F
ClientSampled :
PB97546BL

Tgt Ion:188 Resp: 640542
Ion Ratio Lower Upper
188 100
94 11.5 10.0 15.0
80 12.1 11.2 16.8

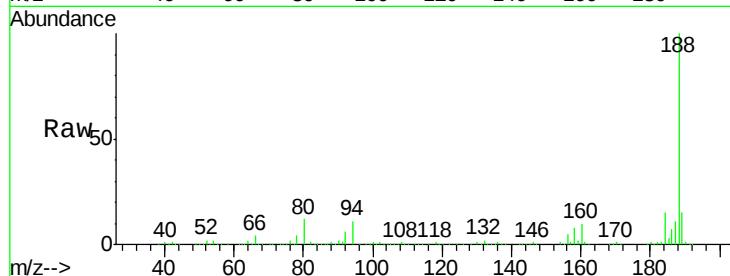


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

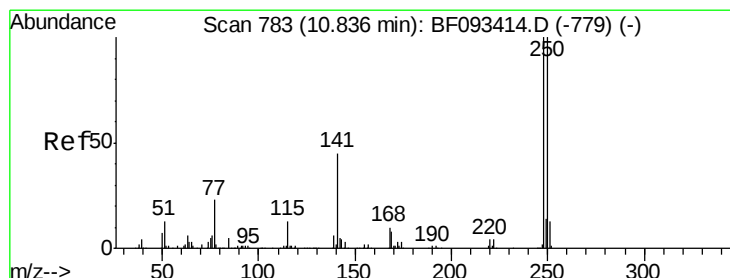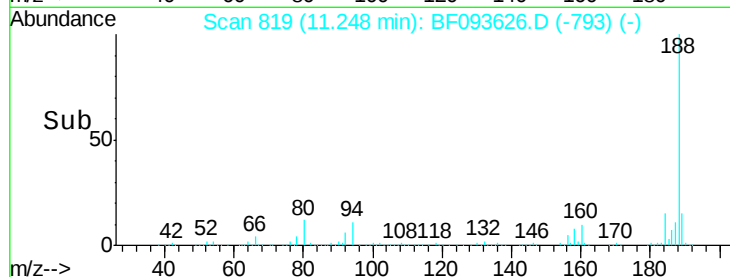
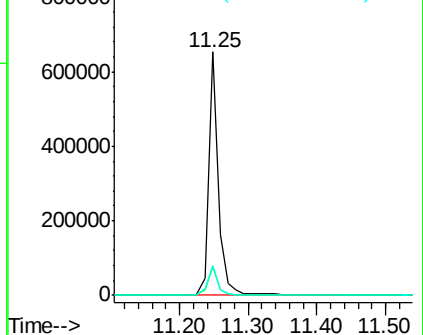



#66
4-Bromophenyl-phenylether
Concen: 3.43 ng
RT: 10.55 min Scan# 758
Delta R.T. -0.24 min
Lab File: BF093626.D
Acq: 14 Mar 2017 00:12

Tgt Ion:248 Resp: 23225
Ion Ratio Lower Upper
248 100
250 203.0 76.9 115.3#
141 667.3 68.2 102.4#

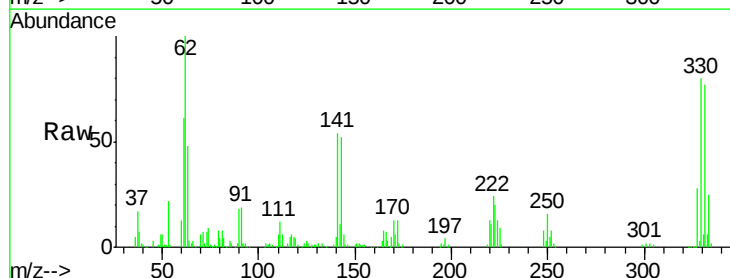

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

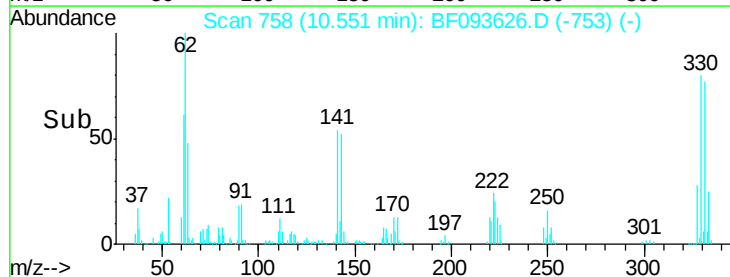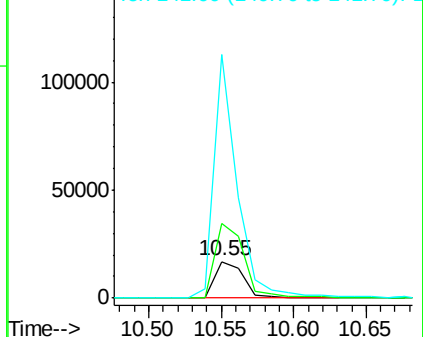

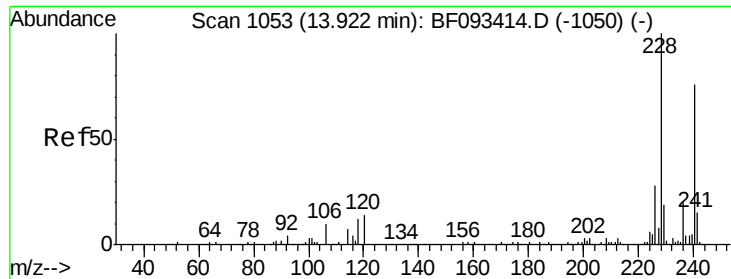

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.90 min Scan# 1051

Delta R.T. 0.01 min

Lab File: BF093626.D

Acq: 14 Mar 2017 00:12

Instrument :

BNA_F

ClientSampleId :

PB97546BL


Tgt Ion:240 Resp: 506232

Ion Ratio Lower Upper

240 100

120 10.3 12.9 19.3#




236 26.0 20.9 31.3

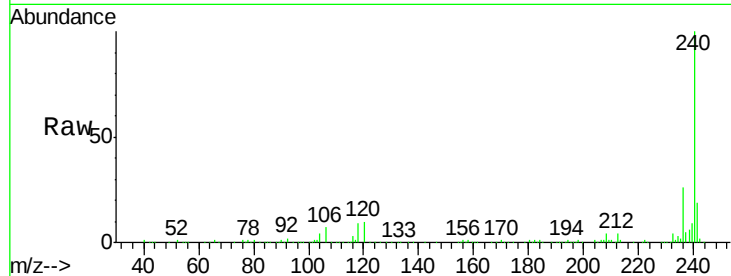

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

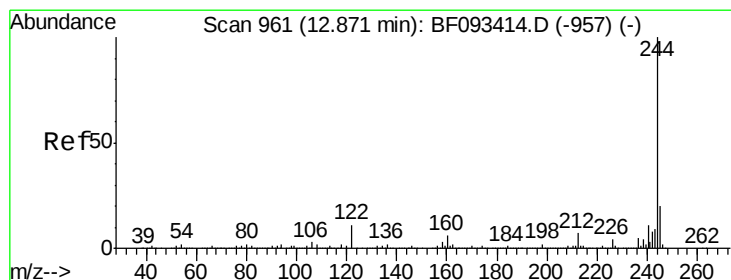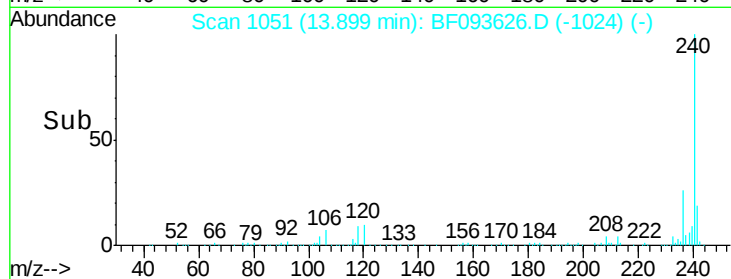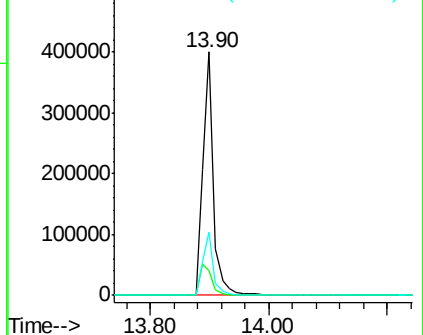

#78

Terphenyl-d14

Concen: 74.35 ng

RT: 12.84 min Scan# 958

Delta R.T. 0.01 min

Lab File: BF093626.D

Acq: 14 Mar 2017 00:12


Tgt Ion:244 Resp: 1447603

Ion Ratio Lower Upper

244 100

212 7.9 6.2 9.2



122 12.6 11.4 17.2

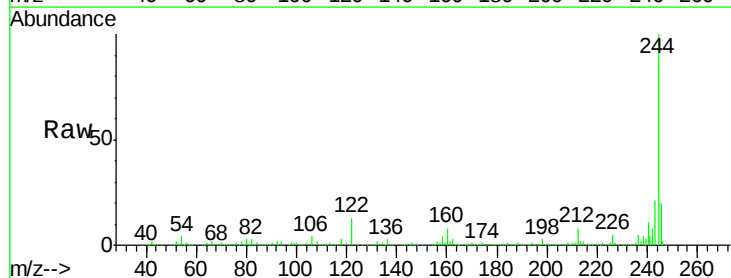


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

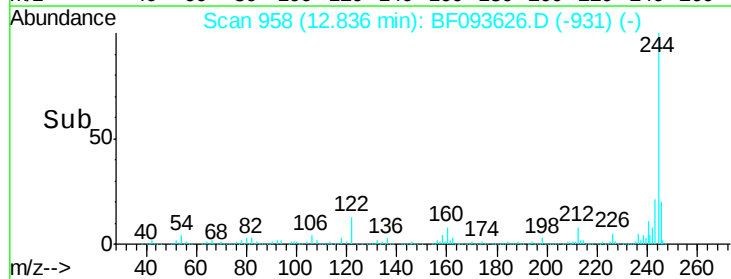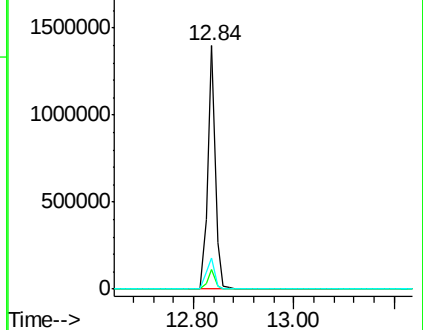


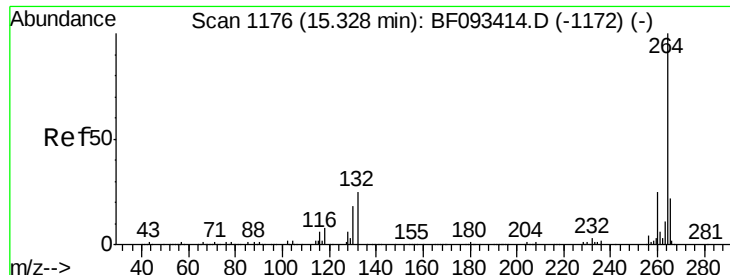

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.31 min Scan# 1174
Delta R.T. 0.02 min
Lab File: BF093626.D
Acq: 14 Mar 2017 00:12

Instrument :
BNA_F
ClientSampleId :
PB97546BL

Tgt Ion: 264 Resp: 350365
Ion Ratio Lower Upper
264 100
260 23.7 19.2 28.8
265 20.9 17.4 26.0

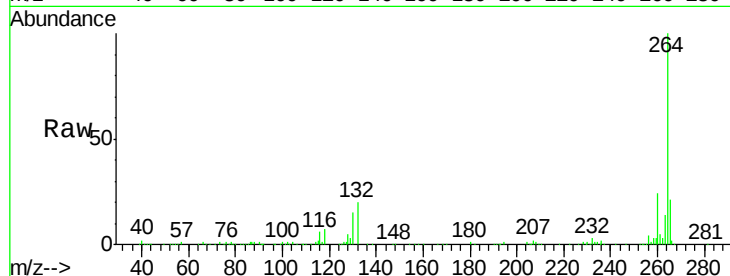

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

