
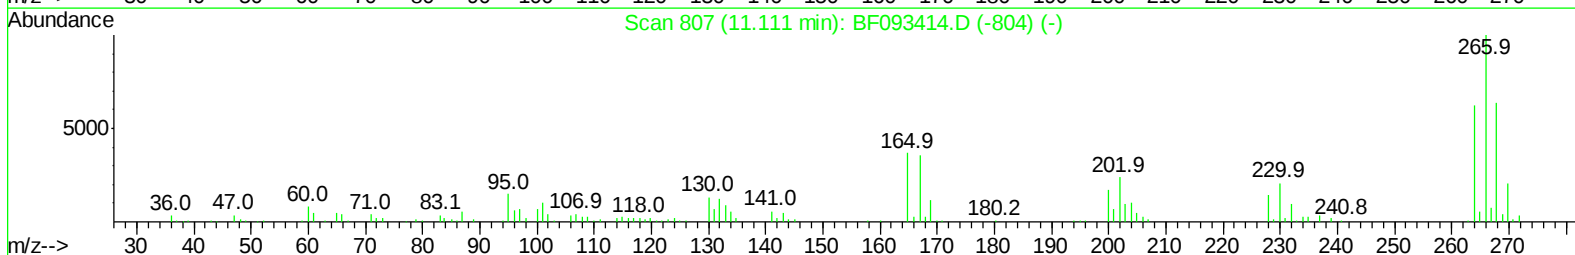
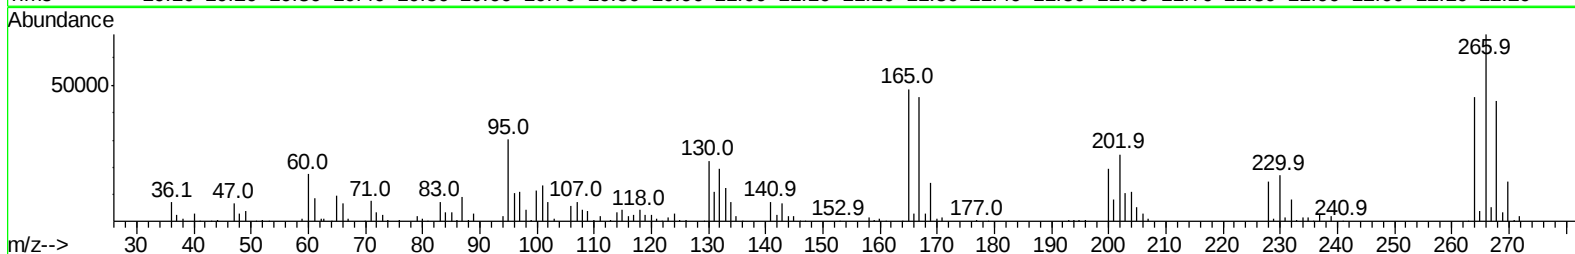


Data Path : Z:\HPCHEM1\BNA F\Data\BF031317\
Data File : BF093624.D
Acq On : 13 Mar 2017 23:18
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 08:08:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 13 15:05:08 2017
Response via : Initial Calibration

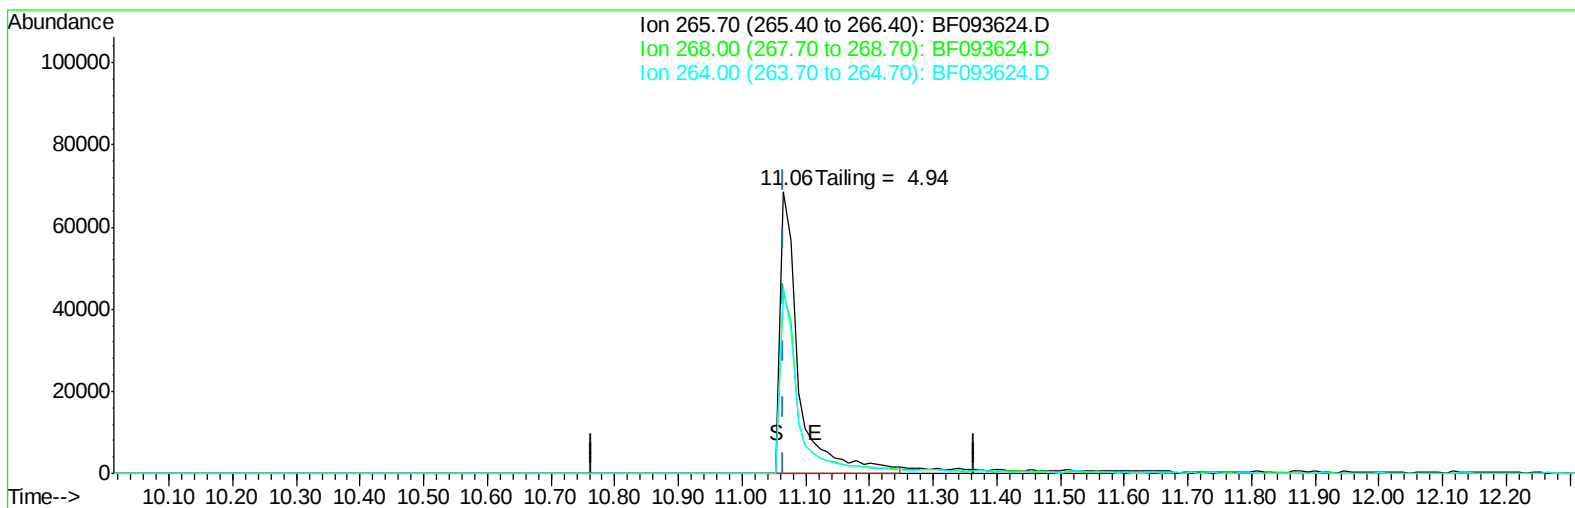

TIC: BF093624.D

(69) Pentachlorophenol (C)




11.065min (-0.000) 0.00ng

response 141864

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	64.24
264.00	62.90	66.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF031317\
Data File : BF093624.D
Acq On : 13 Mar 2017 23:18
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 08:08:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 13 15:05:08 2017
Response via : Initial Calibration

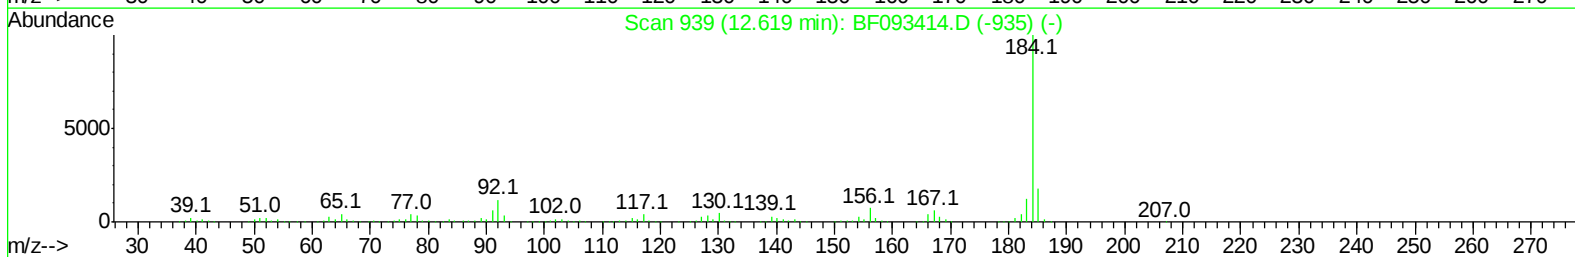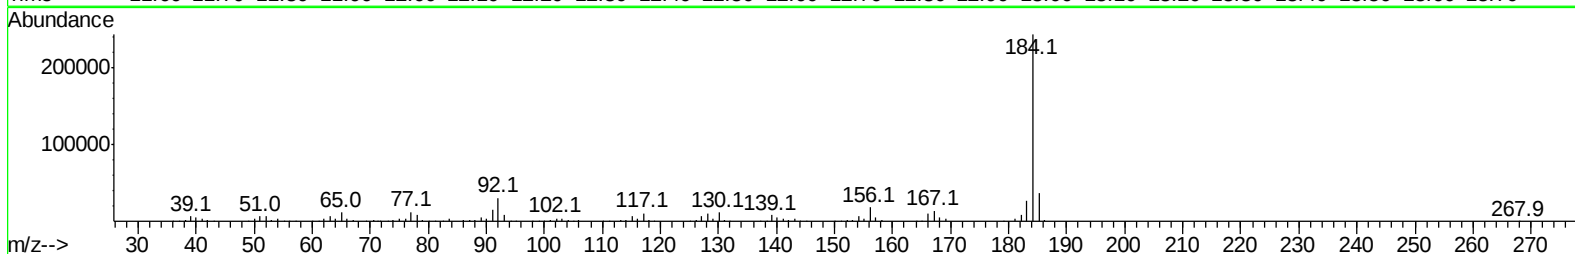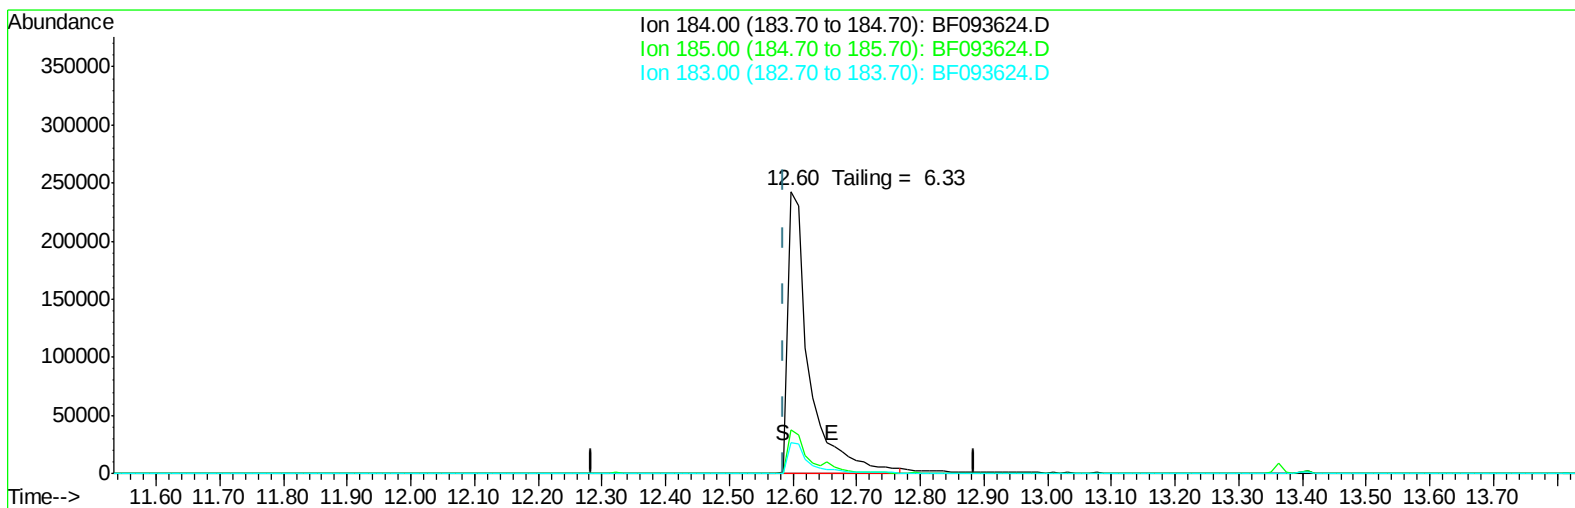

TIC: BF093624.D

(76) Benzidine

12.596min (+0.011) 0.00ng

response 573221

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.47
183.00	11.50	11.14
0.00	0.00	0.00