
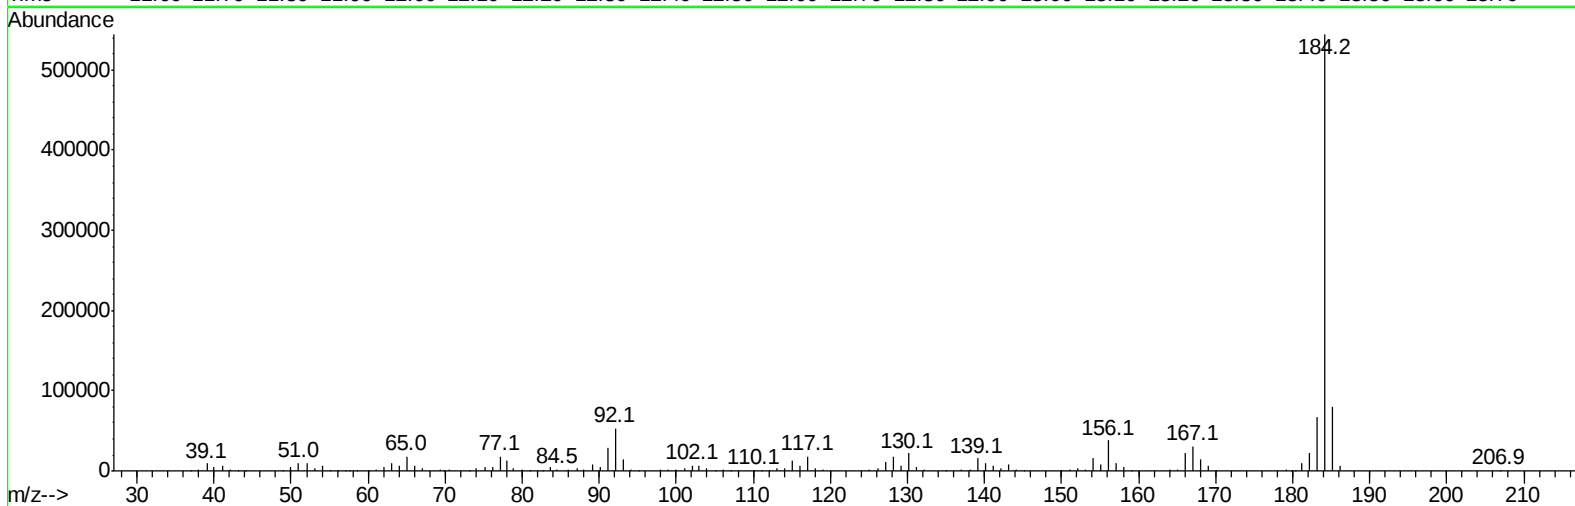


Data Path : Z:\HPCHEM1\BNA F\Data\BF031317\
Data File : BF093649.D
Acq On : 14 Mar 2017 10:47
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 08:26:21 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 13 15:05:08 2017
Response via : Initial Calibration

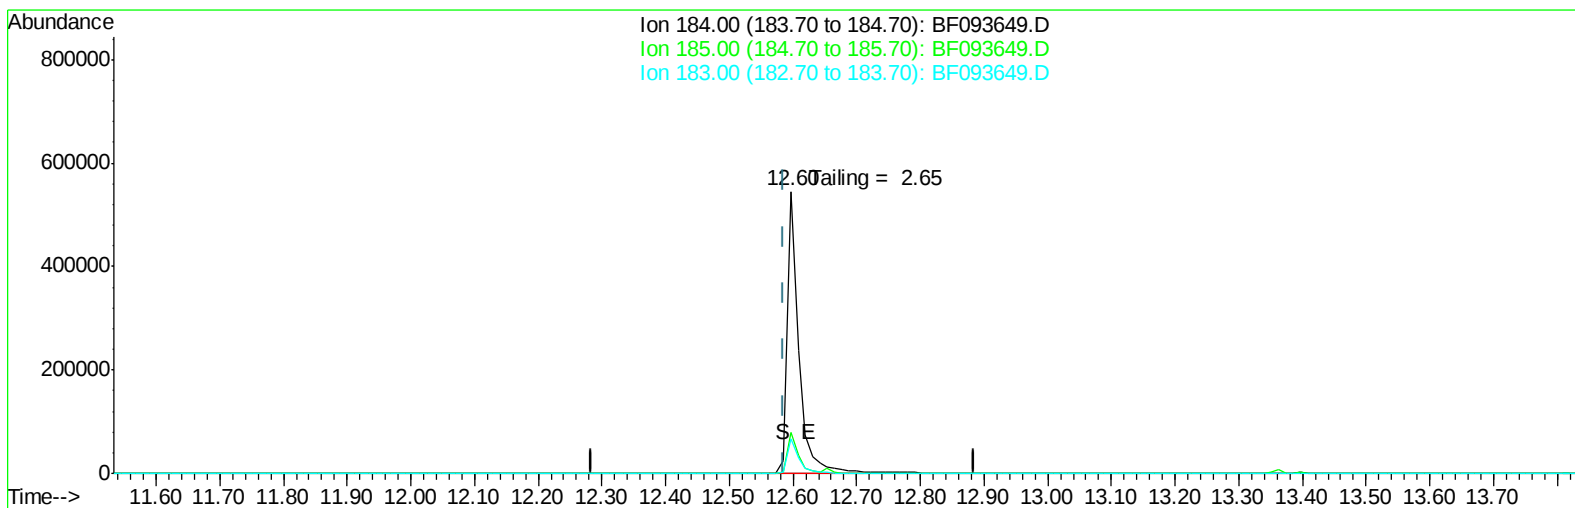

TIC: BF093649.D

(76) Benzidine




12.596min (+0.011) 0.00ng

response 682792

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.67
183.00	11.50	12.20
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF031317\
Data File : BF093649.D
Acq On : 14 Mar 2017 10:47
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 08:26:21 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 13 15:05:08 2017
Response via : Initial Calibration

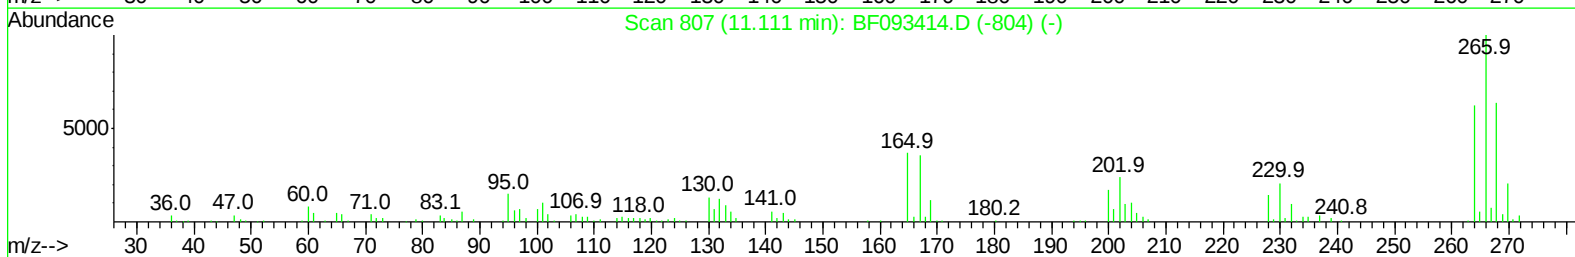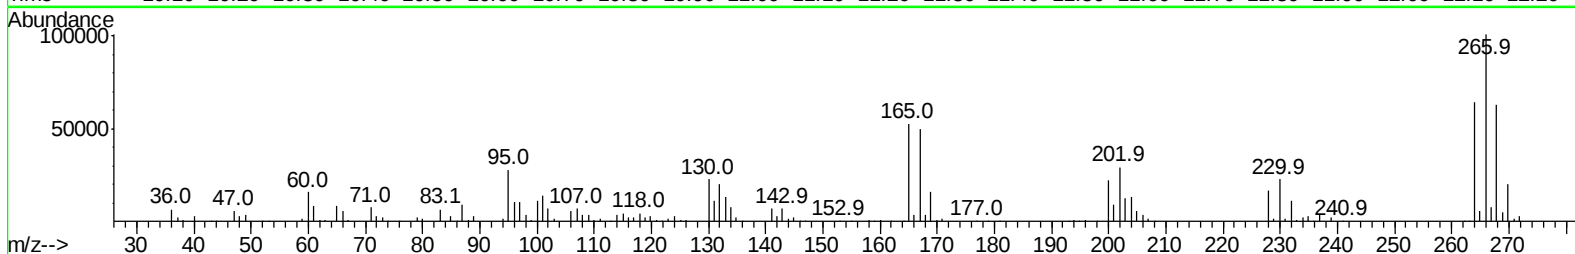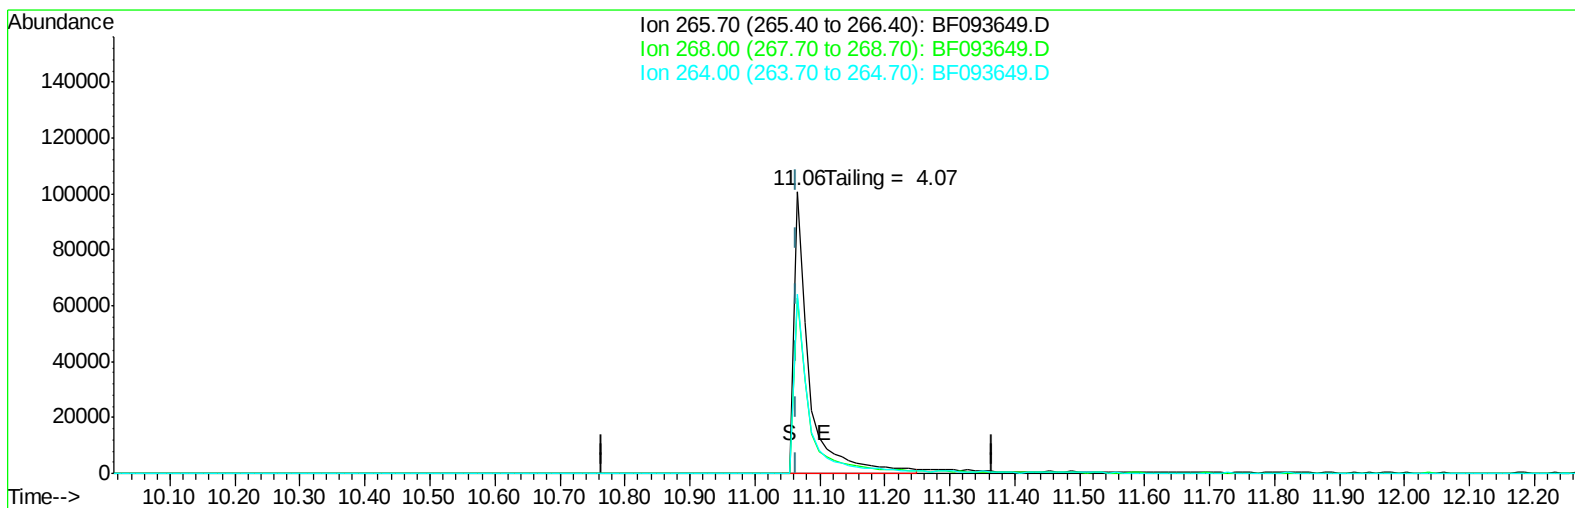

TIC: BF093649.D

(69) Pentachlorophenol (C)

11.065min (-0.000) 0.00ng

response 164197

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	62.50
264.00	62.90	63.57
0.00	0.00	0.00