

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031317\
 Data File : BF093628.D
 Acq On : 14 Mar 2017 1:07
 Operator : SJ/MA
 Sample : PB97546TB
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB97546TB

Quant Time: Mar 14 02:28:42 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 13 15:05:08 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.71	152	182529	20.00	ng	-0.01
21) Naphthalene-d8	8.00	136	722256	20.00	ng	-0.01
38) Acenaphthene-d10	9.76	164	339871	20.00	ng	0.00
63) Phenanthrene-d10	11.25	188	662677	20.00	ng	0.00
75) Chrysene-d12	13.90	240	510099	20.00	ng	0.01
86) Perylene-d12	15.31	264	345191	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	1450864	132.29	ng	0.00
7) Phenol-d6	6.37	99	1775052	128.35	ng	-0.01
23) Nitrobenzene-d5	7.28	82	1085426	83.38	ng	-0.02
41) 2,4,6-Tribromophenol	10.56	330	312604	141.17	ng	0.01
44) 2-Fluorobiphenyl	9.09	172	1735776	95.00	ng	0.00
78) Terphenyl-d14	12.84	244	1425990	72.68	ng	0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031317\
Data File : BF093628.D
Acq On : 14 Mar 2017 1:07
Operator : SJ/MA
Sample : PB97546TB
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB97546TB

Quant Time: Mar 14 02:28:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 13 15:05:08 2017
Response via : Initial Calibration

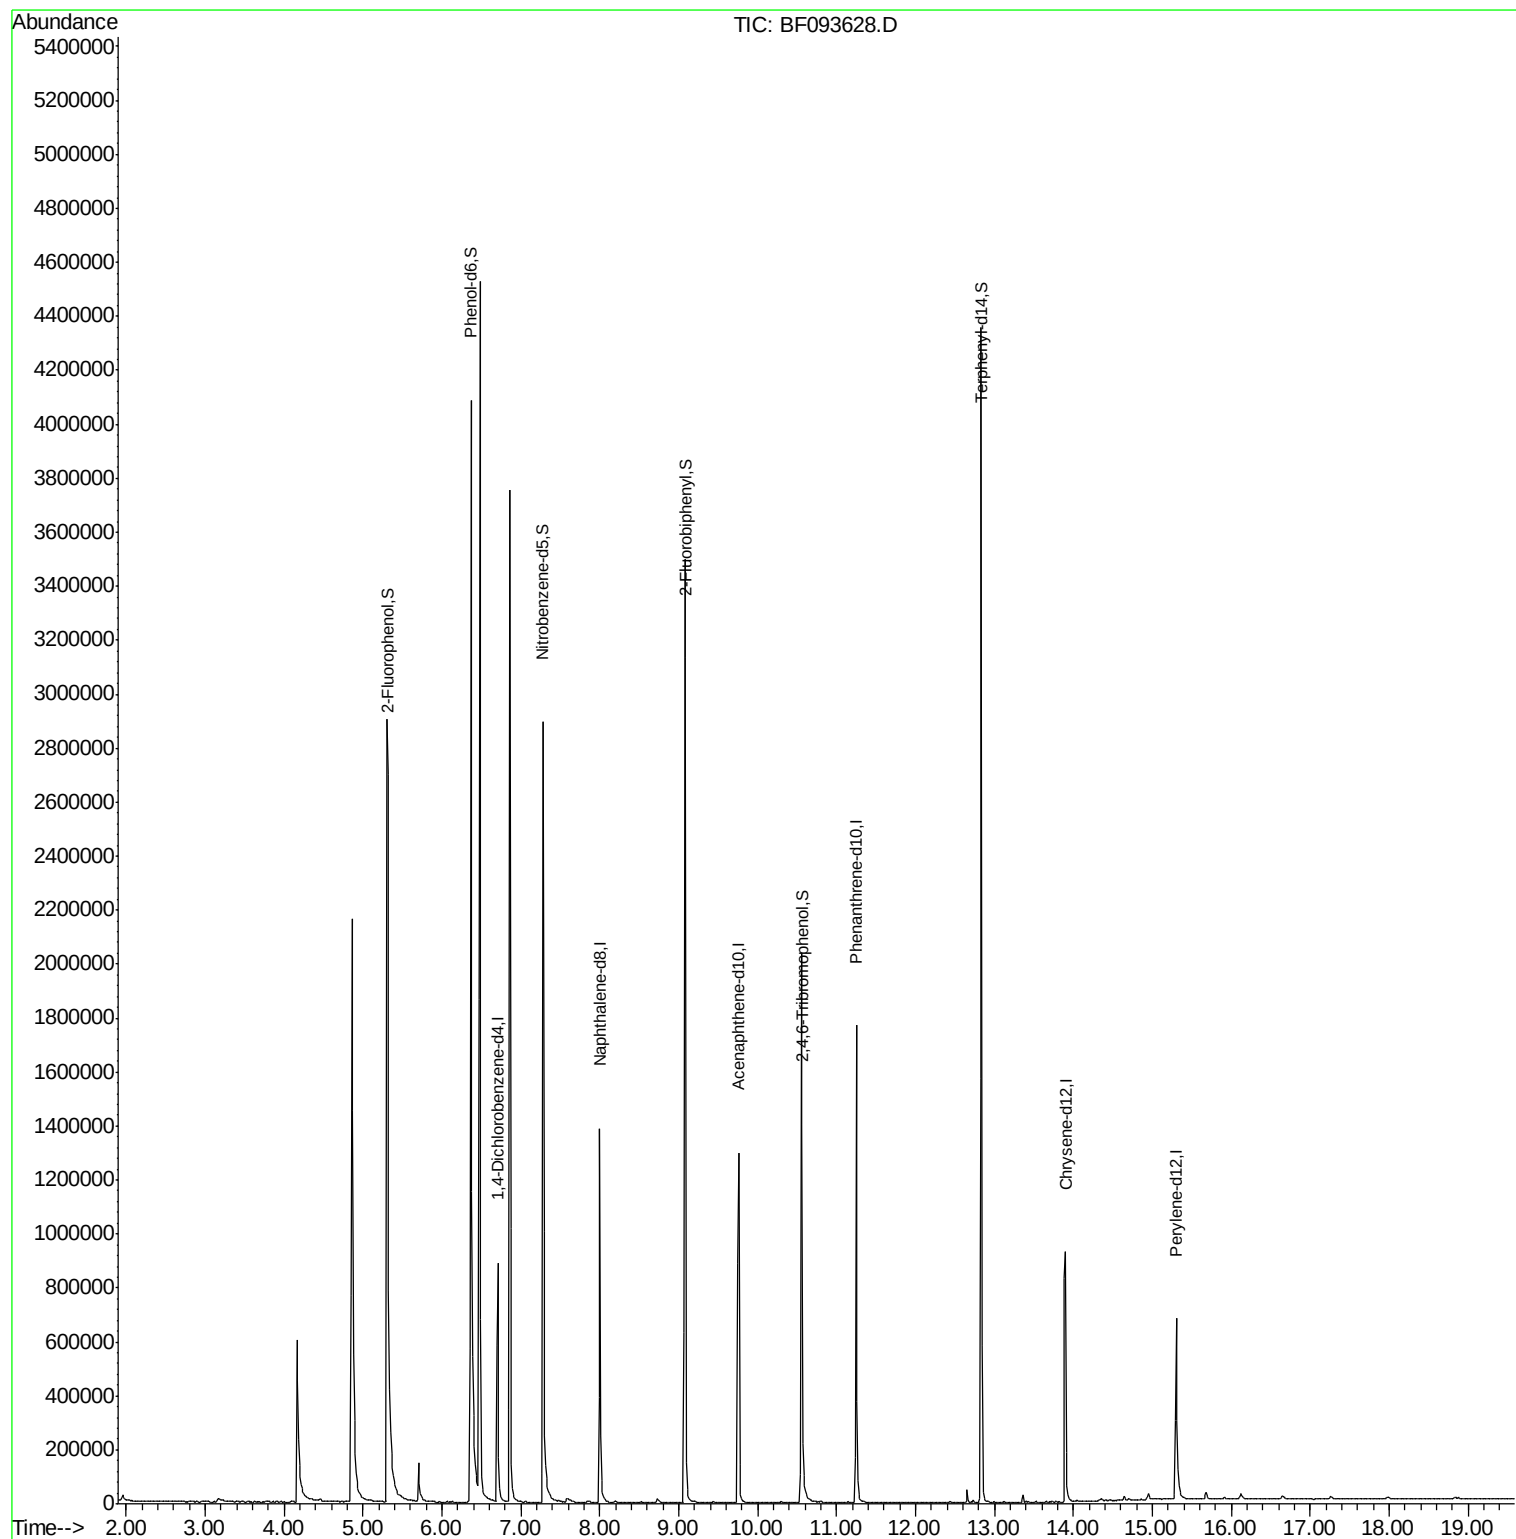

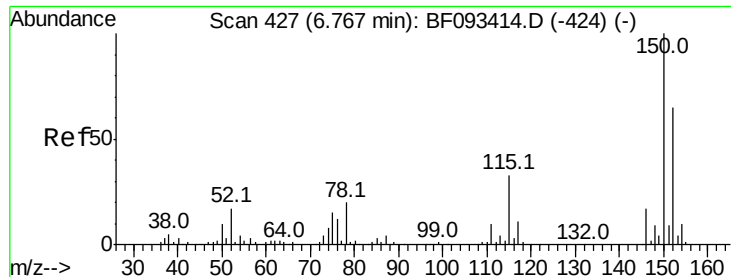

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.71 min Scan# 422

Delta R.T. -0.01 min

Lab File: BF093628.D

Acq: 14 Mar 2017 1:07

Instrument :

BNA_F

ClientSampleId :

PB97546TB


Tot Ion:152 Resp: 182529

Ion Ratio Lower Upper

152 100

150 157.5 124.9 187.3




115 57.1 46.0 69.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

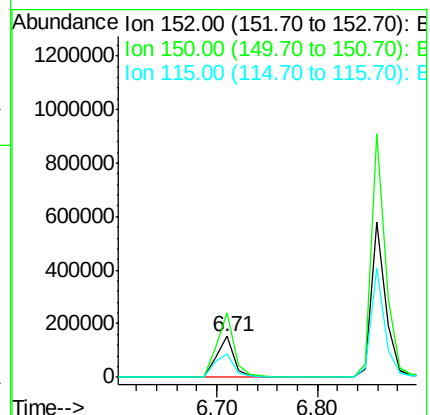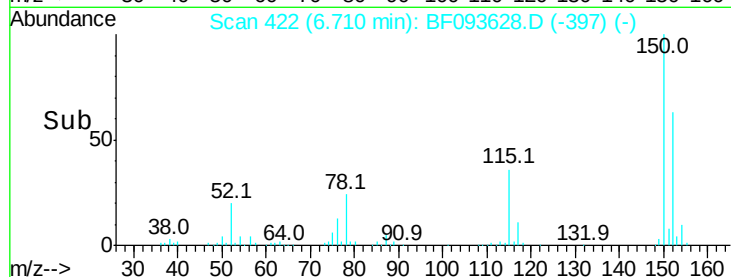

#5

2-Fluorophenol

Concen: 132.29 ng

RT: 5.32 min Scan# 300

Delta R.T. 0.00 min

Lab File: BF093628.D

Acq: 14 Mar 2017 1:07


Tgt Ion:112 Resp: 1450864

Ion Ratio Lower Upper

112 100

64 58.3 46.1 69.1



63 30.5 23.8 35.6




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

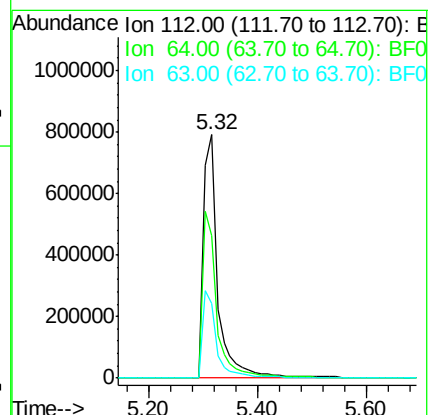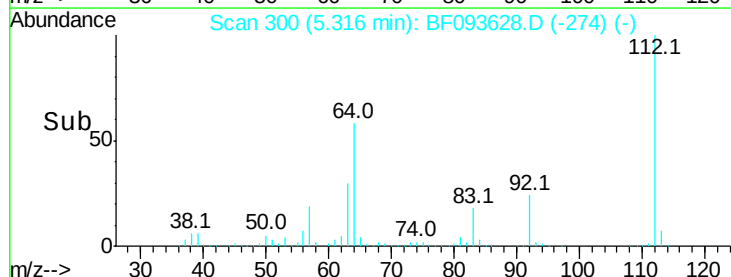

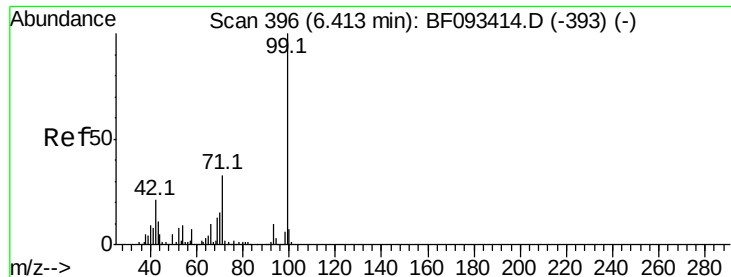

#7

Phenol-d6

Concen: 128.35 ng

RT: 6.37 min Scan# 392

Delta R.T. -0.01 min

Lab File: BF093628.D

Acq: 14 Mar 2017 1:07

Instrument :

BNA_F

ClientSampleId :

PB97546TB





Tot Ion: 99 Resp: 1775052

Ion Ratio Lower Upper

99 100

42 20.8 15.6 23.4

71 34.1 27.5 41.3

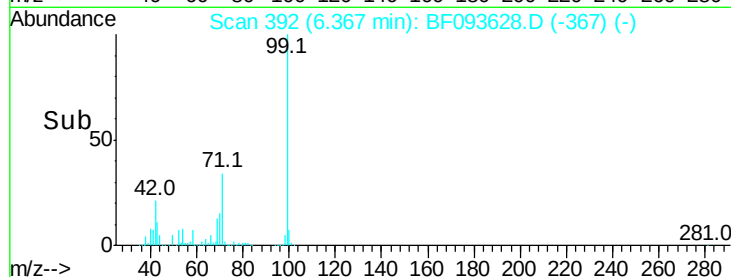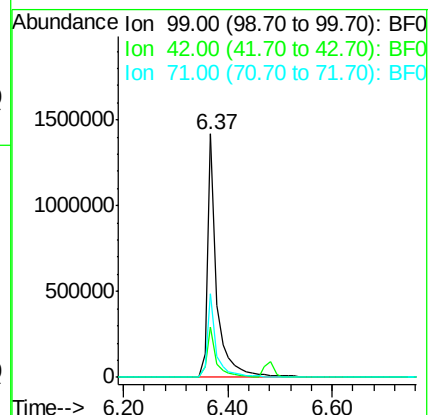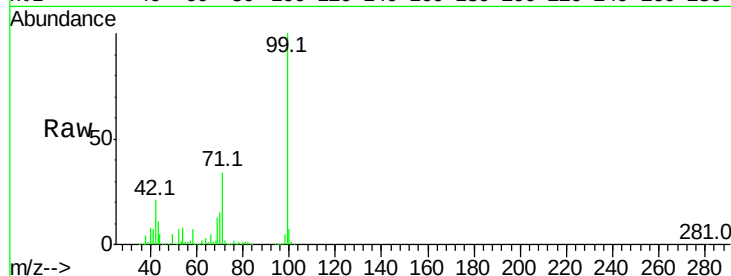

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.00 min Scan# 535

Delta R.T. -0.01 min

Lab File: BF093628.D

Acq: 14 Mar 2017 1:07

Tgt Ion: 136 Resp: 722256




Ion Ratio Lower Upper


136 100

137 10.7 8.4 12.6

54 9.1 4.5 6.7#

68 6.7 3.6 5.4#

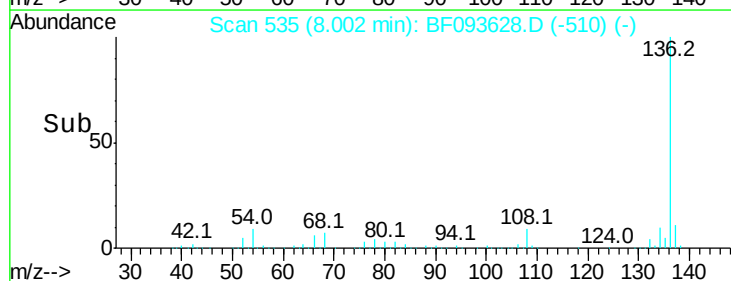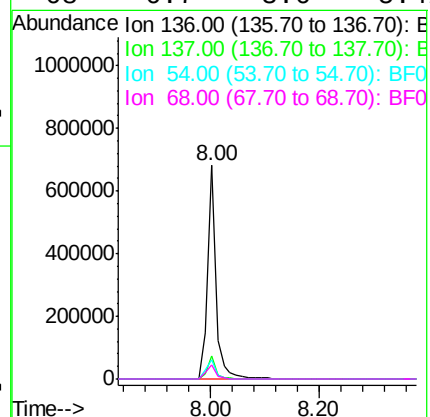


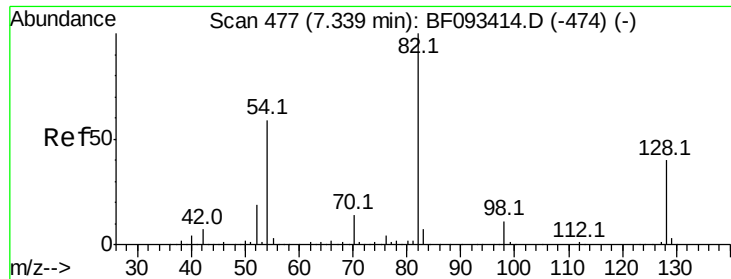




#23
Nitrobenzene-d5
Concen: 83.38 ng
RT: 7.28 min Scan# 472
Delta R.T. -0.02 min
Lab File: BF093628.D
Acq: 14 Mar 2017 1:07

Instrument :
BNA_F
ClientSampleId :
PB97546TB

Tot Ion: 82 Resp: 1085426
Ion Ratio Lower Upper
82 100
128 38.0 34.6 52.0
54 61.1 39.5 59.3#




Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

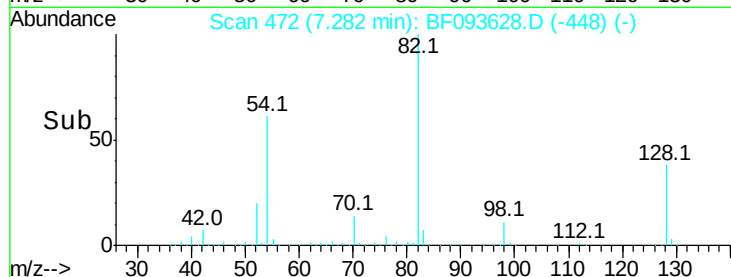
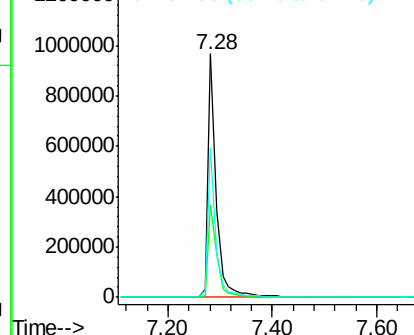



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.76 min Scan# 689
Delta R.T. 0.00 min
Lab File: BF093628.D
Acq: 14 Mar 2017 1:07

Tgt Ion:164 Resp: 339871
Ion Ratio Lower Upper
164 100
162 102.4 80.2 120.2
160 47.7 36.9 55.3



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

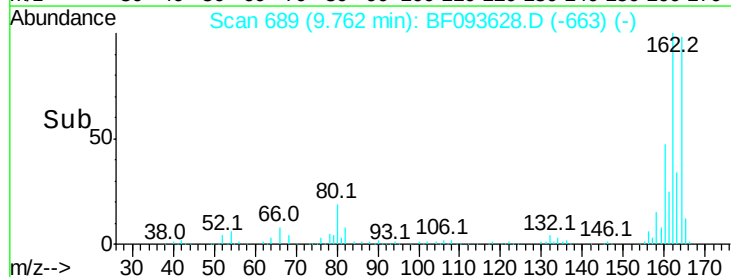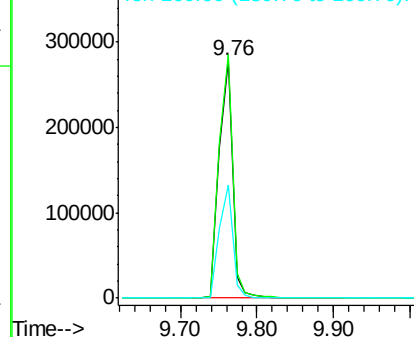


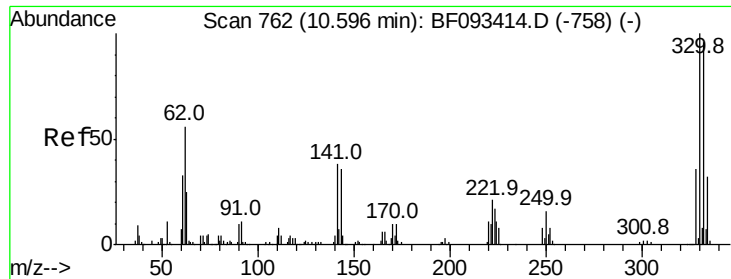




#41
 2,4,6-Tribromophenol
 Concen: 141.17 ng
 RT: 10.56 min Scan# 759
 Delta R.T. 0.01 min
 Lab File: BF093628.D
 Acq: 14 Mar 2017 1:07

Instrument :
 BNA_F
 ClientSampleId :
 PB97546TB

Tot Ion:330 Resp: 312604
 Ion Ratio Lower Upper
 330 100
 332 96.5 77.4 116.2
 141 39.9 34.1 51.1




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

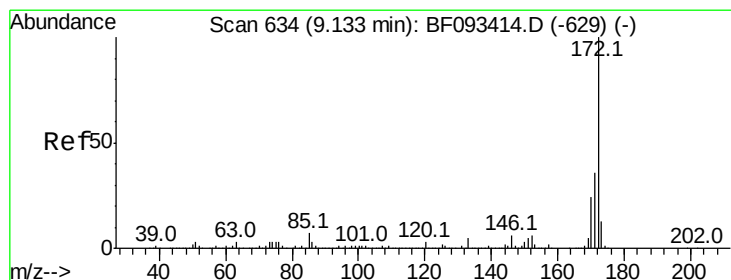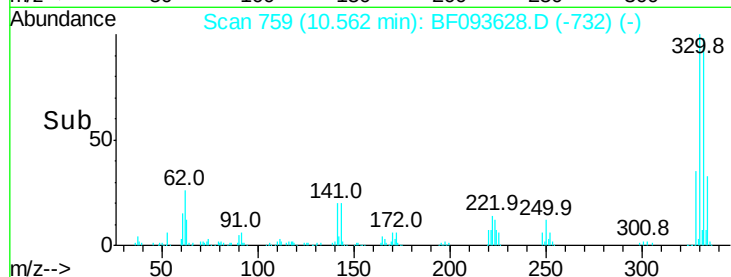
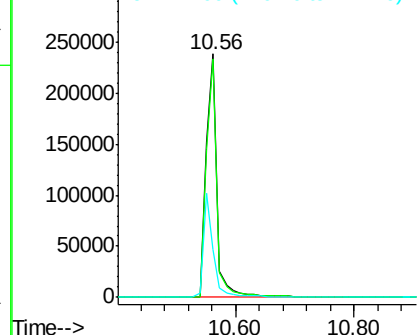



#44
 2-Fluorobiphenyl
 Concen: 95.00 ng
 RT: 9.09 min Scan# 630
 Delta R.T. 0.00 min
 Lab File: BF093628.D
 Acq: 14 Mar 2017 1:07

Tgt Ion:172 Resp: 1735776
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.4 44.0
 170 24.4 20.2 30.4

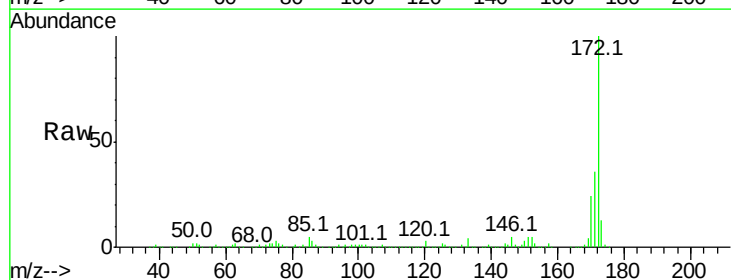

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

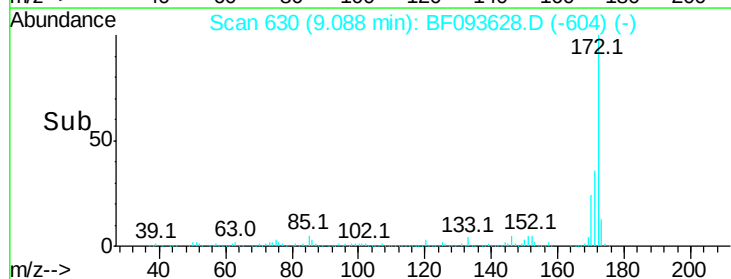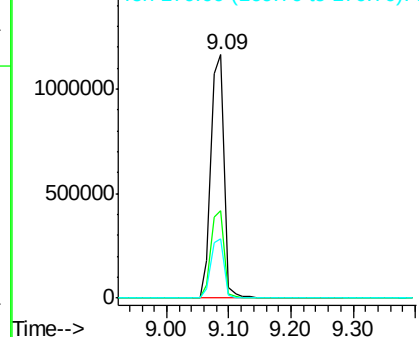

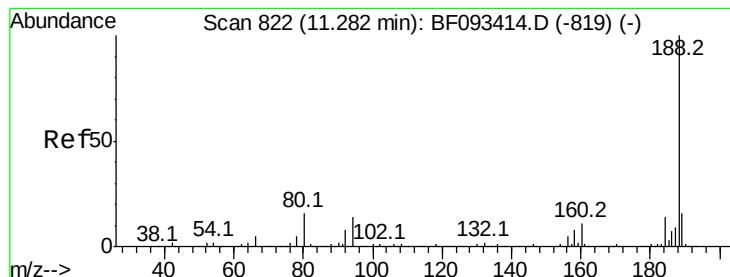

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.25 min Scan# 819

Delta R.T. 0.00 min

Lab File: BF093628.D

Acq: 14 Mar 2017 1:07

Instrument :

BNA_F

ClientSampleId :

PB97546TB


Tot Ion:188 Resp: 662677

Ion Ratio Lower Upper

188 100

94 11.5 10.0 15.0




80 12.2 11.2 16.8

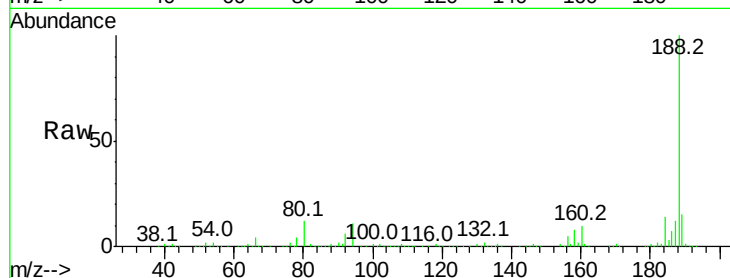

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

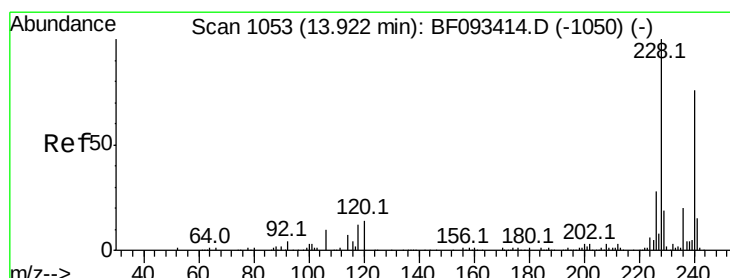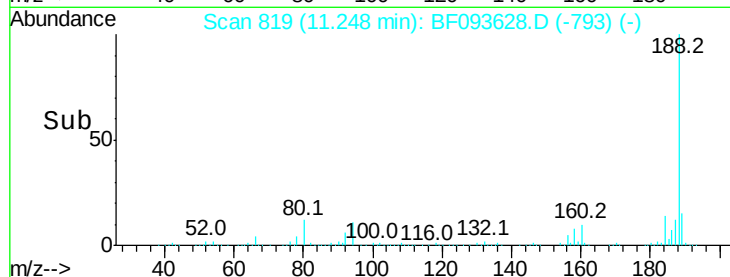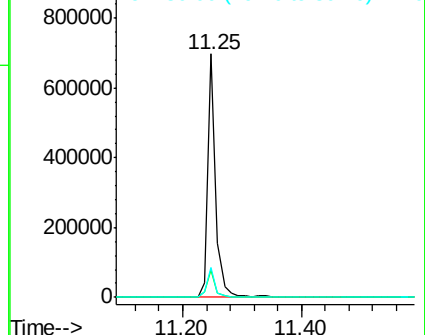

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.90 min Scan# 1051

Delta R.T. 0.01 min

Lab File: BF093628.D

Acq: 14 Mar 2017 1:07


Tgt Ion:240 Resp: 510099

Ion Ratio Lower Upper

240 100

120 10.1 12.9 19.3#



236 26.0 20.9 31.3

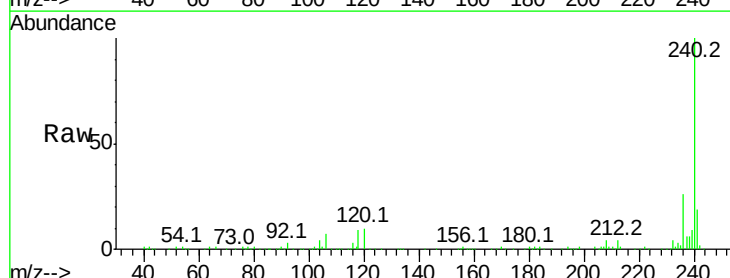


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

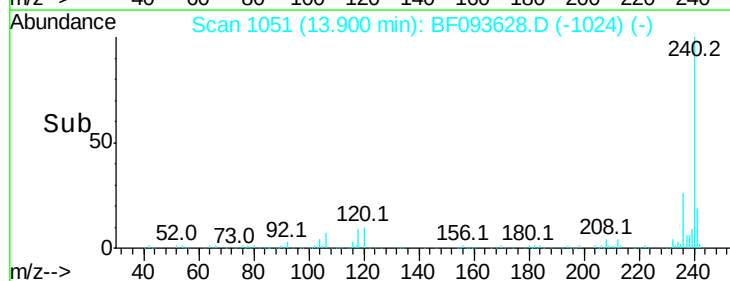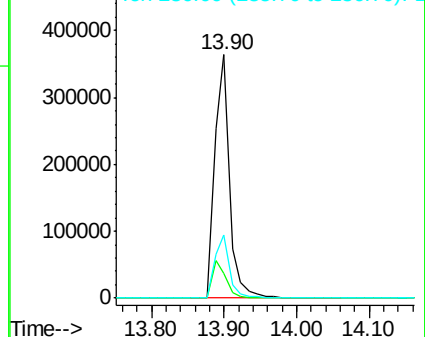

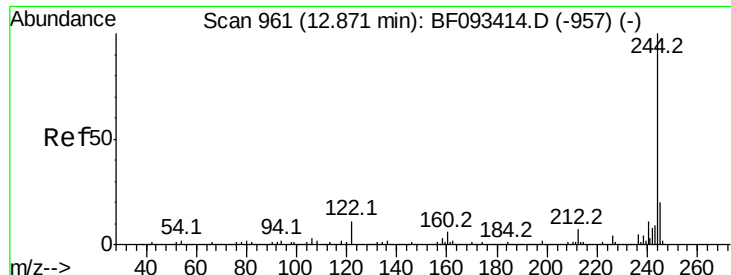

#78

Terphenyl-d14

Concen: 72.68 ng

RT: 12.84 min Scan# 958

Delta R.T. 0.01 min

Lab File: BF093628.D

Acq: 14 Mar 2017 1:07

Instrument :

BNA_F

ClientSampleId :

PB97546TB


Tot Ion:244 Resp: 1425990

Ion Ratio Lower Upper

244 100

212 8.0 6.2 9.2




122 12.6 11.4 17.2



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

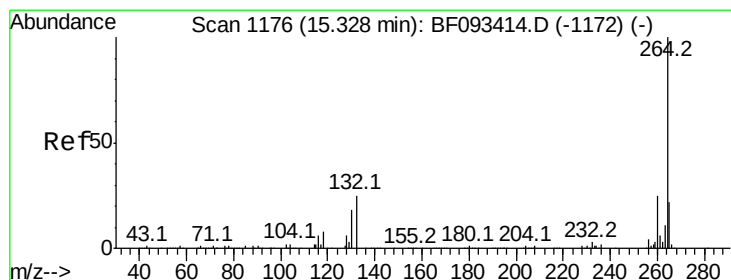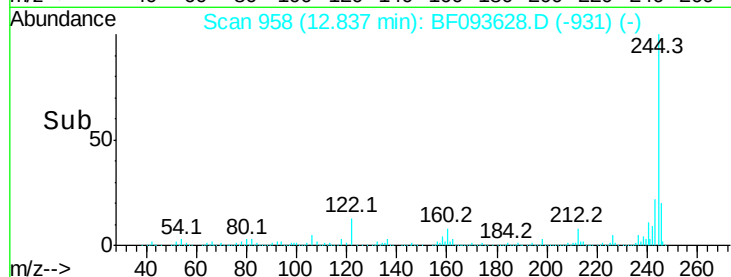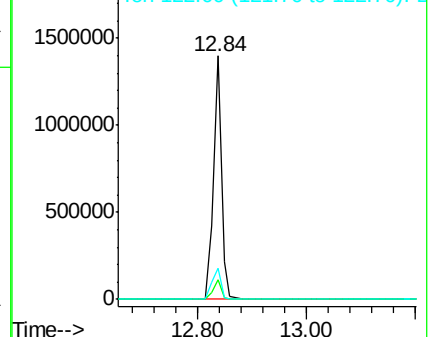

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.31 min Scan# 1174

Delta R.T. 0.02 min

Lab File: BF093628.D

Acq: 14 Mar 2017 1:07


Tgt Ion:264 Resp: 345191

Ion Ratio Lower Upper

264 100

260 24.8 19.2 28.8

265 21.5 17.4 26.0



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

