

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031317\
 Data File : BF093634.D
 Acq On : 14 Mar 2017 3:53
 Operator : SJ/MA
 Sample : I2199-26
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 D-103

Quant Time: Mar 14 04:43:34 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 13 15:05:08 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.71	152	191427	20.00	ng	-0.01
21) Naphthalene-d8	8.00	136	772265	20.00	ng	-0.01
38) Acenaphthene-d10	9.76	164	356434	20.00	ng	0.00
63) Phenanthrene-d10	11.25	188	706597	20.00	ng	0.00
75) Chrysene-d12	13.90	240	502795	20.00	ng	0.01
86) Perylene-d12	15.32	264	96939	20.00	ng	0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	1746714	151.86	ng	0.00
7) Phenol-d6	6.37	99	2183255	150.53	ng	-0.01
23) Nitrobenzene-d5	7.28	82	1459480	104.86	ng	-0.02
41) 2,4,6-Tribromophenol	10.56	330	426027	183.46	ng	0.01
44) 2-Fluorobiphenyl	9.09	172	2244069	117.11	ng	0.00
78) Terphenyl-d14	12.84	244	1846818	95.50	ng	0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031317\
Data File : BF093634.D
Acq On : 14 Mar 2017 3:53
Operator : SJ/MA
Sample : I2199-26
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
D-103

Quant Time: Mar 14 04:43:34 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 13 15:05:08 2017
Response via : Initial Calibration

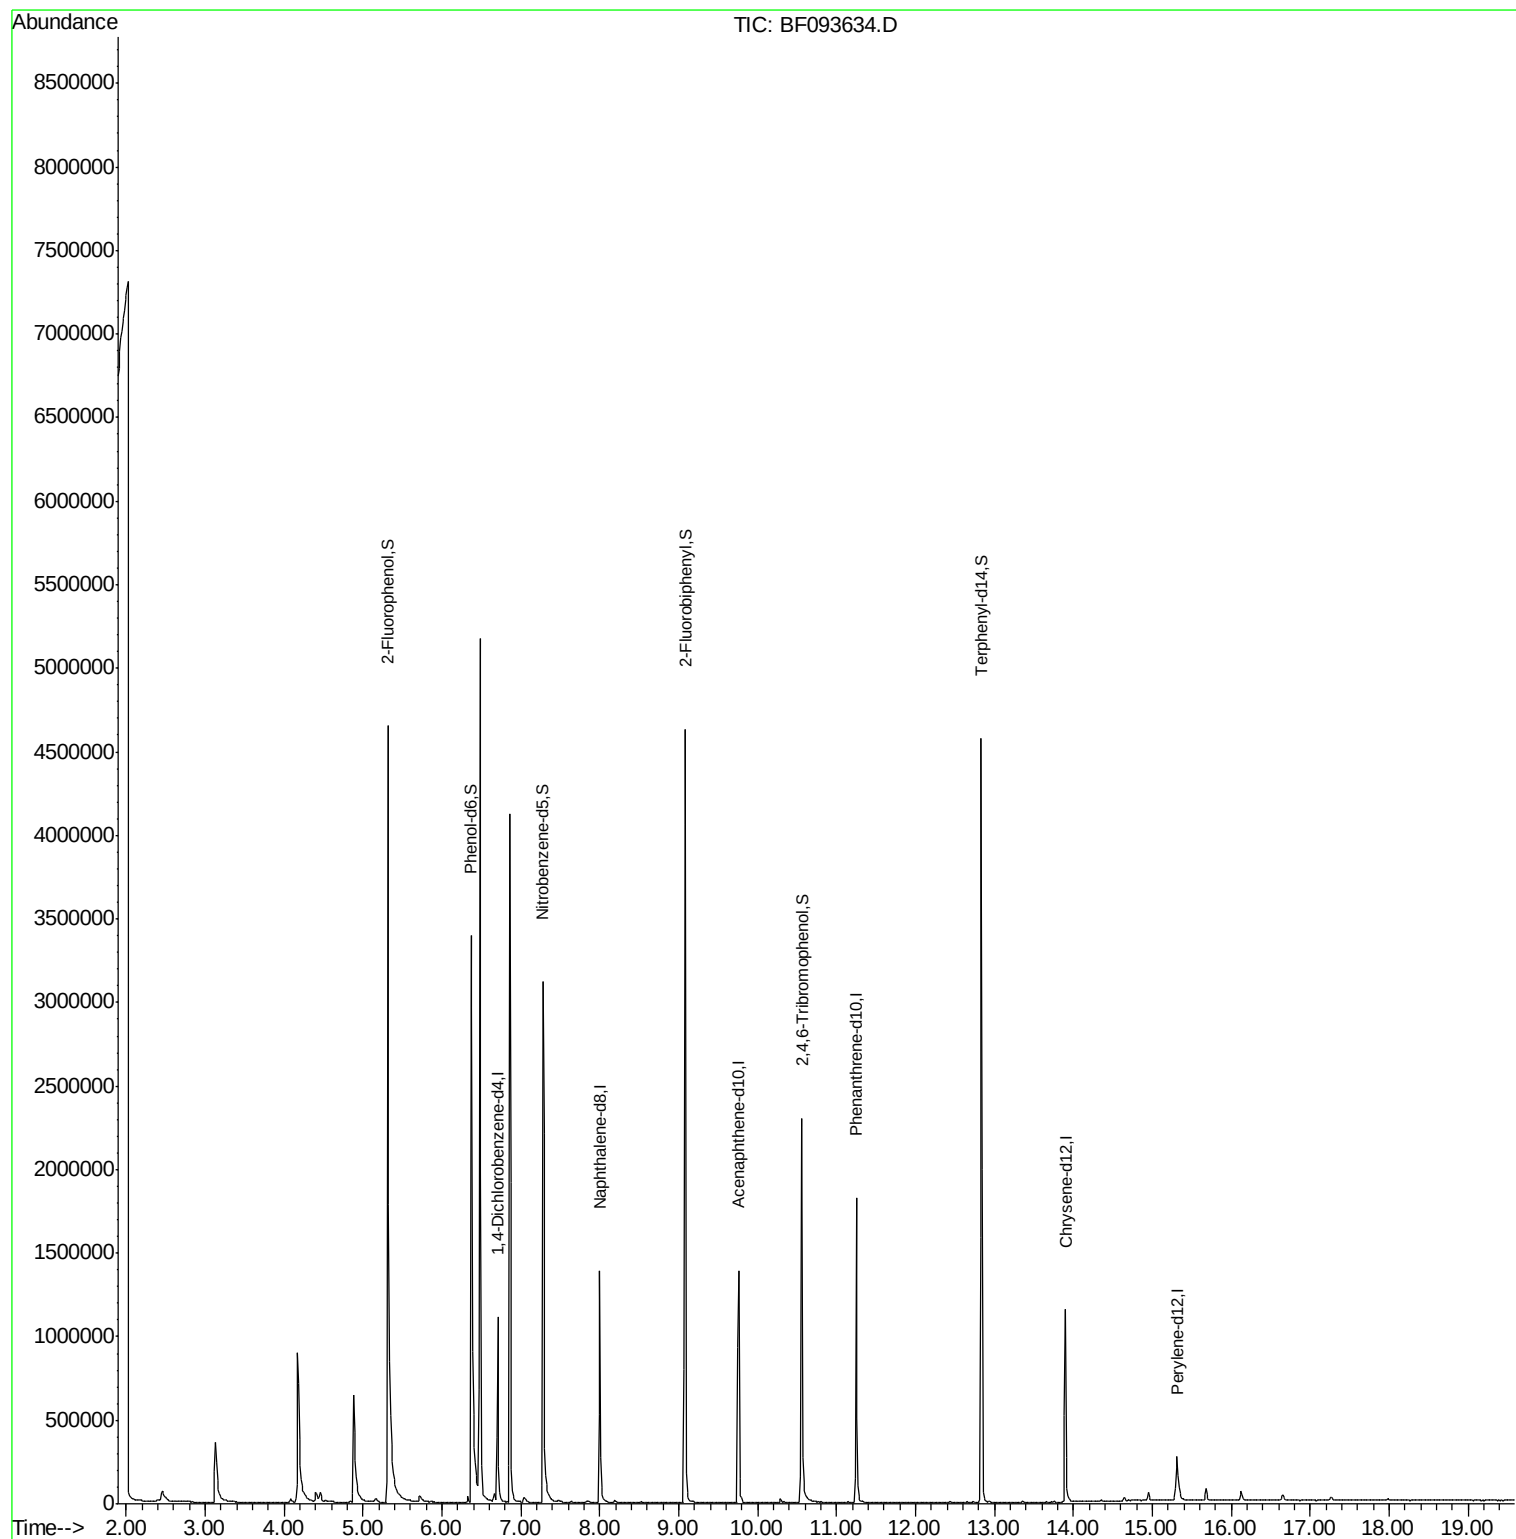

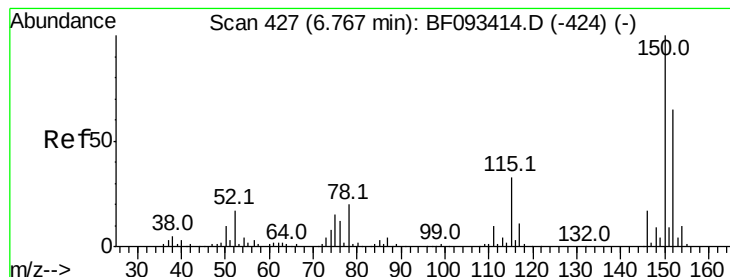


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.71 min Scan# 422
 Delta R.T. -0.01 min
 Lab File: BF093634.D
 Acq: 14 Mar 2017 3:53

Instrument :
 BNA_F
 ClientSampleId :
 D-103

Tot Ion	Ratio	Lower	Upper
152	100		
150	157.1	124.9	187.3
115	57.4	46.0	69.0

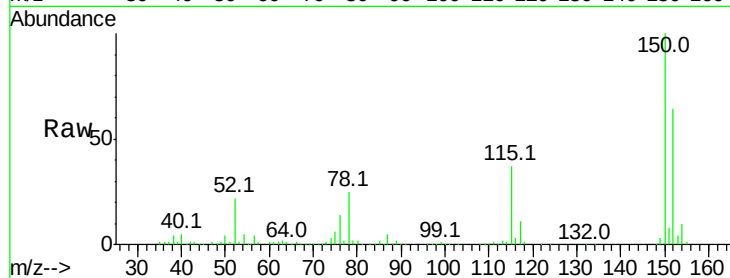


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

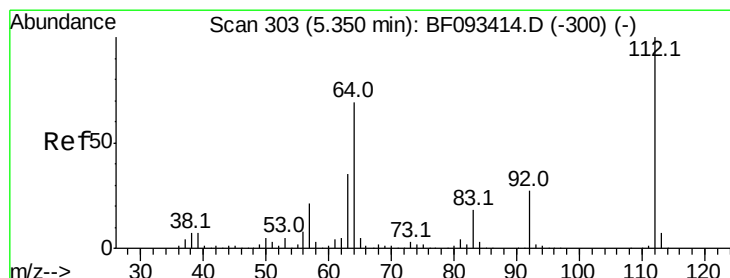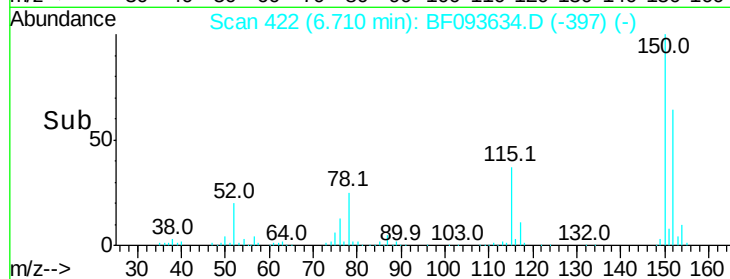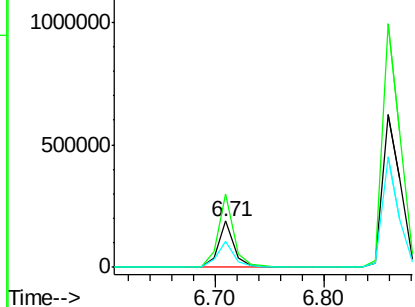



#5


2-Fluorophenol
 Concen: 151.86 ng
 RT: 5.32 min Scan# 300
 Delta R.T. -0.00 min
 Lab File: BF093634.D
 Acq: 14 Mar 2017 3:53

Tgt Ion	Ratio	Lower	Upper
112	100		
64	66.5	46.1	69.1
63	34.7	23.8	35.6

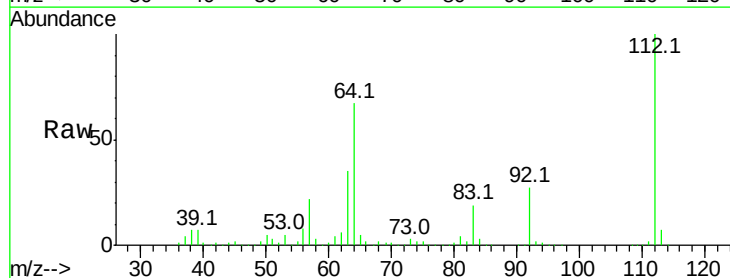

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

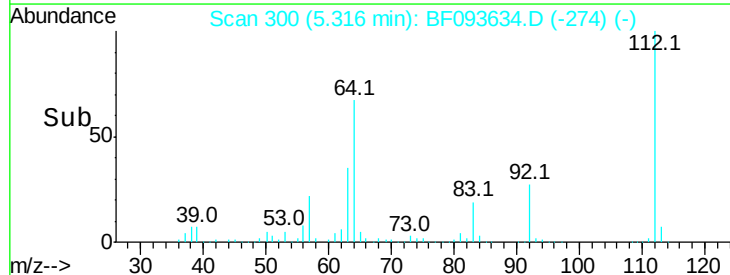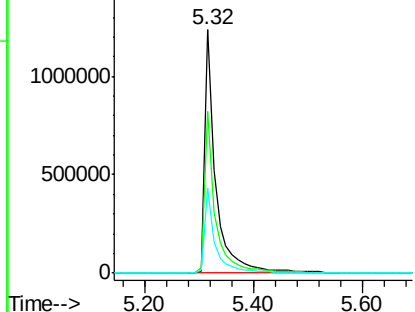

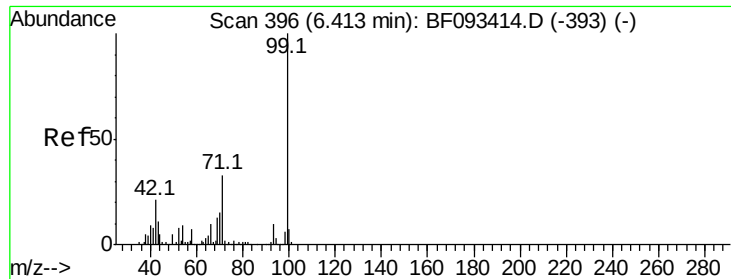

#7

Phenol-d6

Concen: 150.53 ng

RT: 6.37 min Scan# 392

Delta R.T. -0.01 min

Lab File: BF093634.D

Acq: 14 Mar 2017 3:53

Instrument :

BNA_F

ClientSampled :

D-103


Tot Ion: 99 Resp: 2183255

Ion Ratio Lower Upper

99 100

42 23.4 15.6 23.4#




71 35.3 27.5 41.3

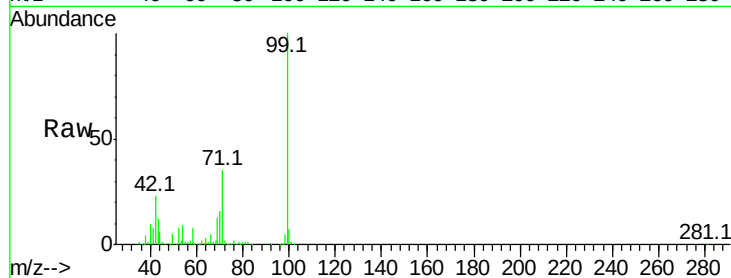

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

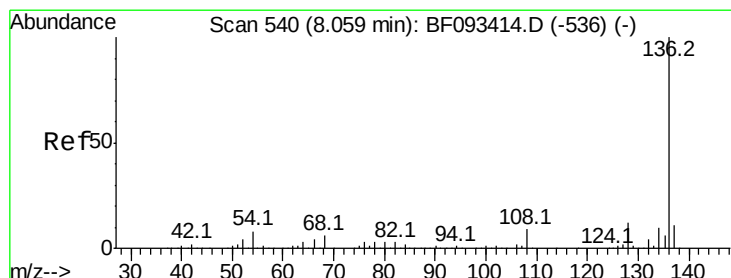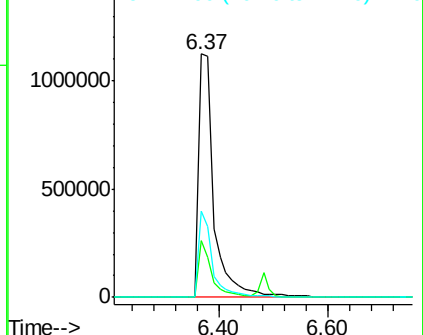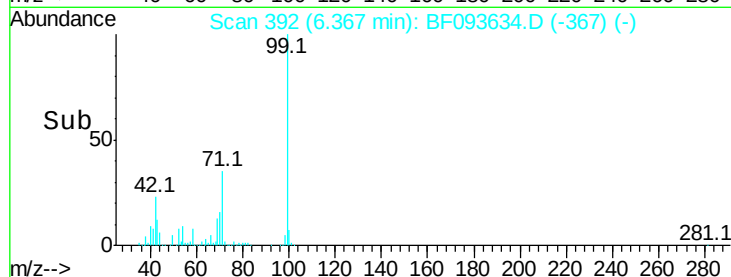

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.00 min Scan# 535

Delta R.T. -0.01 min

Lab File: BF093634.D

Acq: 14 Mar 2017 3:53

Tgt Ion: 136 Resp: 772265


Ion Ratio Lower Upper

136 100

137 10.9 8.4 12.6

54 8.7 4.5 6.7#

68 6.6 3.6 5.4#


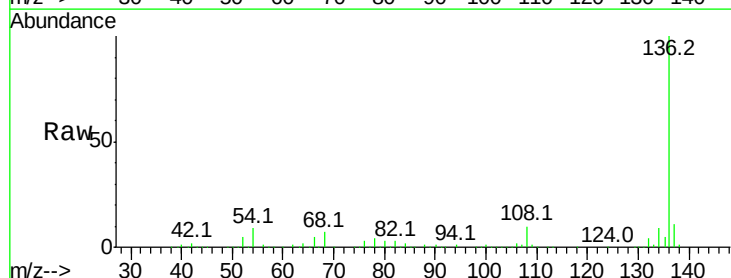



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

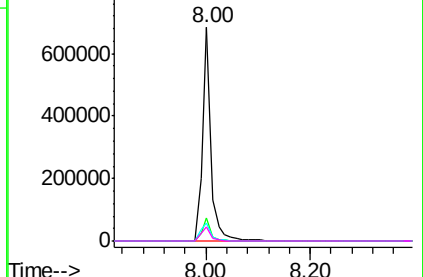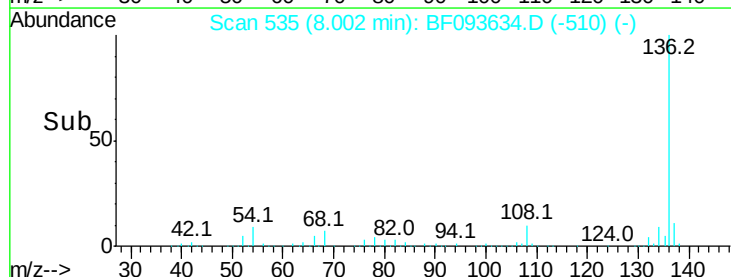




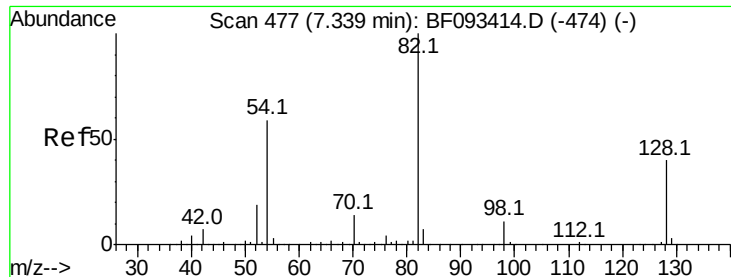


#23
 Nitrobenzene-d5
 Concen: 104.86 ng
 RT: 7.28 min Scan# 472
 Delta R.T. -0.02 min
 Lab File: BF093634.D
 Acq: 14 Mar 2017 3:53

Instrument :
 BNA_F
 ClientSampleId :
 D-103

Tot Ion: 82 Resp: 1459480




Ion	Ratio	Lower	Upper
82	100		
128	37.8	34.6	52.0
54	60.2	39.5	59.3#

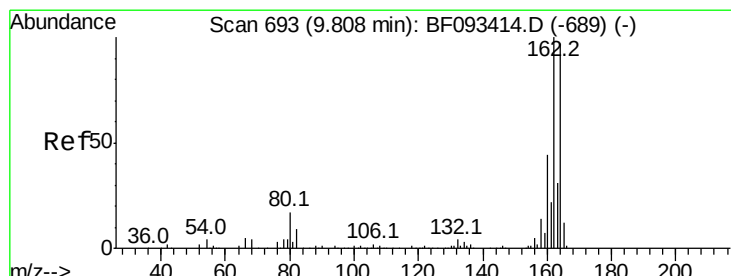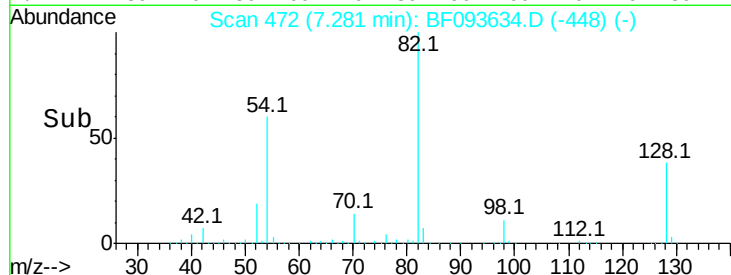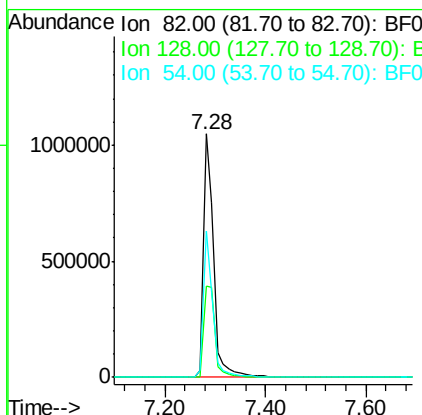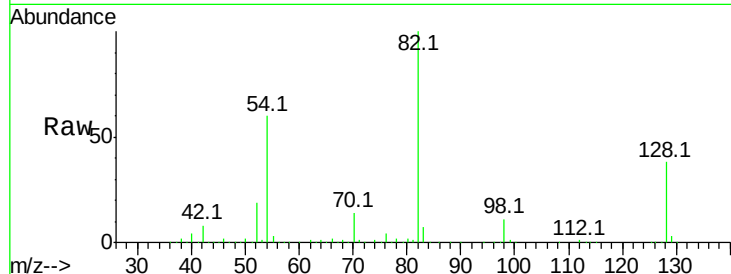


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.76 min Scan# 689
 Delta R.T. -0.00 min
 Lab File: BF093634.D
 Acq: 14 Mar 2017 3:53

Tgt Ion:164 Resp: 356434

Ion	Ratio	Lower	Upper
164	100		
162	105.3	80.2	120.2
160	47.2	36.9	55.3

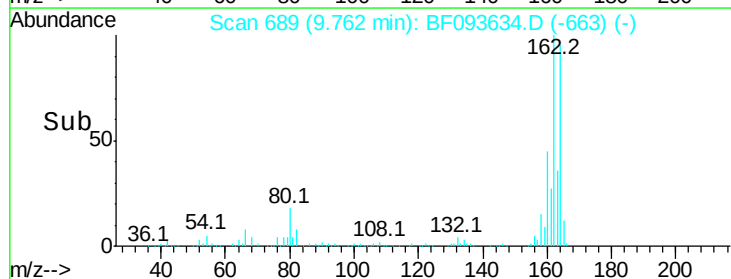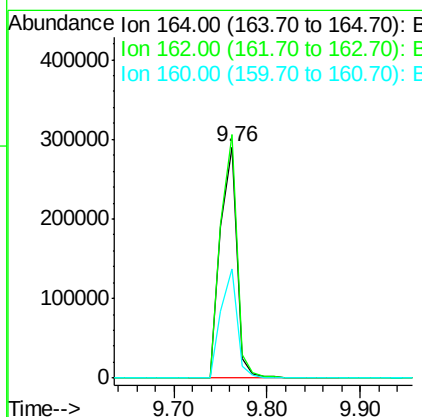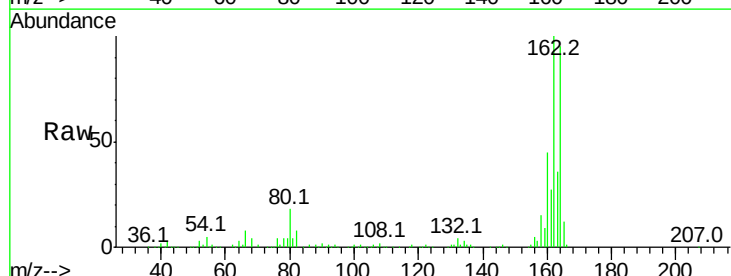


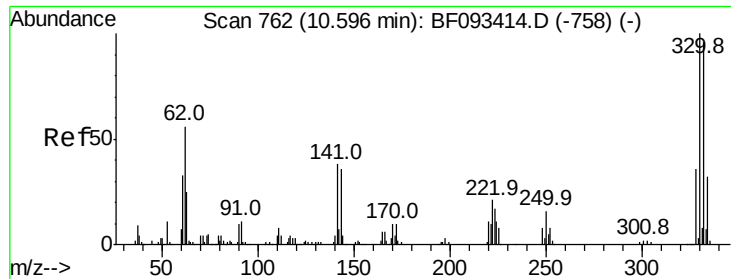




#41
 2,4,6-Tribromophenol
 Concen: 183.46 ng
 RT: 10.56 min Scan# 759
 Delta R.T. 0.01 min
 Lab File: BF093634.D
 Acq: 14 Mar 2017 3:53

Instrument :
 BNA_F
 ClientSampleID :
 D-103

Tot Ion:330 Resp: 426027
 Ion Ratio Lower Upper
 330 100
 332 96.7 77.4 116.2
 141 39.0 34.1 51.1

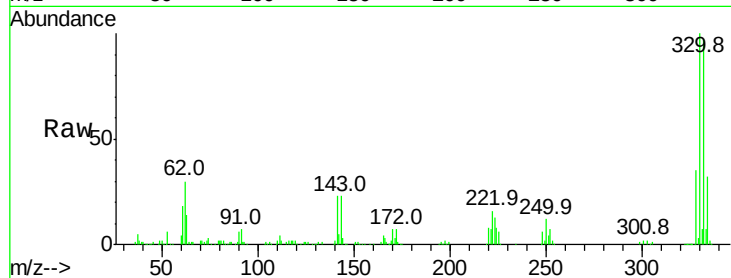


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

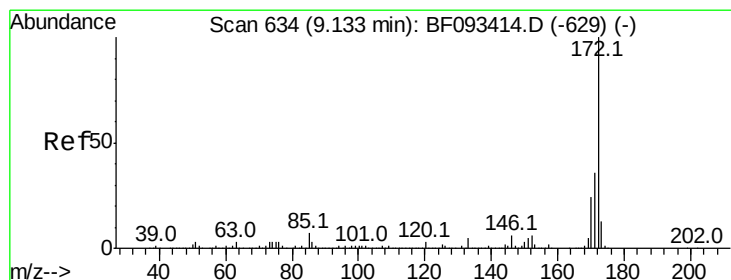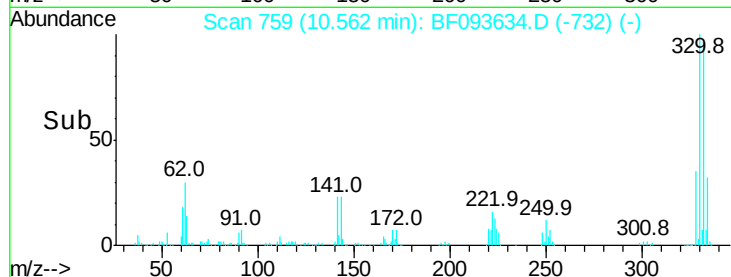
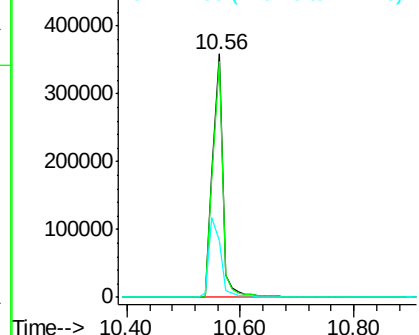



#44
 2-Fluorobiphenyl
 Concen: 117.11 ng
 RT: 9.09 min Scan# 630
 Delta R.T. -0.00 min
 Lab File: BF093634.D
 Acq: 14 Mar 2017 3:53

Tgt Ion:172 Resp: 2244069
 Ion Ratio Lower Upper
 172 100
 171 37.2 29.4 44.0
 170 25.0 20.2 30.4

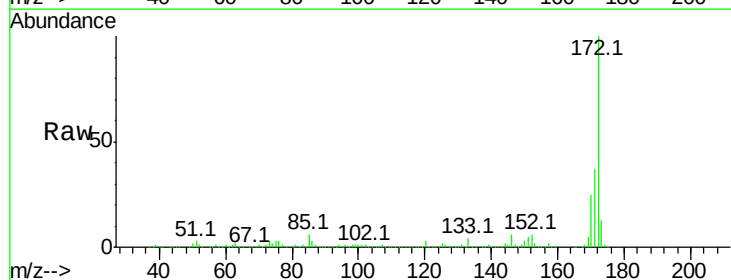

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



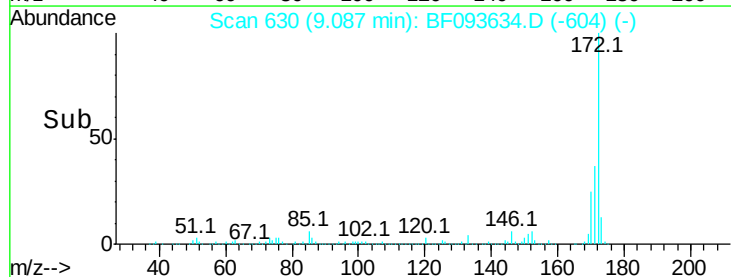
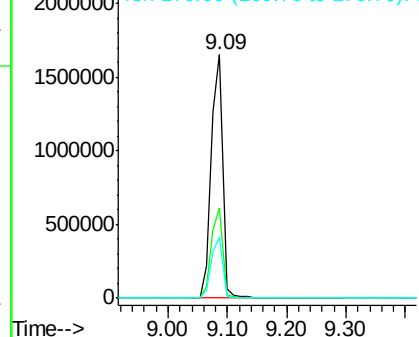


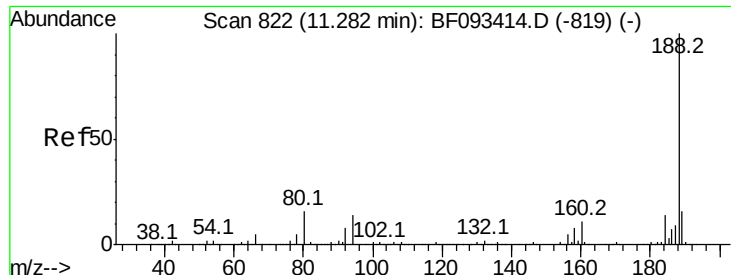

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.25 min Scan# 819
Delta R.T. -0.00 min
Lab File: BF093634.D
Acq: 14 Mar 2017 3:53




Instrument :
BNA_F
ClientSampleID :
D-103


Tot Ion	Ratio	Lower	Upper
188	100		
94	11.9	10.0	15.0
80	12.8	11.2	16.8

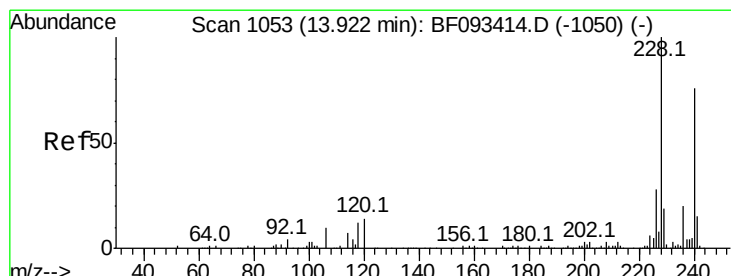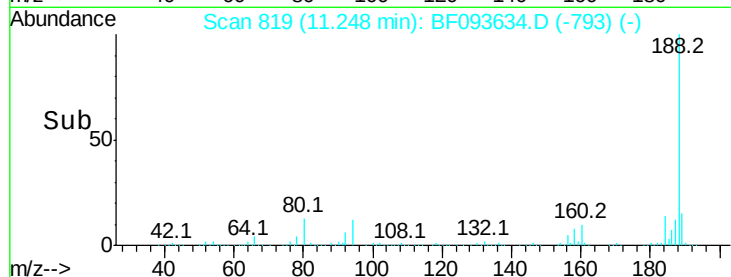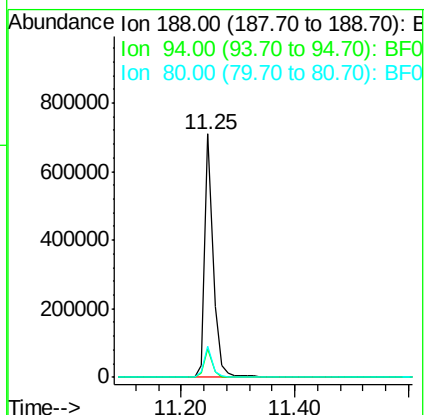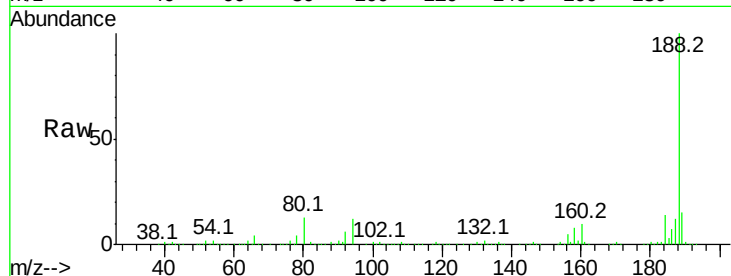

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.90 min Scan# 1051
Delta R.T. 0.01 min
Lab File: BF093634.D
Acq: 14 Mar 2017 3:53

Tgt Ion	Ratio	Lower	Upper
240	100		
120	10.8	12.9	19.3#
236	26.9	20.9	31.3

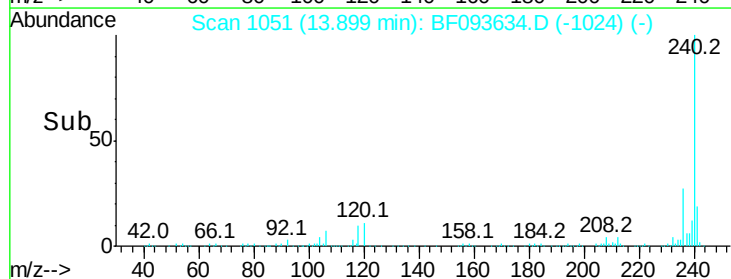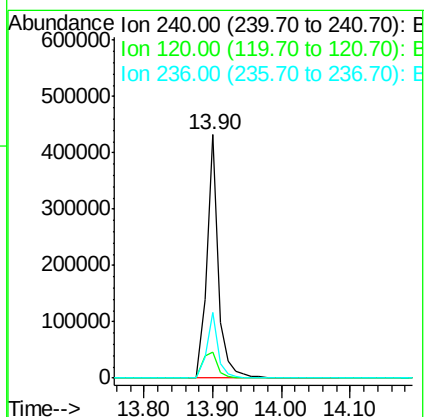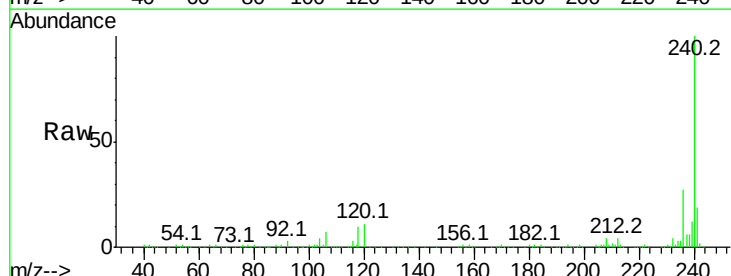

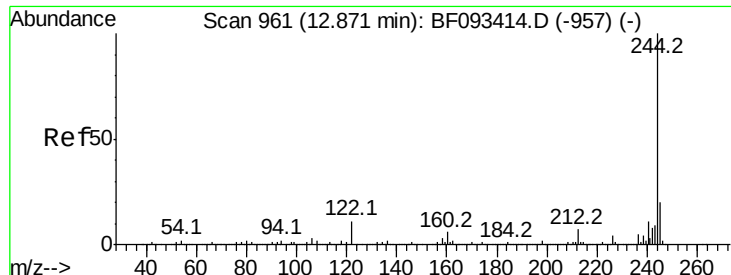

#78

Terphenyl-d14

Concen: 95.50 ng

RT: 12.84 min Scan# 958

Delta R.T. 0.01 min

Lab File: BF093634.D

Acq: 14 Mar 2017 3:53

Instrument :

BNA_F

ClientSampleId :

D-103


Tot Ion:244 Resp: 1846818

Ion Ratio Lower Upper

244 100

212 8.0 6.2 9.2




122 12.5 11.4 17.2

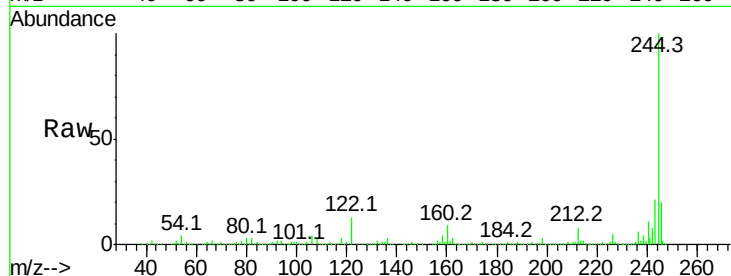

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

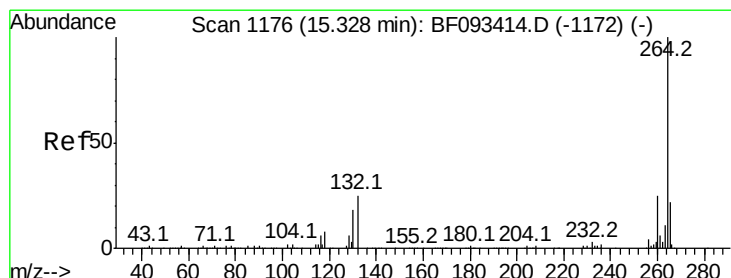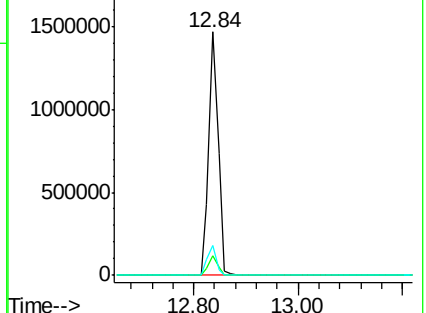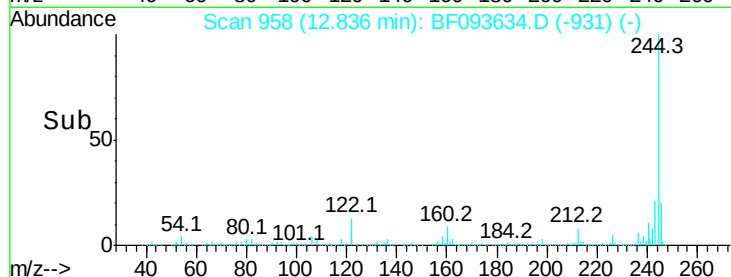

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.32 min Scan# 1175

Delta R.T. 0.03 min

Lab File: BF093634.D

Acq: 14 Mar 2017 3:53


Tgt Ion:264 Resp: 96939

Ion Ratio Lower Upper

264 100

260 36.6 19.2 28.8#

265 20.9 17.4 26.0

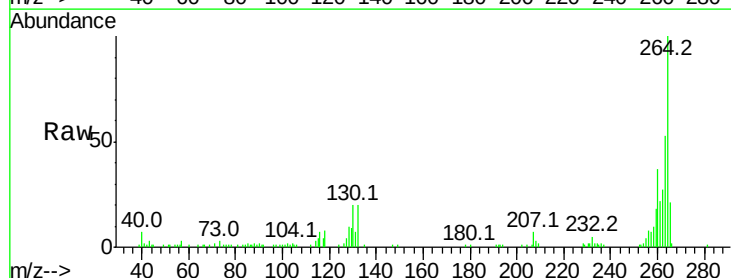

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

