

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031317\
 Data File : BF093648.D
 Acq On : 14 Mar 2017 10:19
 Operator : SJ/MA
 Sample : I2201-24
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 D-127

Quant Time: Mar 15 03:24:36 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 13 15:05:08 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.71	152	189014	20.00	ng	-0.01
21) Naphthalene-d8	8.00	136	767261	20.00	ng	-0.01
38) Acenaphthene-d10	9.75	164	366565	20.00	ng	-0.01
63) Phenanthrene-d10	11.25	188	688209	20.00	ng	0.00
75) Chrysene-d12	13.90	240	570180	20.00	ng	0.01
86) Perylene-d12	15.29	264	400597	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	1672642	147.28	ng	0.00
7) Phenol-d6	6.37	99	2076048	144.96	ng	-0.01
23) Nitrobenzene-d5	7.28	82	1343640	97.17	ng	-0.02
41) 2,4,6-Tribromophenol	10.56	330	401060	167.93	ng	0.01
44) 2-Fluorobiphenyl	9.08	172	2079761	105.53	ng	-0.01
78) Terphenyl-d14	12.84	244	1690795	77.10	ng	0.01


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031317\
Data File : BF093648.D
Acq On : 14 Mar 2017 10:19
Operator : SJ/MA
Sample : I2201-24
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
D-127

Quant Time: Mar 15 03:24:36 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 13 15:05:08 2017
Response via : Initial Calibration

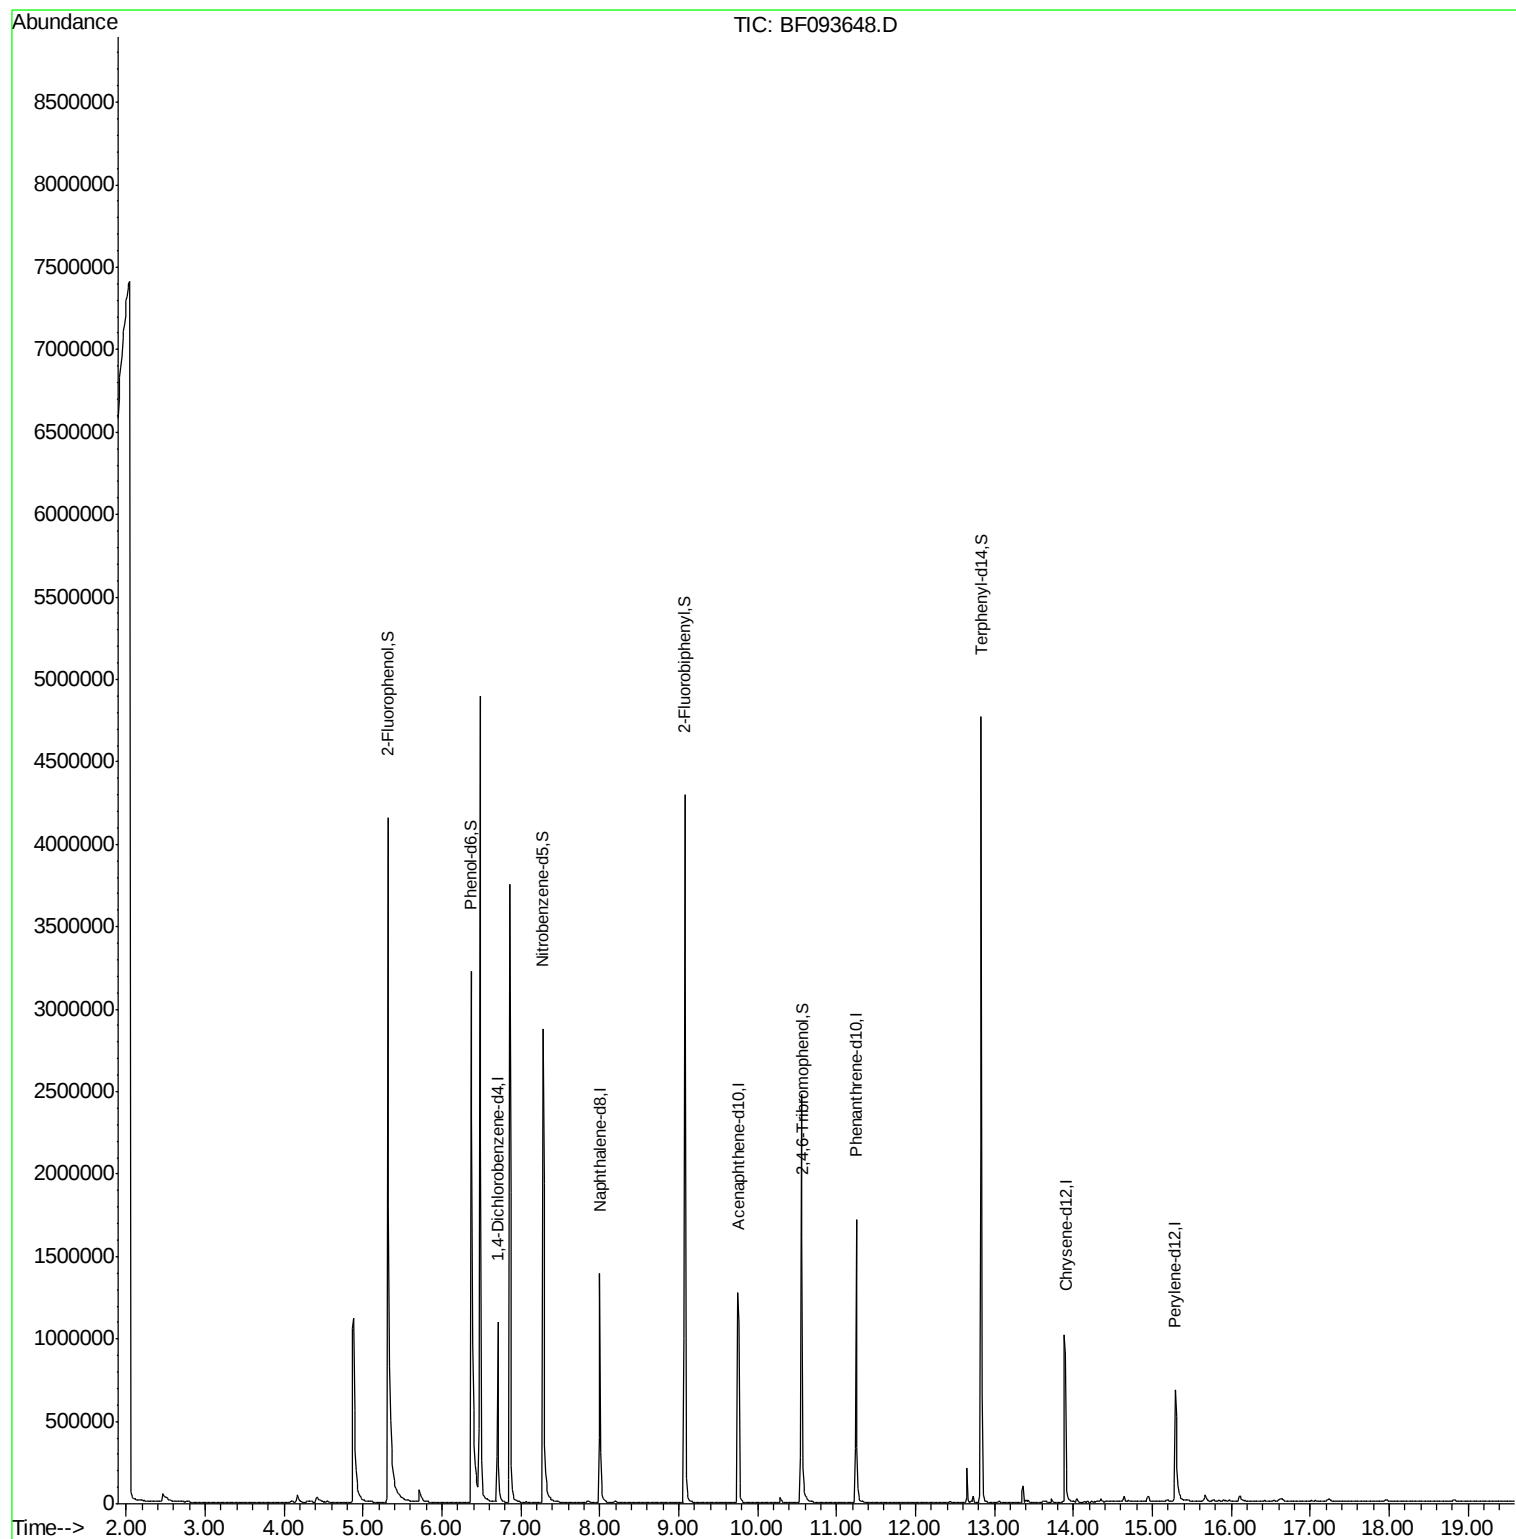

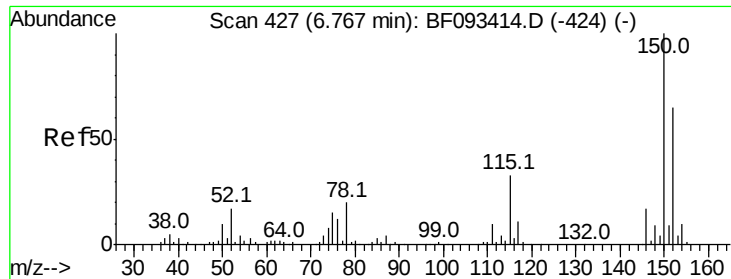


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.71 min Scan# 422
 Delta R.T. -0.01 min
 Lab File: BF093648.D
 Acq: 14 Mar 2017 10:19

Instrument :
 BNA_F
 ClientSampleId :
 D-127

Tot Ion:152 Resp: 189014
 Ion Ratio Lower Upper
 152 100
 150 152.7 124.9 187.3
 115 56.3 46.0 69.0

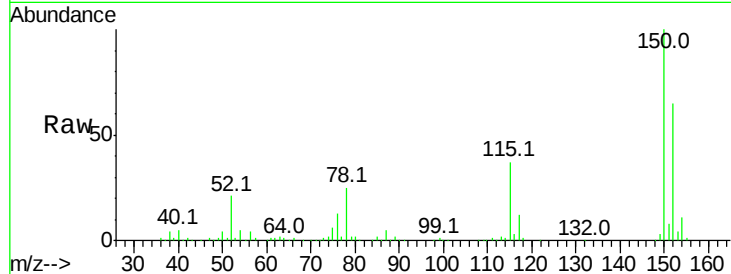


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

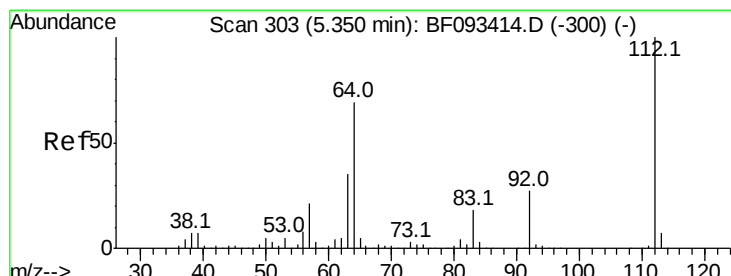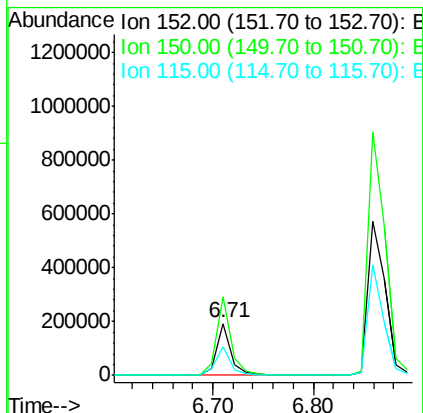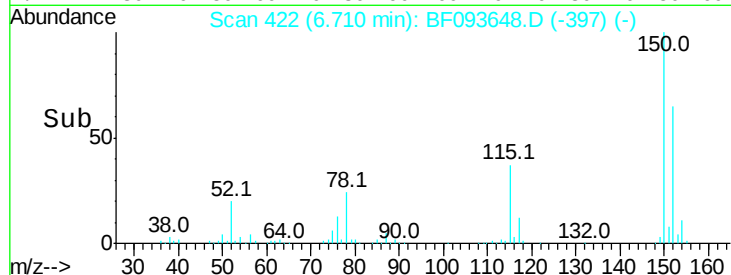



#5


2-Fluorophenol
 Concen: 147.28 ng
 RT: 5.32 min Scan# 300
 Delta R.T. 0.00 min
 Lab File: BF093648.D
 Acq: 14 Mar 2017 10:19

Tgt Ion:112 Resp: 1672642
 Ion Ratio Lower Upper
 112 100
 64 67.9 46.1 69.1
 63 34.3 23.8 35.6

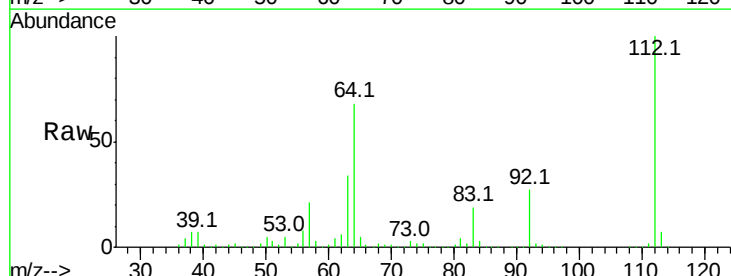

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

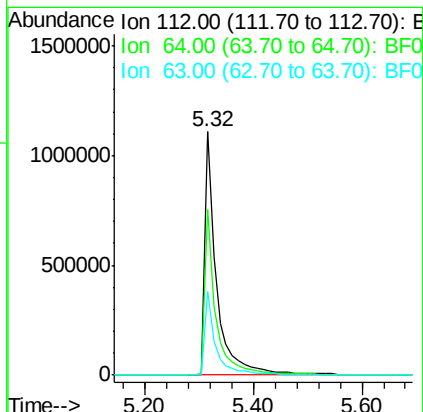

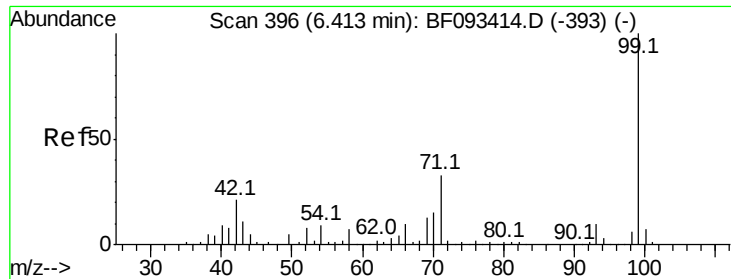

#7

Phenol-d6

Concen: 144.96 ng

RT: 6.37 min Scan# 392

Delta R.T. -0.01 min

Lab File: BF093648.D

Acq: 14 Mar 2017 10:19

Instrument :

BNA_F

ClientSampled :

D-127


Tot Ion: 99 Resp: 2076048

Ion Ratio Lower Upper




99 100

42 22.6 15.6 23.4

71 34.7 27.5 41.3

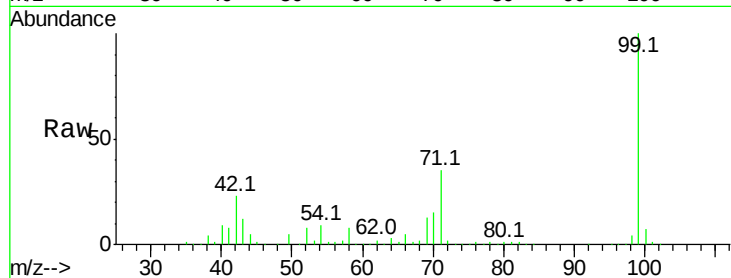

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

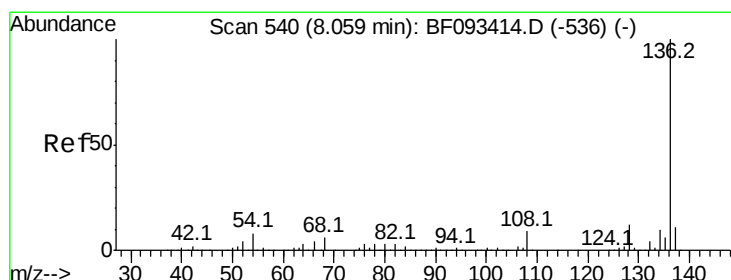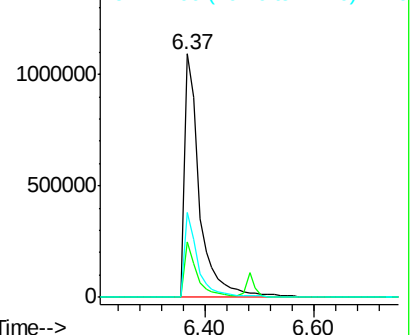

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.00 min Scan# 535

Delta R.T. -0.01 min

Lab File: BF093648.D

Acq: 14 Mar 2017 10:19

Tgt Ion: 136 Resp: 767261


Ion Ratio Lower Upper

136 100



137 10.6 8.4 12.6

54 8.8 4.5 6.7#

68 6.6 3.6 5.4#

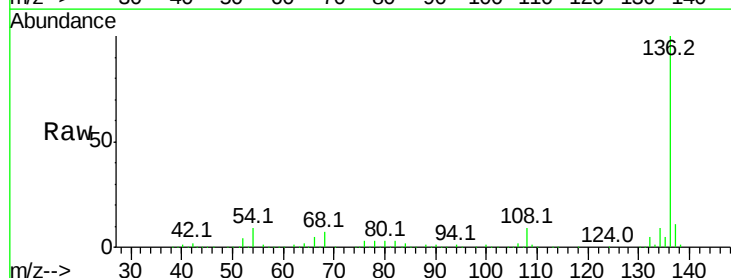

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

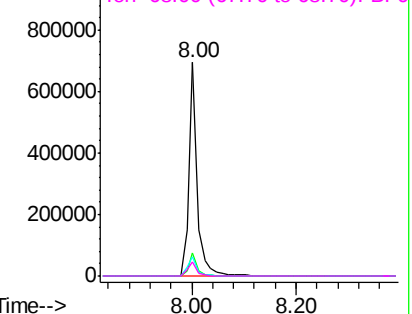






#23
 Nitrobenzene-d5
 Concen: 97.17 ng
 RT: 7.28 min Scan# 472
 Delta R.T. -0.02 min
 Lab File: BF093648.D
 Acq: 14 Mar 2017 10:19

Instrument :
 BNA_F
 ClientSampleId :
 D-127

Tot Ion: 82 Resp: 1343640
 Ion Ratio Lower Upper
 82 100
 128 37.7 34.6 52.0
 54 60.4 39.5 59.3#

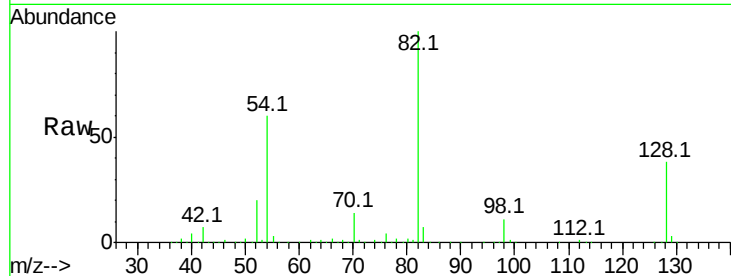


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

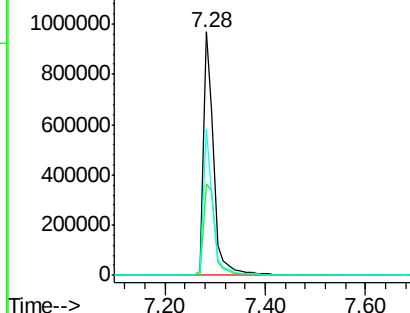




#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.75 min Scan# 688
 Delta R.T. -0.01 min
 Lab File: BF093648.D
 Acq: 14 Mar 2017 10:19

Tgt Ion:164 Resp: 366565
 Ion Ratio Lower Upper
 164 100
 162 103.0 80.2 120.2
 160 44.2 36.9 55.3

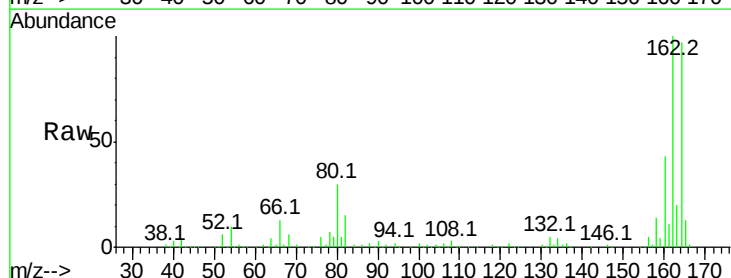

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

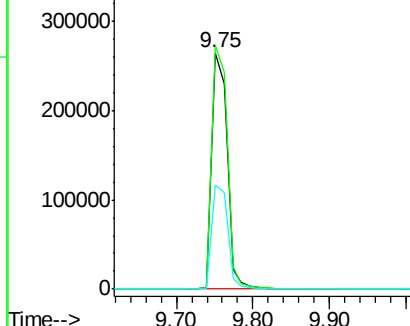







#41
 2,4,6-Tribromophenol
 Concen: 167.93 ng
 RT: 10.56 min Scan# 759
 Delta R.T. 0.01 min
 Lab File: BF093648.D
 Acq: 14 Mar 2017 10:19

Instrument :
 BNA_F
 ClientSampleId :
 D-127

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.0	77.4	116.2
141	36.9	34.1	51.1

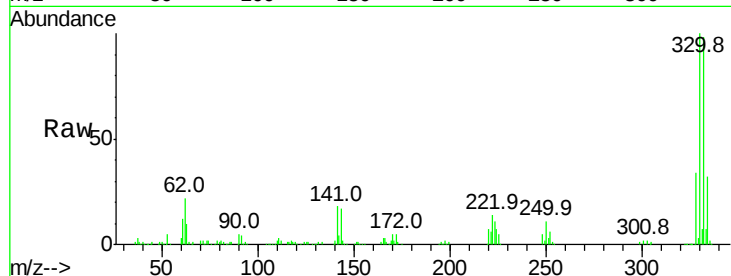


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

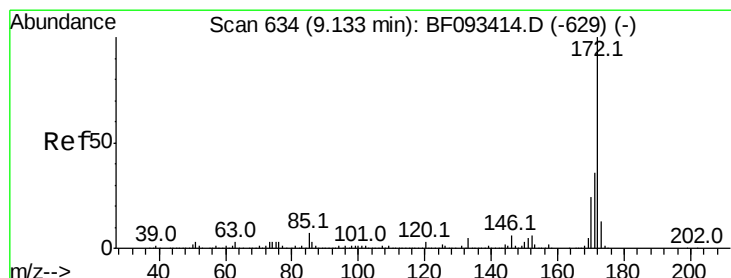
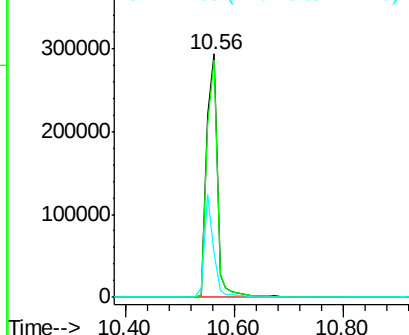



#44
 2-Fluorobiphenyl
 Concen: 105.53 ng
 RT: 9.08 min Scan# 629
 Delta R.T. -0.01 min
 Lab File: BF093648.D
 Acq: 14 Mar 2017 10:19

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.6	29.4	44.0
170	24.5	20.2	30.4

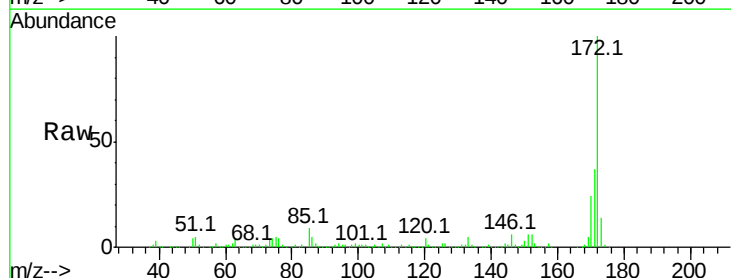

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



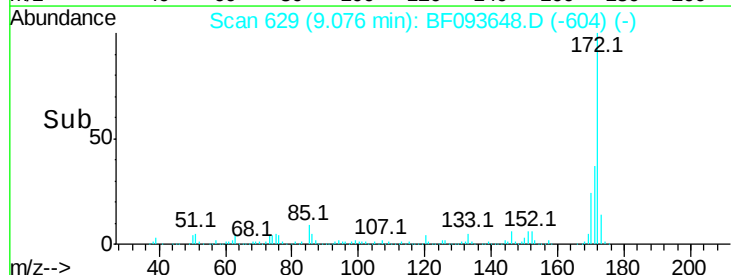
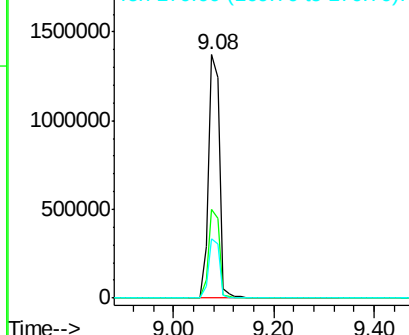




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.25 min Scan# 819
Delta R.T. 0.00 min
Lab File: BF093648.D
Acq: 14 Mar 2017 10:19




Instrument :
BNA_F
ClientSampleId :
D-127

Tot Ion:188 Resp: 688209
Ion Ratio Lower Upper
188 100
94 10.8 10.0 15.0
80 11.4 11.2 16.8

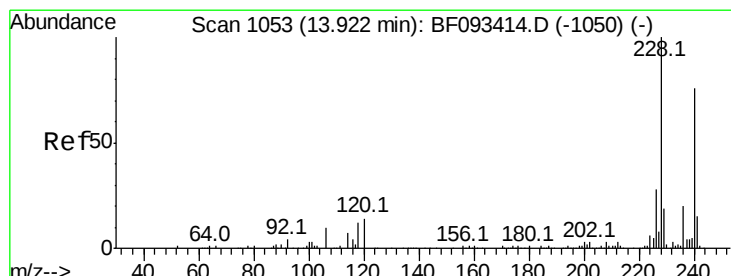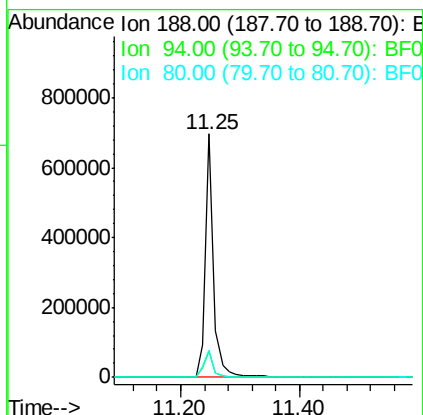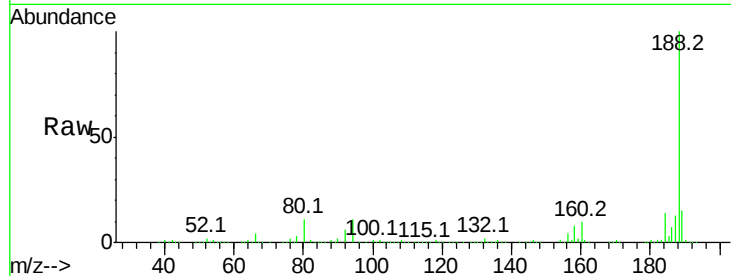

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.90 min Scan# 1051
Delta R.T. 0.01 min
Lab File: BF093648.D
Acq: 14 Mar 2017 10:19

Tgt Ion:240 Resp: 570180
Ion Ratio Lower Upper
240 100
120 9.8 12.9 19.3#
236 25.7 20.9 31.3

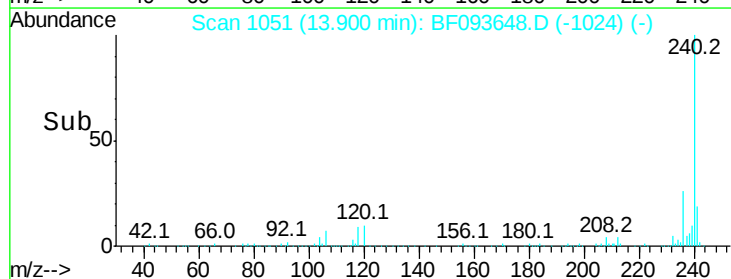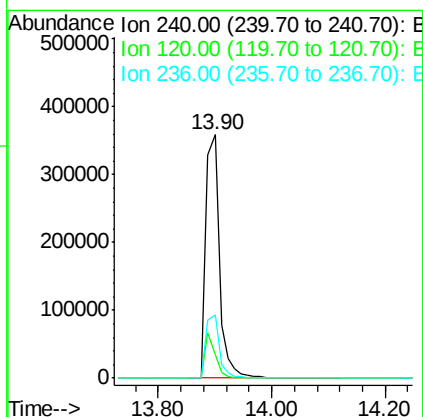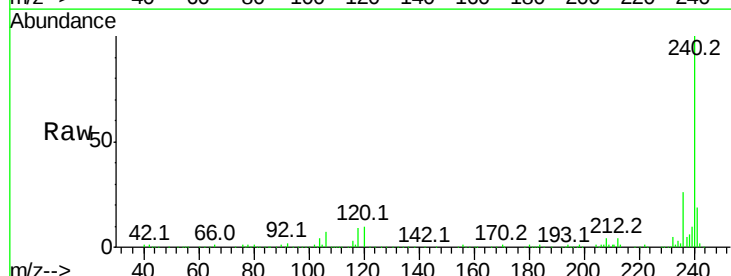



#78

Terphenyl-d14

Concen: 77.10 ng

RT: 12.84 min Scan# 958

Delta R.T. 0.01 min

Lab File: BF093648.D

Acq: 14 Mar 2017 10:19

Instrument :

BNA_F

ClientSampleId :

D-127


Tot Ion:244 Resp: 1690795

Ion Ratio Lower Upper

244 100

212 7.8 6.2 9.2




122 12.1 11.4 17.2

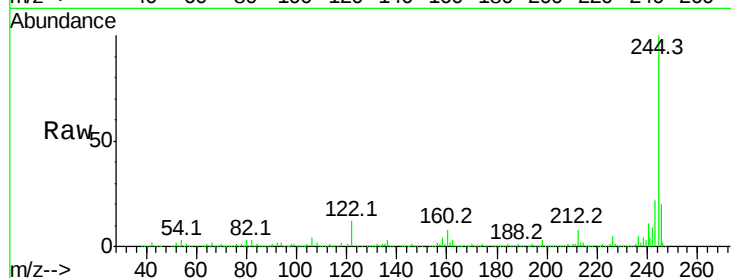

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

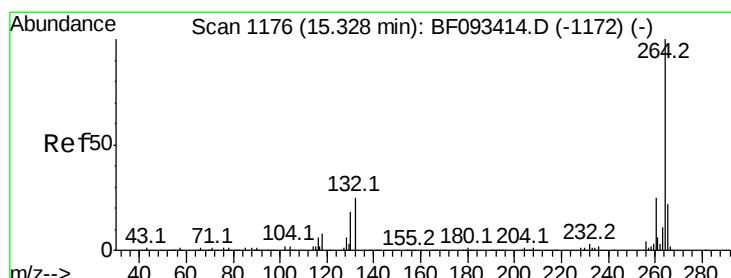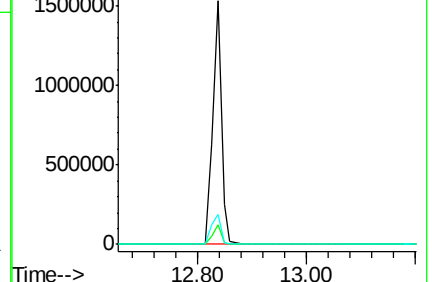

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.29 min Scan# 1173

Delta R.T. 0.01 min

Lab File: BF093648.D

Acq: 14 Mar 2017 10:19


Tgt Ion:264 Resp: 400597

Ion Ratio Lower Upper

264 100

260 24.1 19.2 28.8

265 21.6 17.4 26.0

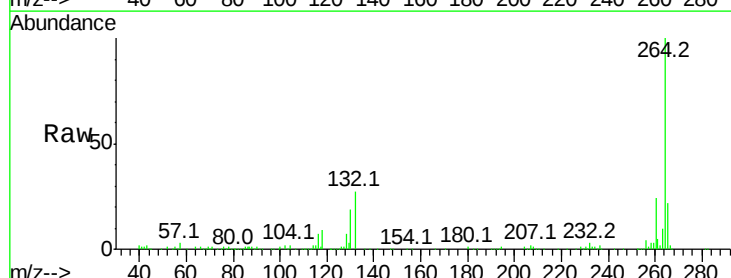

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

