


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031317\
 Data File : BF093624.D
 Acq On : 13 Mar 2017 23:18
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 13 15:05:08 2017

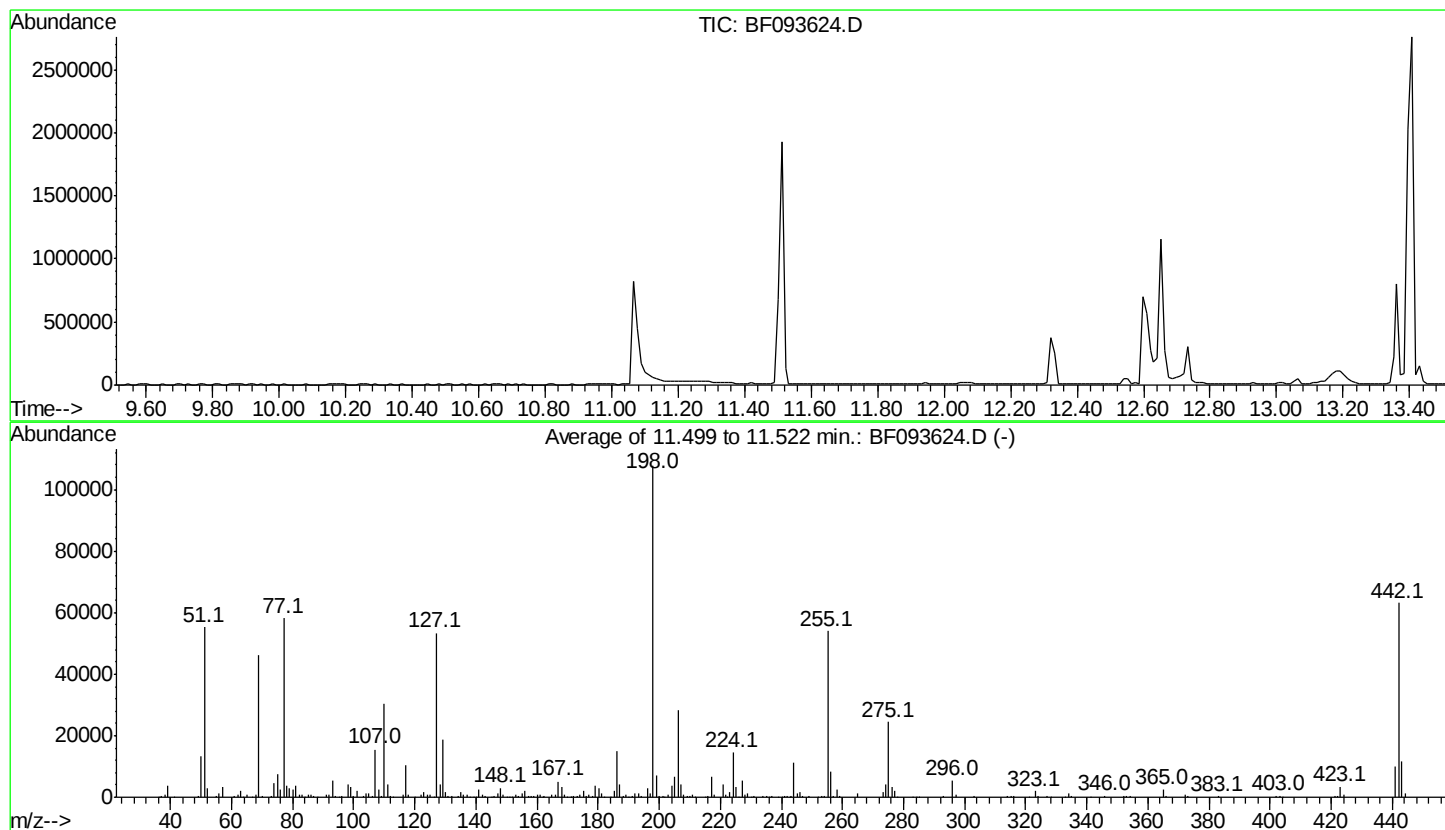

AutoFind: Scans 841, 842, 843; Background Corrected with Scan 837

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.2	55180	PASS
68	69	0.00	2	1.8	828	PASS
69	198	0.00	100	42.8	46171	PASS
70	69	0.00	2	0.6	273	PASS
127	198	10	80	49.5	53382	PASS
197	198	0.00	2	1.0	1096	PASS
198	198	100	100	100.0	107786	PASS
199	198	5	9	6.7	7177	PASS
275	198	10	60	22.7	24415	PASS
365	198	1	100	2.1	2314	PASS
441	442	0.01	24	15.9	10020	PASS
442	198	50	100	58.5	63093	PASS
443	442	15	24	18.4	11582	PASS