


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031317\
 Data File : BF093649.D
 Acq On : 14 Mar 2017 10:47
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 13 15:05:08 2017

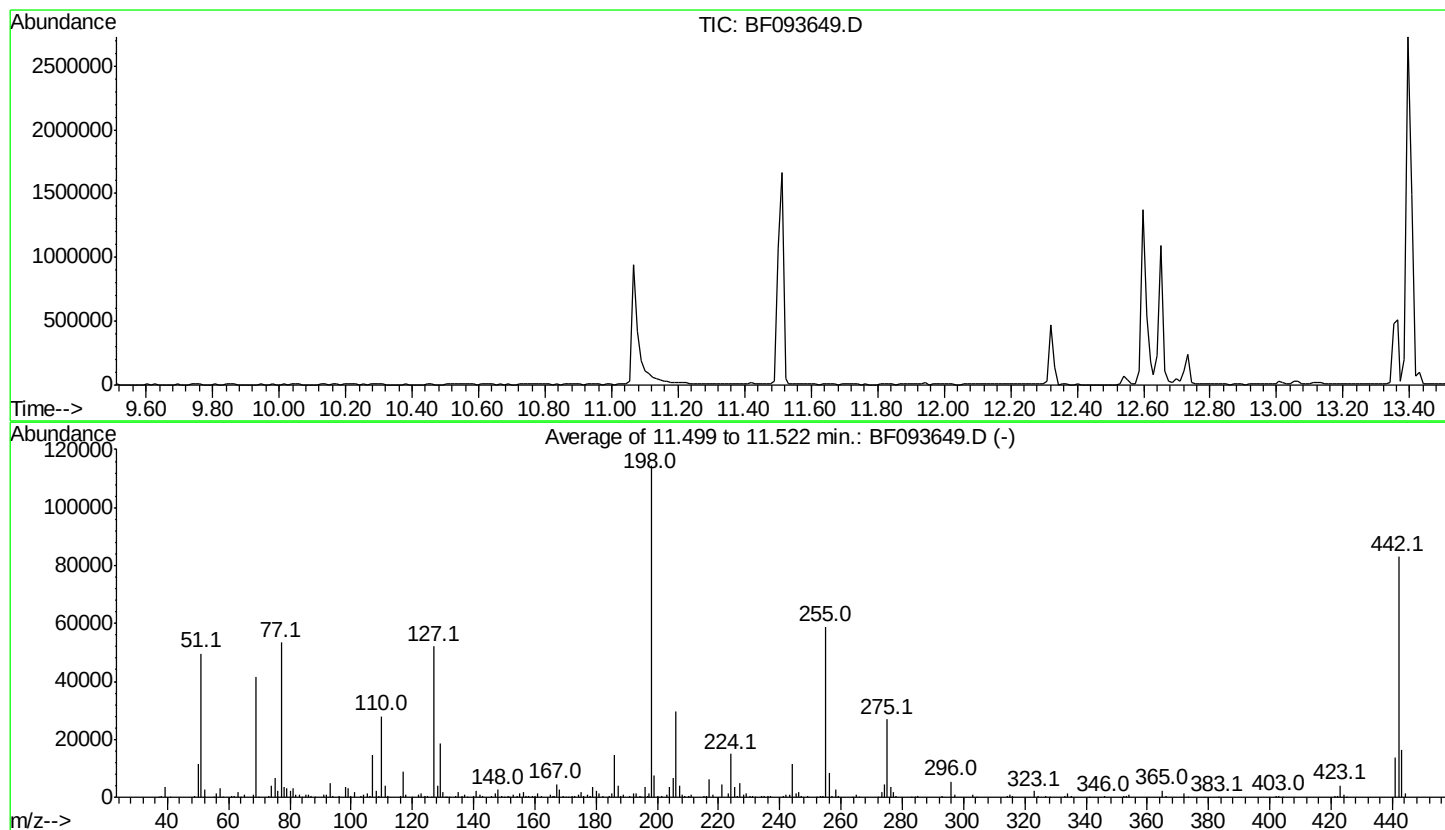

AutoFind: Scans 841, 842, 843; Background Corrected with Scan 837

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.3	49534	PASS
68	69	0.00	2	1.7	717	PASS
69	198	0.00	100	36.2	41470	PASS
70	69	0.00	2	0.3	125	PASS
127	198	10	80	45.4	51998	PASS
197	198	0.00	2	1.1	1229	PASS
198	198	100	100	100.0	114472	PASS
199	198	5	9	6.8	7740	PASS
275	198	10	60	23.5	26954	PASS
365	198	1	100	2.1	2396	PASS
441	442	0.01	24	16.4	13581	PASS
442	198	50	100	72.4	82877	PASS
443	442	15	24	19.6	16244	PASS