
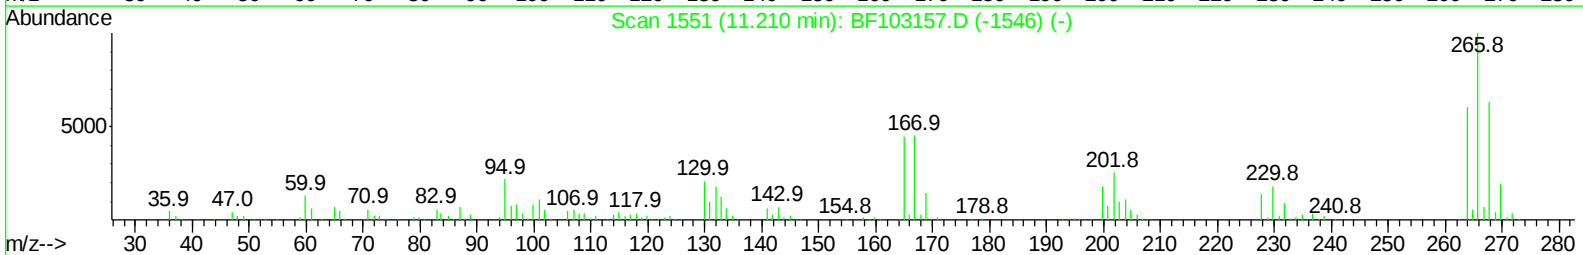
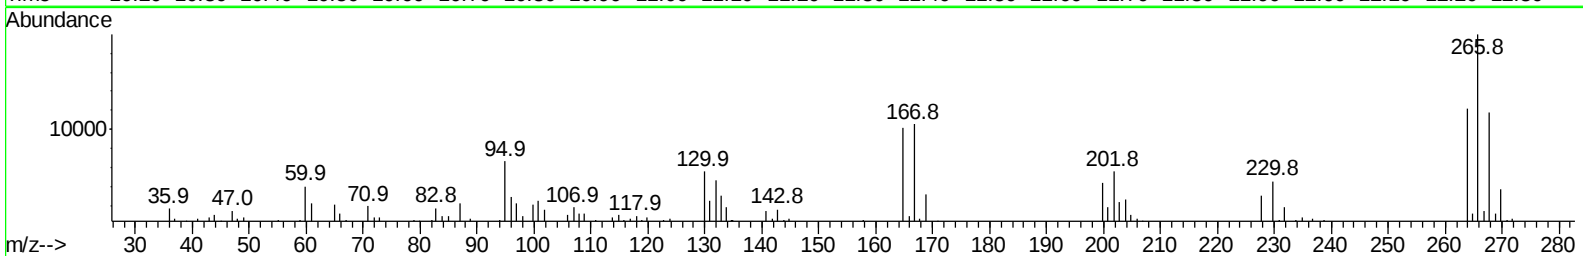


Data Path : Z:\HPCHEM1\BNA F\DATA\BF031318\
Data File : BF103596.D
Acq On : 13 Mar 2018 11:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 05:14:16 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 09 11:47:13 2018
Response via : Initial Calibration

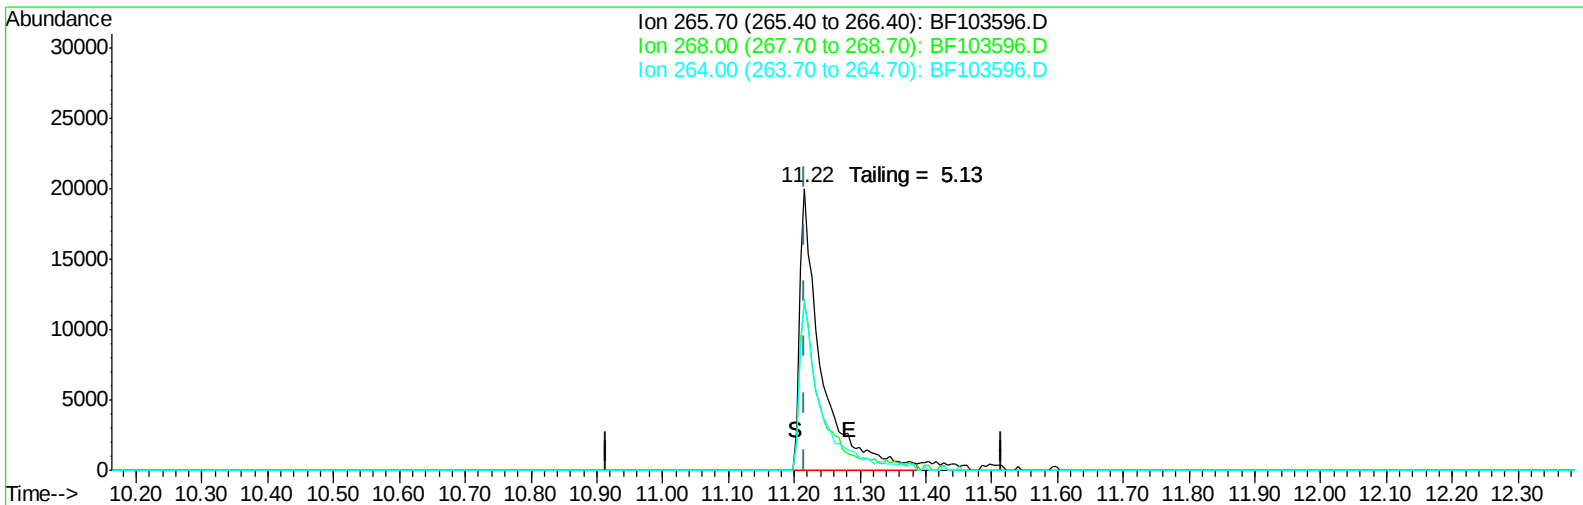

TIC: BF103596.D

(69) Pentachlorophenol (C)




11.216min (+0.000) 70968.82ng

response 45394

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.99
264.00	61.90	60.88
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031318\
Data File : BF103596.D
Acq On : 13 Mar 2018 11:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 05:14:16 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 09 11:47:13 2018
Response via : Initial Calibration

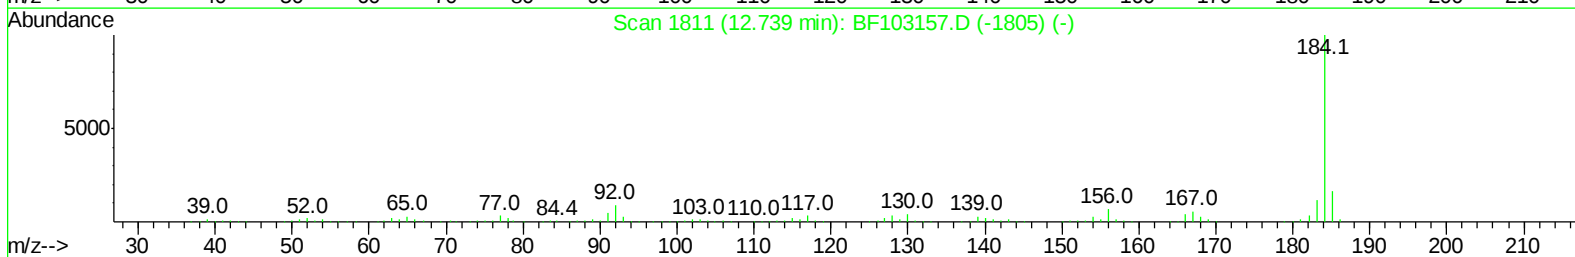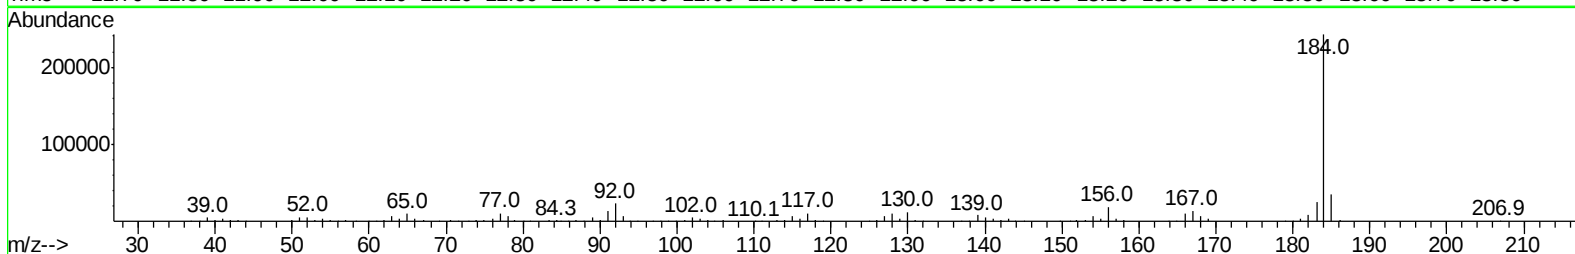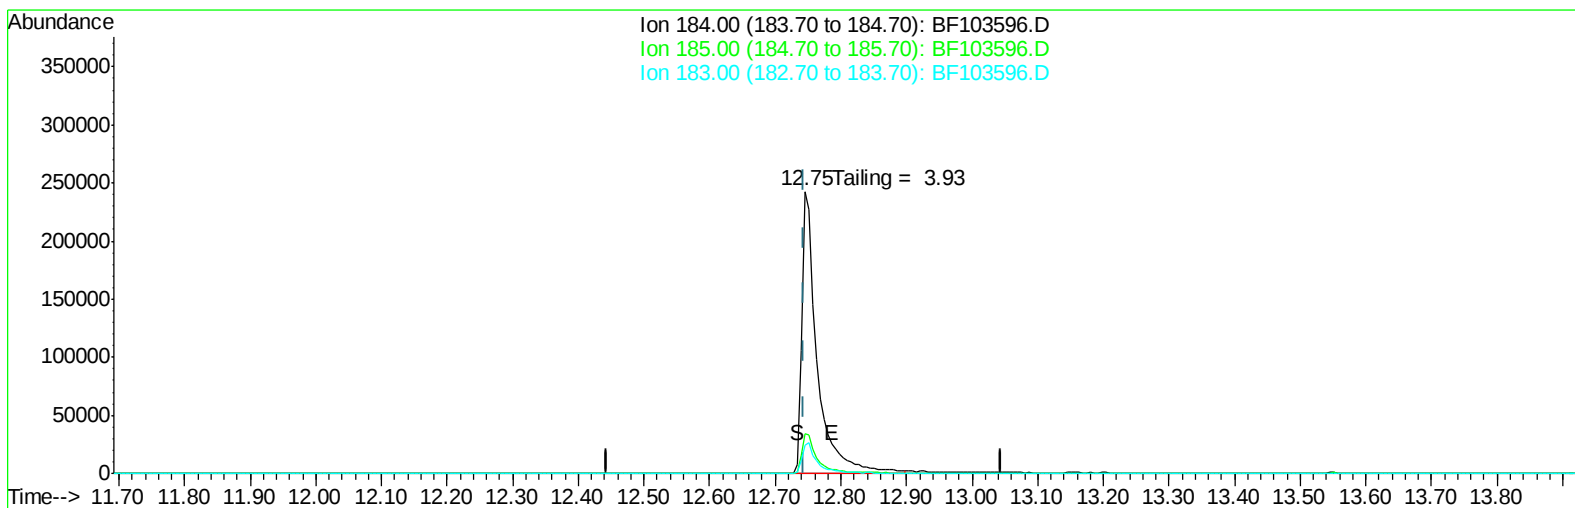

TIC: BF103596.D

(76) Benzidine

12.745min (+0.000) 0.00ng

response 400614

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.20
183.00	11.60	10.14
0.00	0.00	0.00