
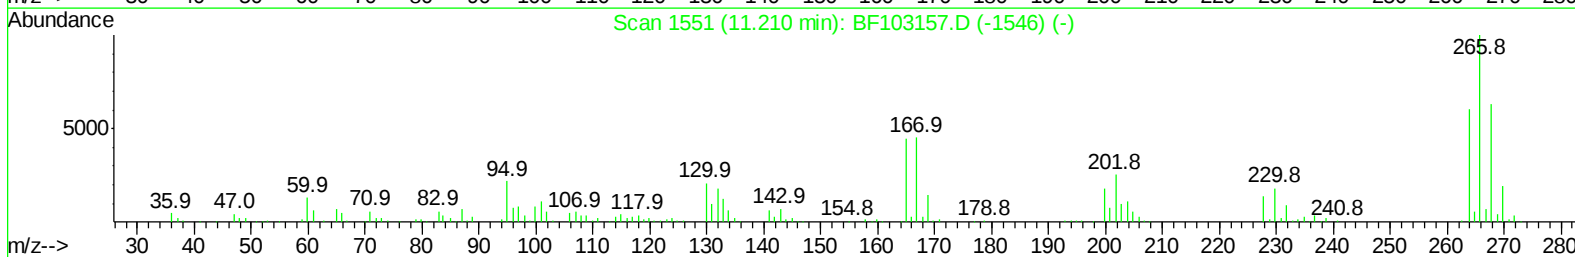
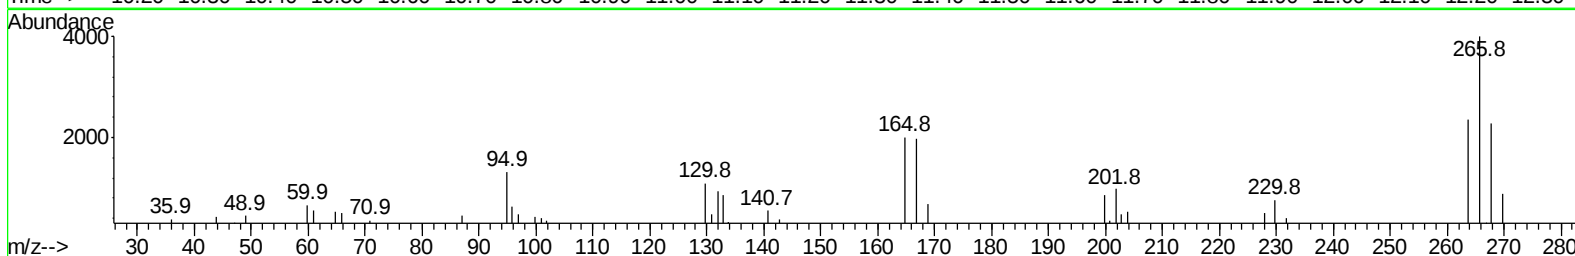


Data Path : Z:\HPCHEM1\BNA F\DATA\BF031318\
Data File : BF103622.D
Acq On : 14 Mar 2018 00:09
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 05:15:30 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 09 11:47:13 2018
Response via : Initial Calibration

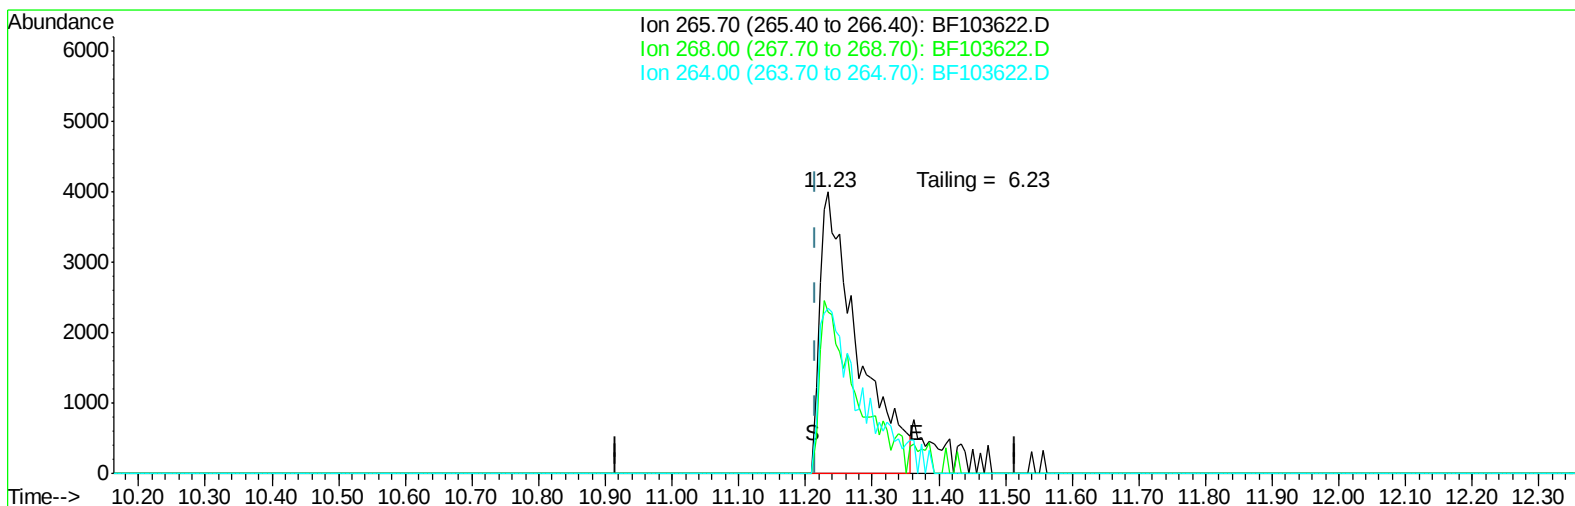

TIC: BF103622.D

(69) Pentachlorophenol (C)




11.233min (+0.018) 26279.13ng

response 15947

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.16
264.00	61.90	58.71
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031318\
 Data File : BF103622.D
 Acq On : 14 Mar 2018 00:09
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 05:15:30 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 09 11:47:13 2018
 Response via : Initial Calibration

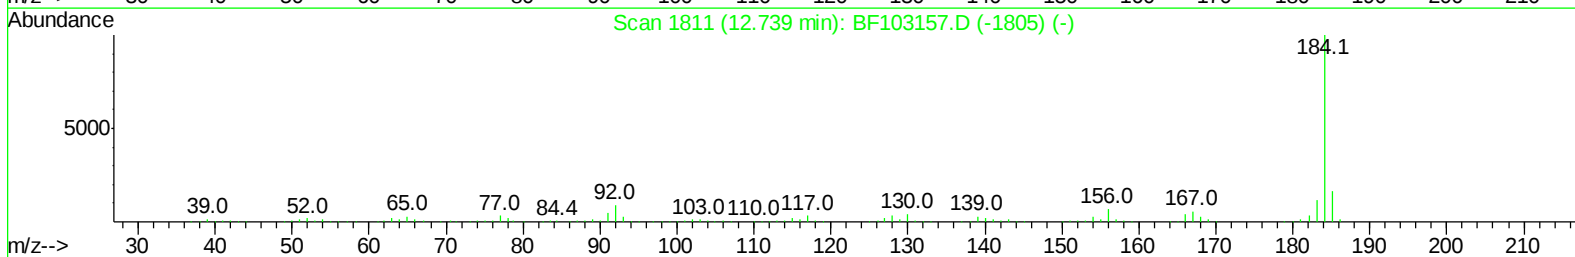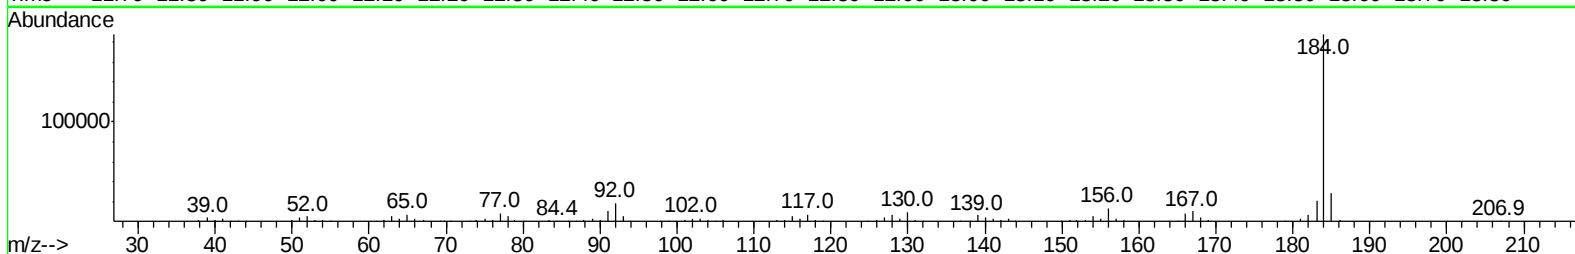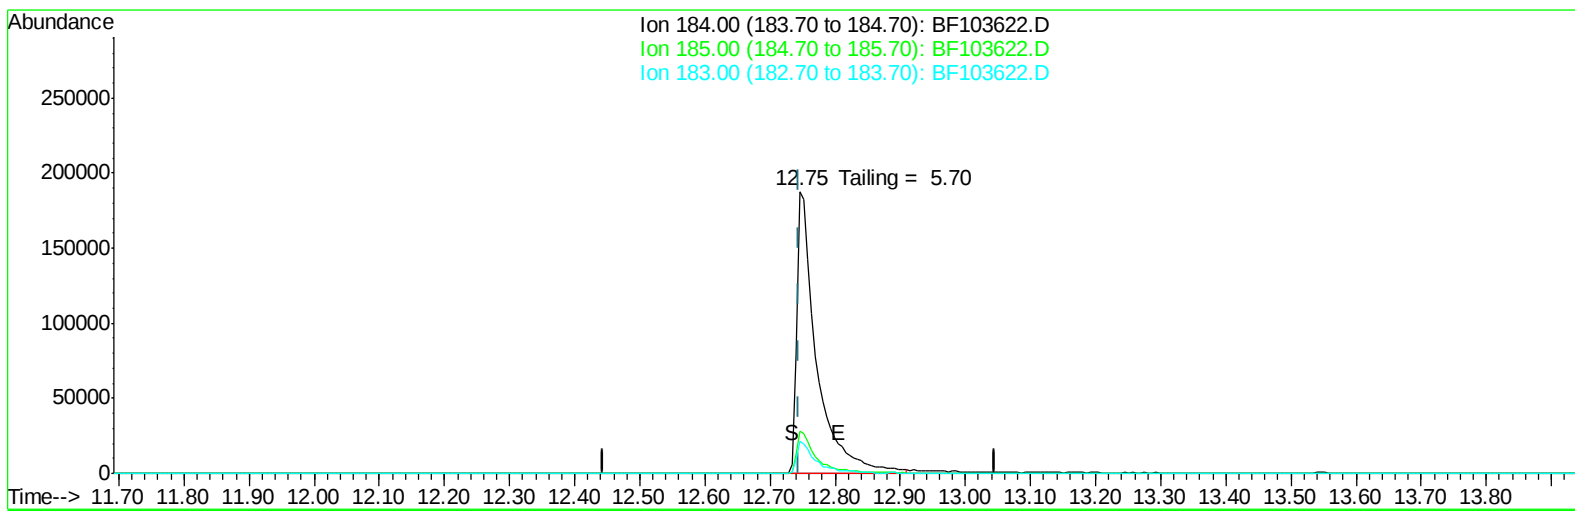

TIC: BF103622.D

(76) Benzidine

12.745min (+0.000) 0.00ng

response 398917

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.91
183.00	11.60	11.18
0.00	0.00	0.00