


Data Path : Z:\HPCHEM1\BNA F\Data\BF031318\
Data File : BF103596.D
Acq On : 13 Mar 2018 11:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 09 11:47:13 2018

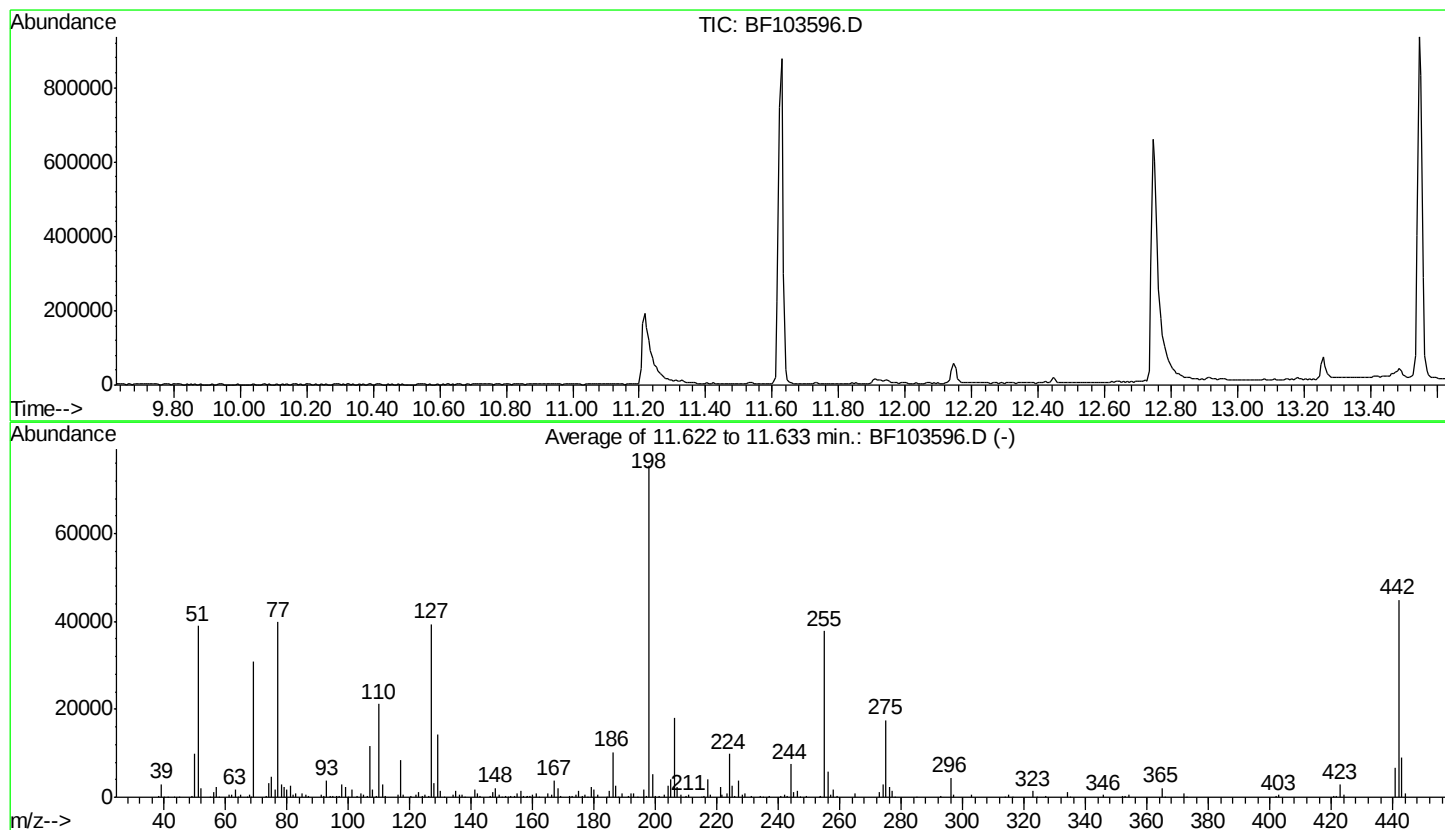

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.7	39016	PASS
68	69	0.00	2	1.5	473	PASS
69	198	0.00	100	41.1	30977	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.2	39398	PASS
197	198	0.00	2	0.6	432	PASS
198	198	100	100	100.0	75450	PASS
199	198	5	9	7.0	5268	PASS
275	198	10	60	23.2	17535	PASS
365	198	1	100	2.9	2180	PASS
441	443	0.01	100	76.2	6847	PASS
442	198	50	100	59.5	44882	PASS
443	442	15	24	20.0	8985	PASS