


Data Path : Z:\HPCHEM1\BNA_F\Data\BF031318\
Data File : BF103622.D
Acq On : 14 Mar 2018 00:09
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 09 11:47:13 2018

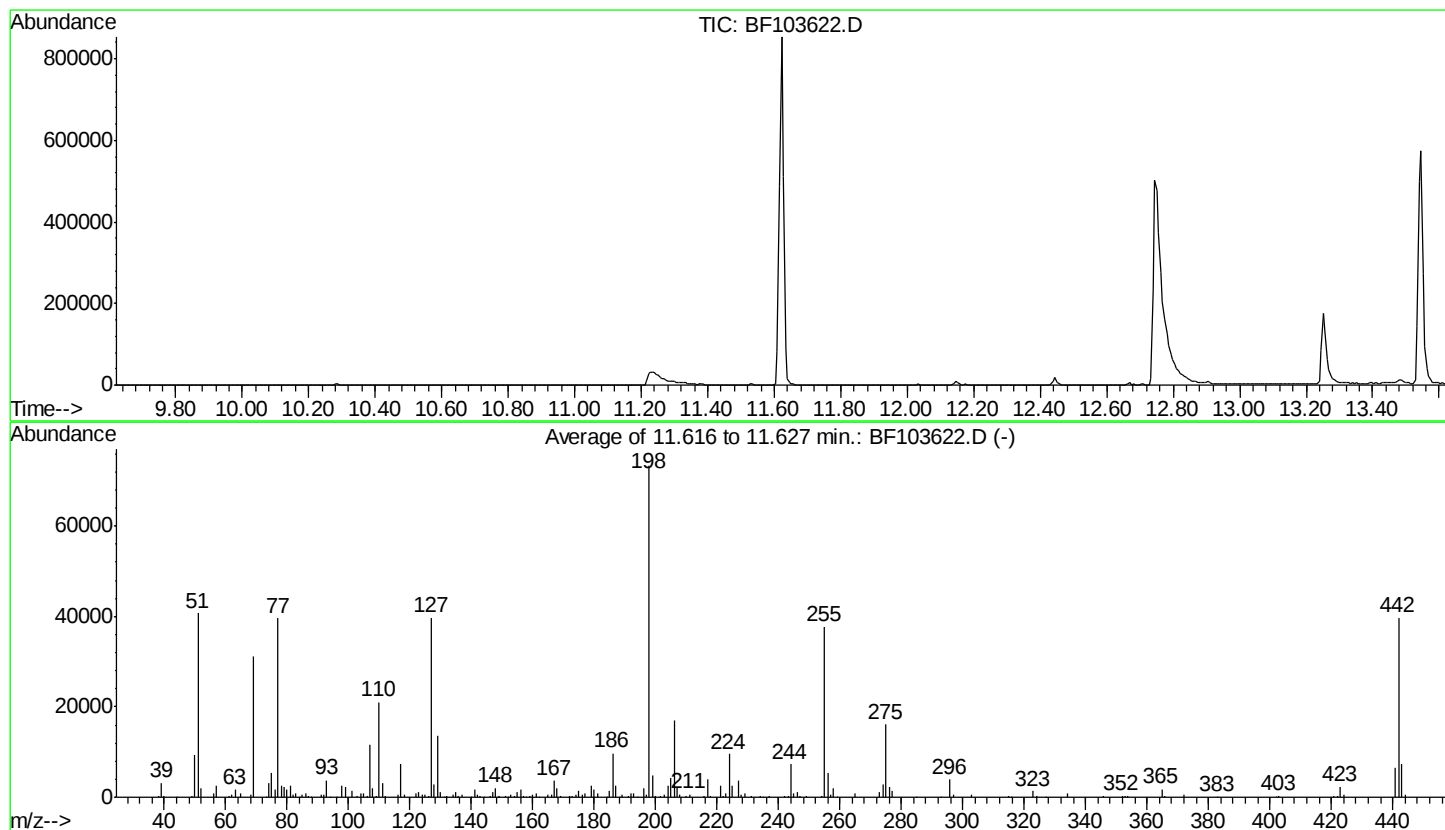

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.5	40752	PASS
68	69	0.00	2	1.8	564	PASS
69	198	0.00	100	42.3	31050	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.2	39749	PASS
197	198	0.00	2	0.8	597	PASS
198	198	100	100	100.0	73392	PASS
199	198	5	9	6.5	4760	PASS
275	198	10	60	22.0	16136	PASS
365	198	1	100	2.5	1829	PASS
441	443	0.01	100	89.3	6655	PASS
442	198	50	100	54.1	39695	PASS
443	442	15	24	18.8	7455	PASS