

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF031319\
 Data File : BF113043.D
 Acq On : 13 Mar 2019 22:42
 Operator : JU/SJ
 Sample : K1693-07 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Mar 14 02:03:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 13 03:42:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	154981	20.00	ng	0.00
21) Naphthalene-d8	8.01	136	666252	20.00	ng	0.00
39) Acenaphthene-d10	9.76	164	384965	20.00	ng	-0.01
64) Phenanthrene-d10	11.23	188	709186	20.00	ng	-0.01
76) Chrysene-d12	13.86	240	539976	20.00	ng	0.00
87) Perylene-d12	15.27	264	507580	20.00	ng	0.00

System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	167642	16.83	ng	-0.01
7) Phenol-d6	6.36	99	230596	18.43	ng	-0.01
23) Nitrobenzene-d5	7.28	82	131297	11.79	ng	-0.02
42) 2,4,6-Tribromophenol	10.54	330	96690	23.66	ng	-0.01
45) 2-Fluorobiphenyl	9.08	172	362899	11.57	ng	-0.01
79) Terphenyl-d14	12.82	244	392453	14.09	ng	0.00


Target Compounds				Qvalue		
19) n-Nitroso-di-n-propylamine	7.28	70	17211	2.171	ng	# 77
25) Isophorone	7.28	82	128284	5.348	ng	# 66
31) Naphthalene	8.03	128	232299	7.023	ng	# 98
33) 4-Chloroaniline	8.03	127	29592	2.112	ng	# 33
37) 2-Methylnaphthalene	8.72	142	275952	12.918	ng	# 98
38) 1-Methylnaphthalene	8.82	142	265881	12.849	ng	# 98
52) Acenaphthene	9.79	154	60761	2.496	ng	# 99
54) 2,4-Dinitrophenol	10.05	184	231	6.541	ng	# 23
58) Fluorene	10.30	166	187721	7.476	ng	# 97
65) 4,6-Dinitro-2-methylphenol	10.58	198	687	4.826	ng	# 1
71) Phenanthrene	11.26	178	835057	23.666	ng	# 99
72) Anthracene	11.31	178	177649	4.810	ng	# 97
75) Fluoranthene	12.45	202	782572	20.701	ng	# 96
78) Pyrene	12.67	202	981229	21.555	ng	# 99
81) Benzo(a)anthracene	13.85	228	368690	9.852	ng	# 93
83) Chrysene	13.85	228	368690	10.058	ng	# 97
88) Benzo(b)fluoranthene	14.87	252	442340	13.473	ng	# 98
89) Benzo(k)fluoranthene	14.87	252	442340	14.874	ng	# 98
90) Benzo(a)pyrene	15.21	252	274014	9.436	ng	# 96
92) Benzo(a,h,i)perylene	17.03	276	127673	5.131	ng	# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF031319\
Data File : BF113043.D
Acq On : 13 Mar 2019 22:42
Operator : JU/SJ
Sample : K1693-07 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Mar 14 02:03:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 13 03:42:55 2019
Response via : Initial Calibration

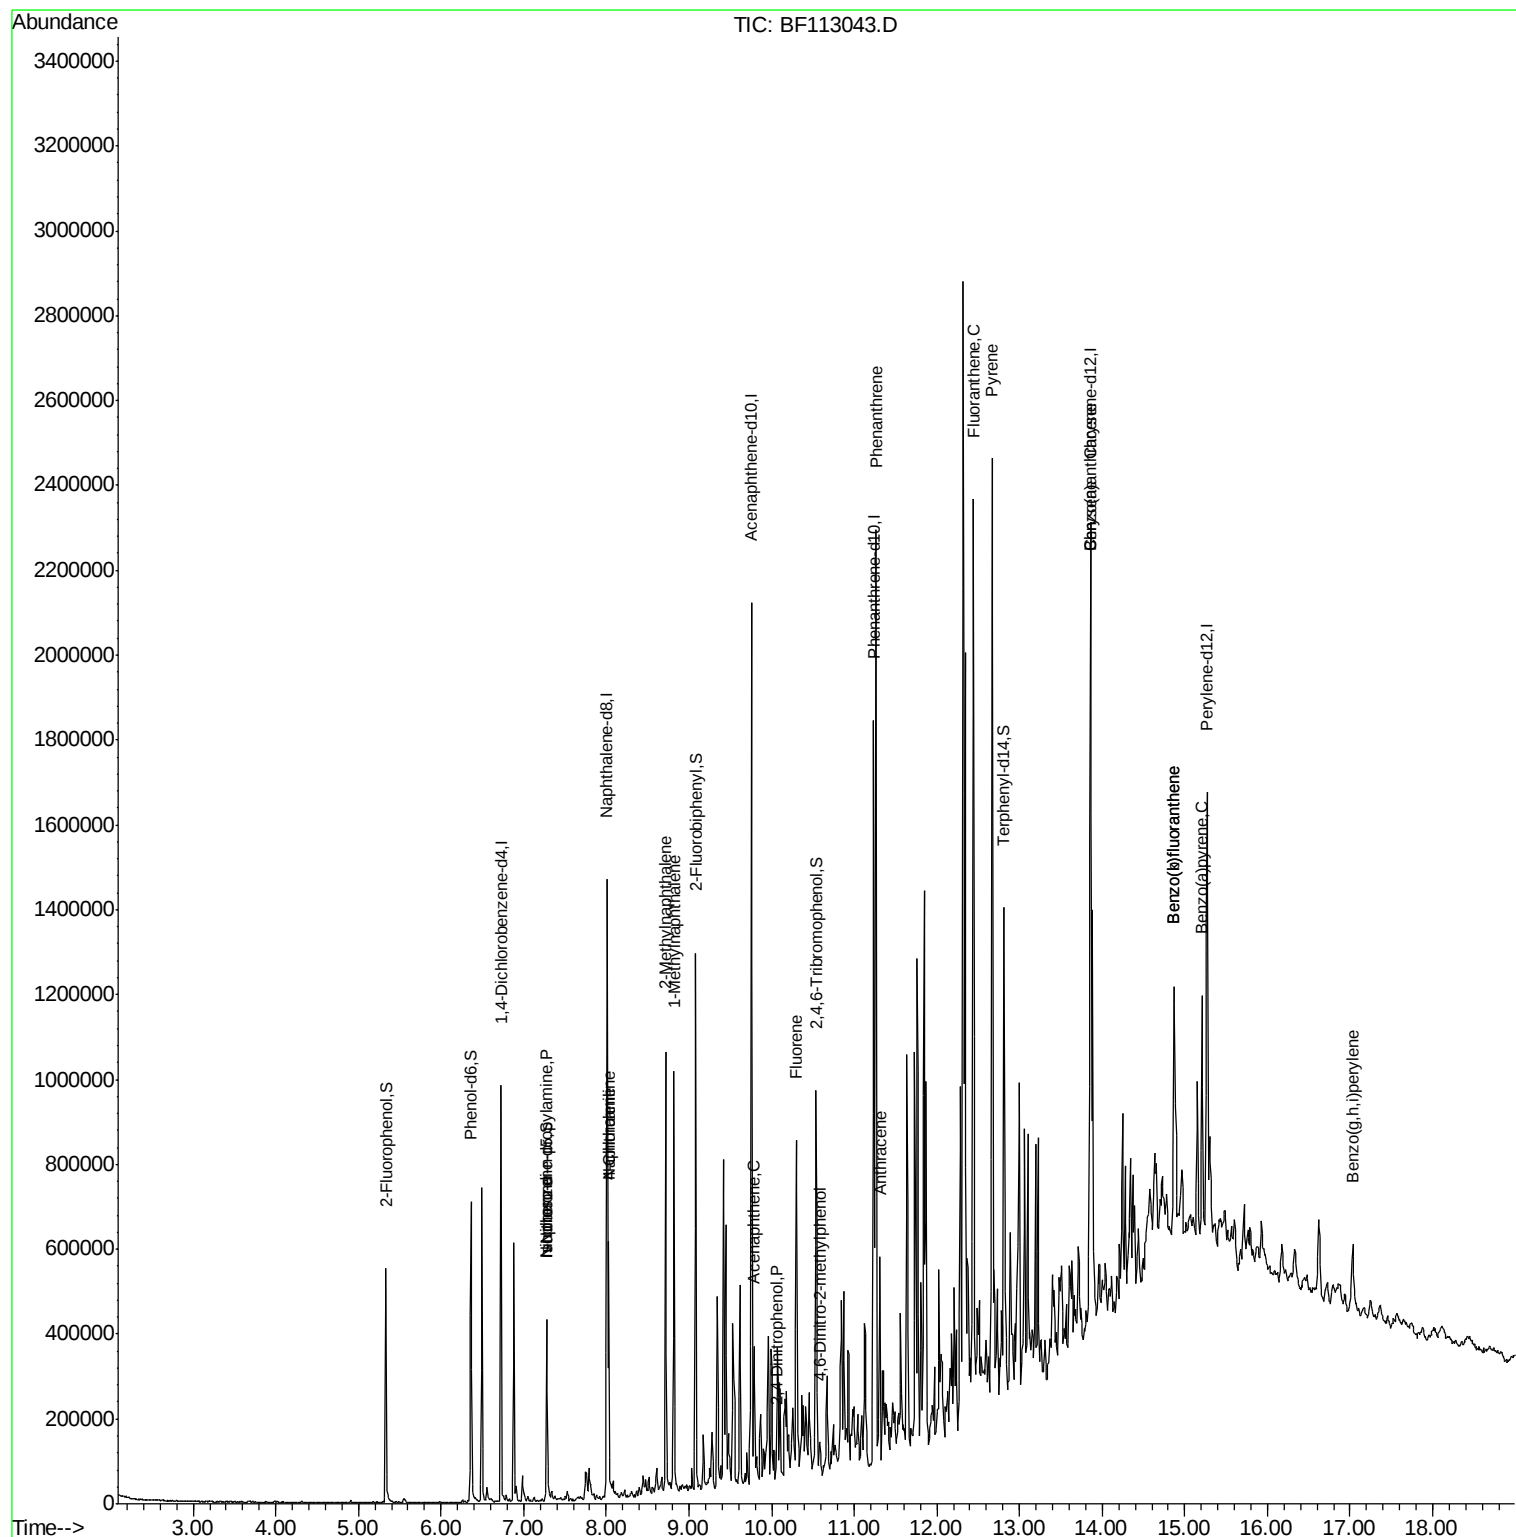




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 789
Delta R.T. -0.01 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 154981
Ion Ratio Lower Upper
152 100
150 154.5 124.2 186.2
115 55.4 48.2 72.4




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

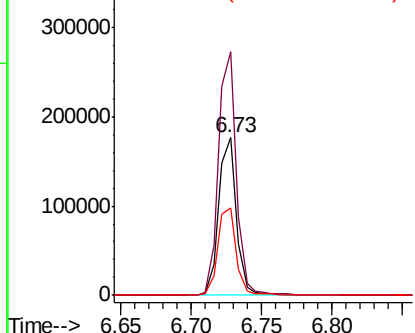



#5


2-Fluorophenol
Concen: 16.826 ng
RT: 5.33 min Scan# 552
Delta R.T. -0.01 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Tgt Ion:112 Resp: 167642
Ion Ratio Lower Upper
112 100
64 55.3 47.6 71.4
63 28.2 24.4 36.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

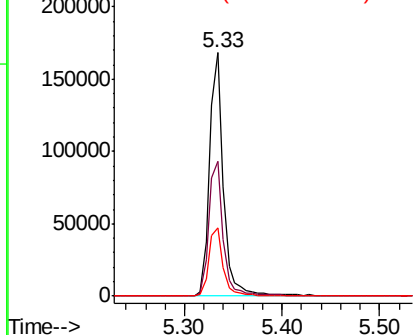

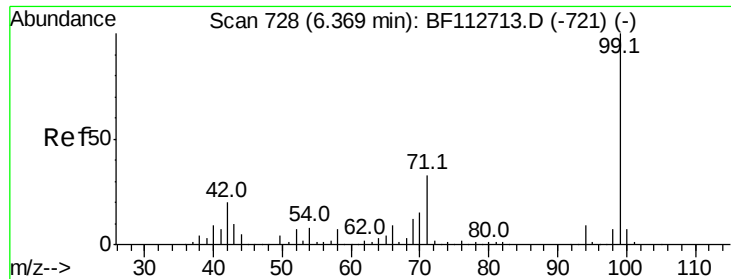

#7

Phenol-d6

Concen: 18.425 ng

RT: 6.36 min Scan# 727

Delta R.T. -0.01 min

Lab File: BF113043.D

Acq: 13 Mar 2019 22:42

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 230596

Ion Ratio Lower Upper

99 100

42 17.5 16.3 24.5




71 29.9 26.2 39.4



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

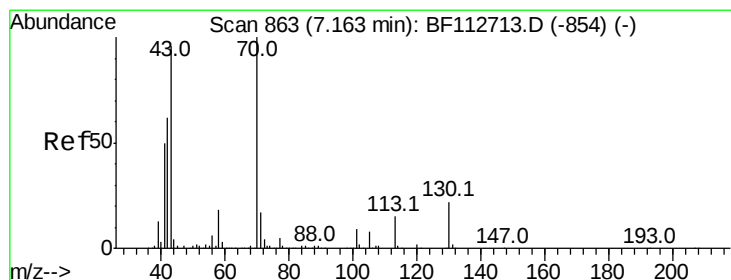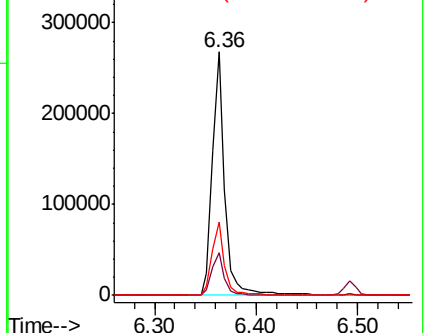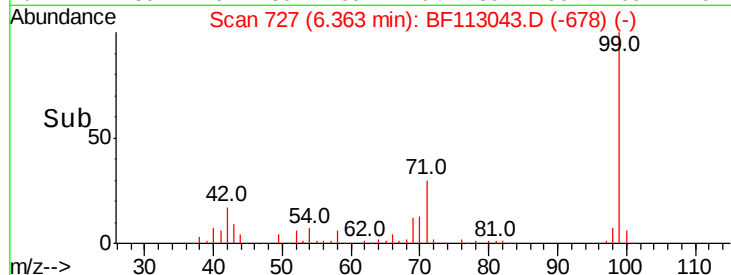

#19

n-Nitroso-di-n-propylamine

Concen: 2.171 ng

RT: 7.28 min Scan# 883

Delta R.T. 0.12 min

Lab File: BF113043.D

Acq: 13 Mar 2019 22:42

Tgt Ion: 70 Resp: 17211


Ion Ratio Lower Upper

70 100

42 49.8 49.9 74.9#

101 0.0 7.4 11.2#

130 3.1 17.4 26.2#






Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

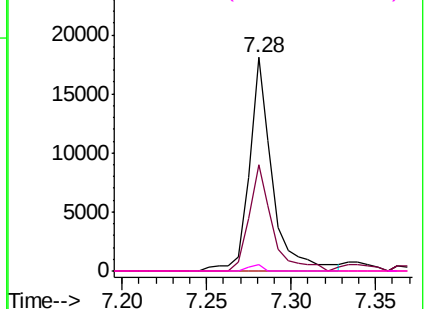


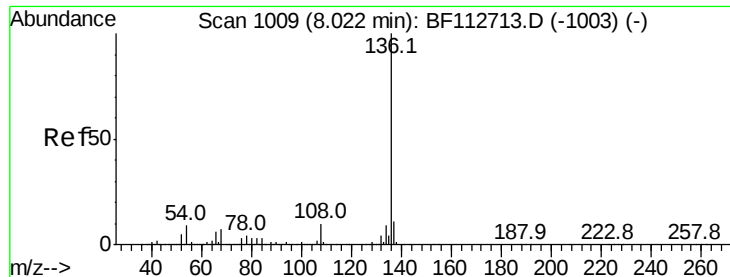




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.01 min Scan# 1007
Delta R.T. -0.01 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Instrument :
BNA_F
ClientSampleId :

Tot Ion:	136	Resp:	666252
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.9	13.3
54	7.5	7.3	10.9
68	5.7	5.4	8.2

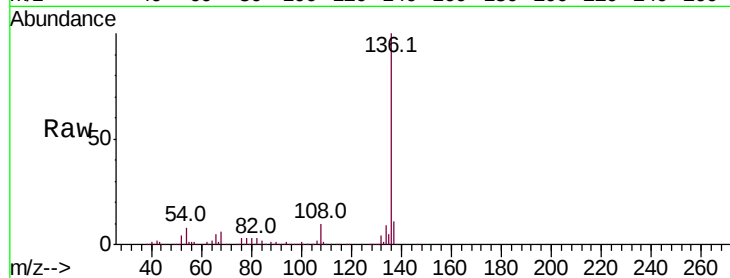


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

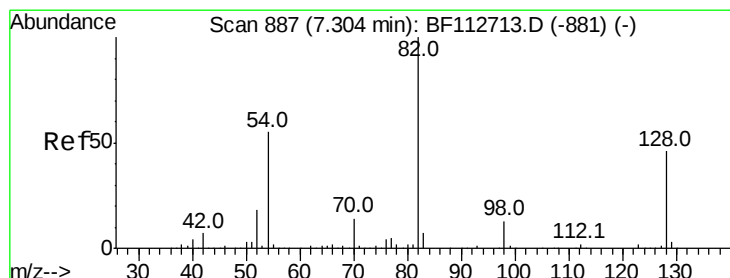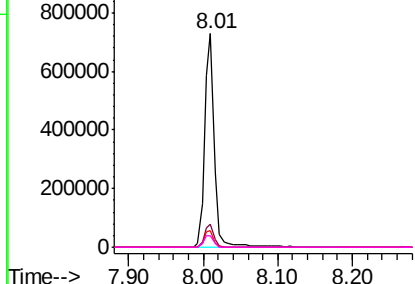
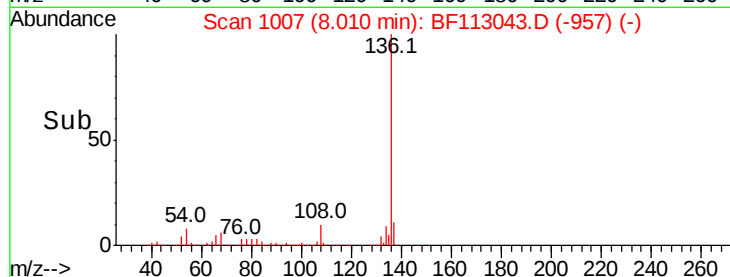



#23
Nitrobenzene-d5
Concen: 11.792 ng
RT: 7.28 min Scan# 883
Delta R.T. -0.02 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Tgt Ion:	82	Resp:	131297
Ion	Ratio	Lower	Upper
82	100		
128	43.6	36.3	54.5
54	52.2	43.7	65.5

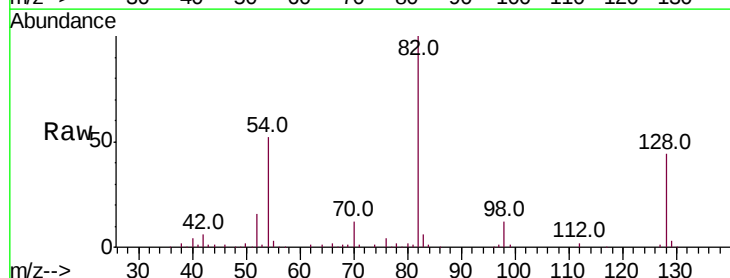

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

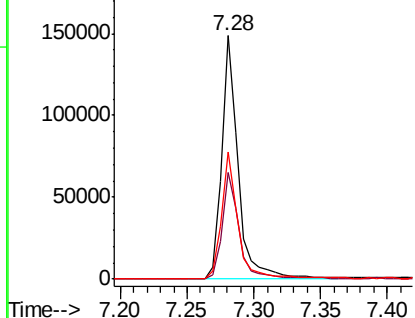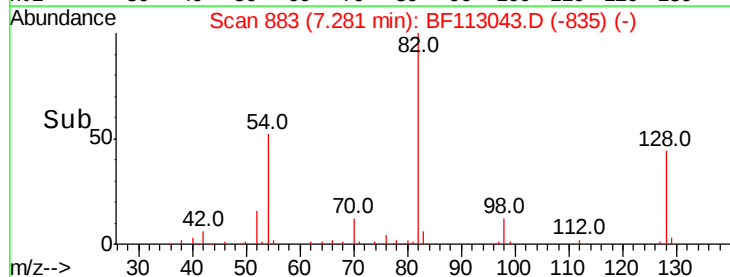



#25

Isophorone

Concen: 5.348 ng

RT: 7.28 min Scan# 883

Delta R.T. -0.28 min

Lab File: BF113043.D

Acq: 13 Mar 2019 22:42

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 128284

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#




138 0.0 13.8 20.8#

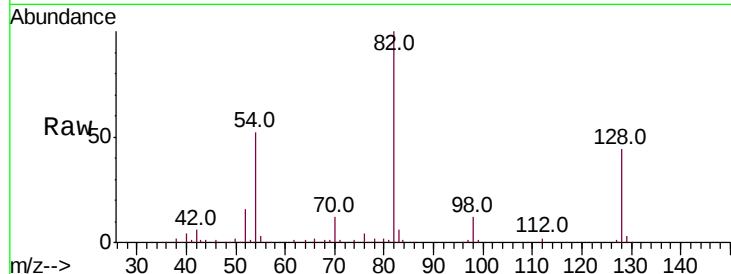

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

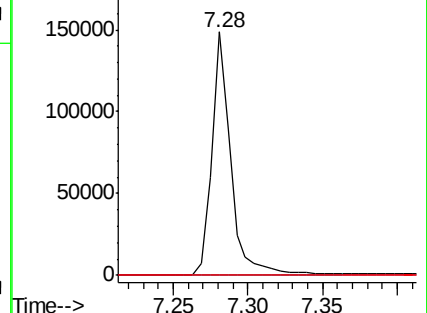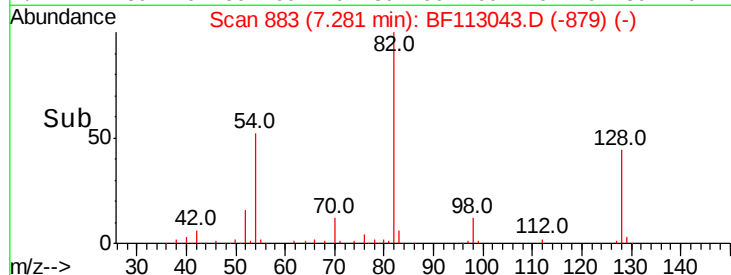

#31

Naphthalene

Concen: 7.023 ng

RT: 8.03 min Scan# 1010

Delta R.T. -0.01 min

Lab File: BF113043.D

Acq: 13 Mar 2019 22:42


Tgt Ion: 128 Resp: 232299

Ion Ratio Lower Upper

128 100

129 10.9 9.3 13.9



127 12.8 10.9 16.3




Abundance Ion 128.00 (127.70 to 128.70): BF1

Ion 129.00 (128.70 to 129.70): BF1

Ion 127.00 (126.70 to 127.70): BF1

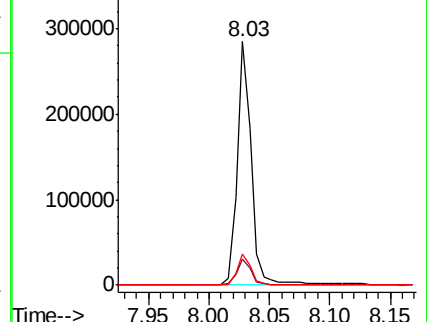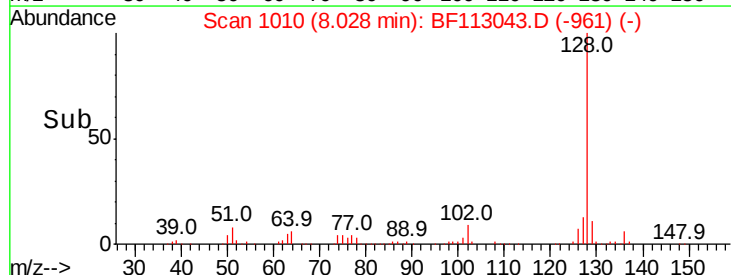


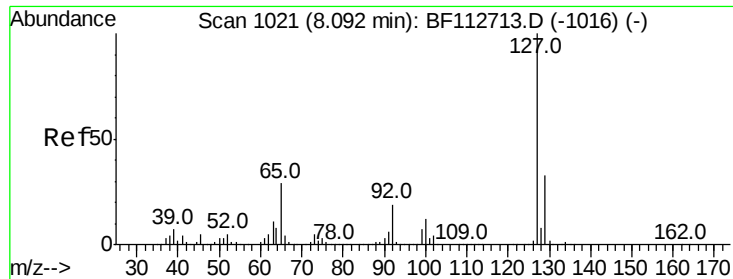




#33
4-Chloroaniline
Concen: 2.112 ng
RT: 8.03 min Scan# 1010
Delta R.T. -0.06 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Instrument :
BNA_F
ClientSampled :

Tot Ion:127 Resp: 29592
Ion Ratio Lower Upper
127 100
129 84.7 26.4 39.6#
65 0.0 23.1 34.7#
92 0.0 14.9 22.3#

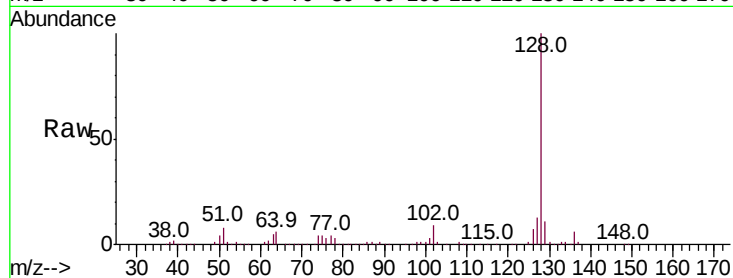


Abundance Ion 127.00 (126.70 to 127.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 65.00 (64.70 to 65.70): BF1
Ion 92.00 (91.70 to 92.70): BF1

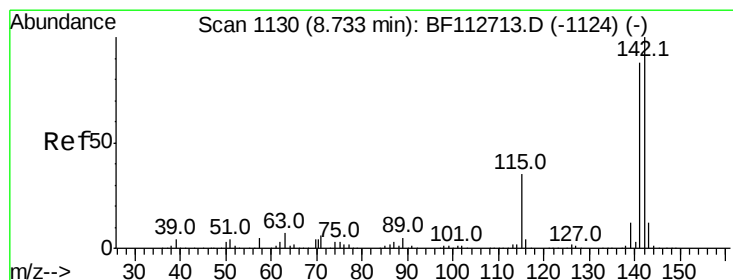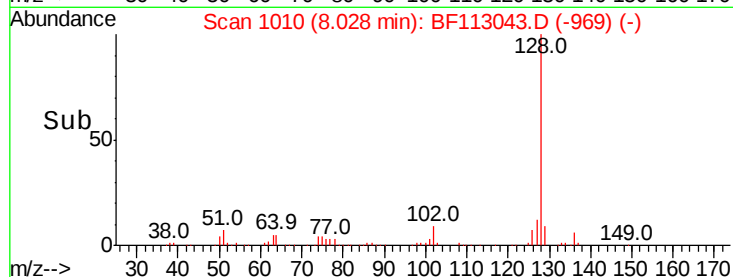
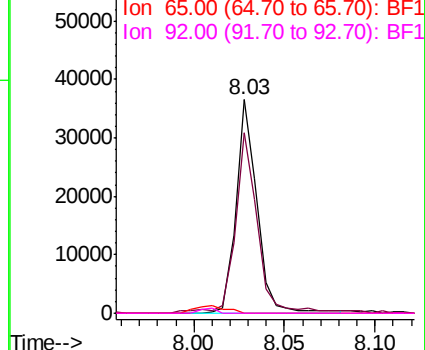



#37
2-Methylnaphthalene
Concen: 12.918 ng
RT: 8.72 min Scan# 1128
Delta R.T. -0.01 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Tgt Ion:142 Resp: 275952
Ion Ratio Lower Upper
142 100
141 87.2 70.3 105.5
115 30.8 27.8 41.6

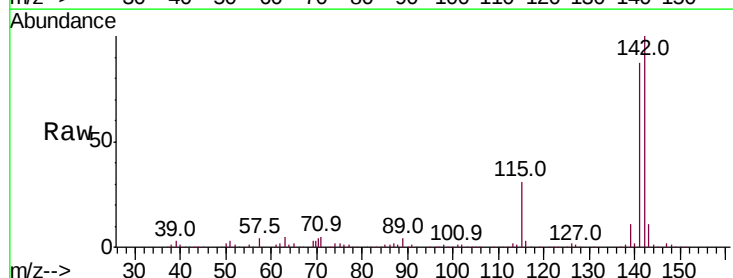

Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E
Ion 115.00 (114.70 to 115.70): E

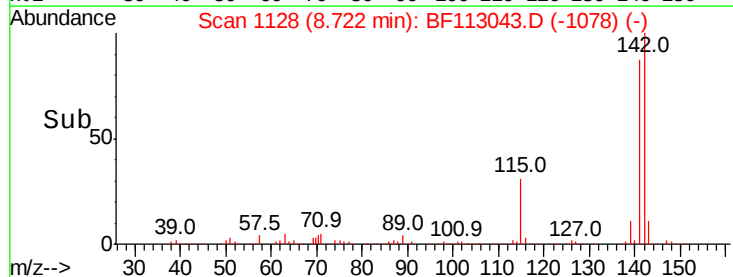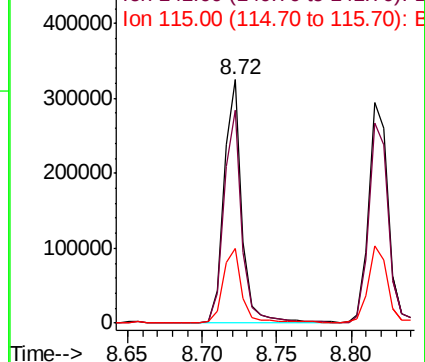


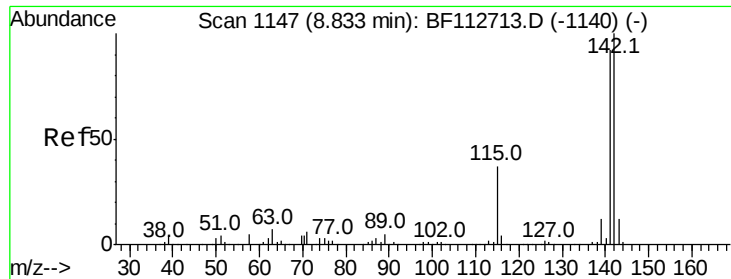




#38
1-Methvlnaphthalene
Concen: 12.849 ng
RT: 8.82 min Scan# 1144
Delta R.T. -0.01 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
142	100		
141	90.5	73.7	110.5
116	3.7	3.1	4.7




Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E
Ion 116.00 (115.70 to 116.70): E


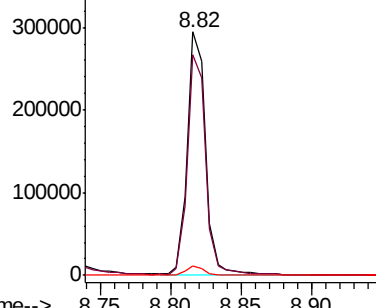



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.76 min Scan# 1304
Delta R.T. -0.01 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Tgt Ion	Ratio	Lower	Upper
164	100		
162	102.4	80.6	120.8
160	46.1	36.0	54.0



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

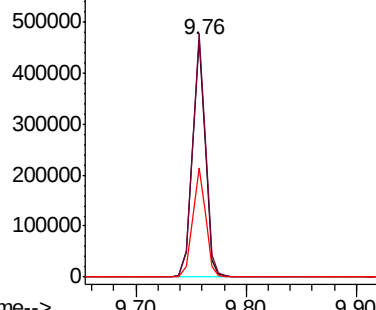







#42
 2,4,6-Tribromophenol
 Concen: 23.659 ng
 RT: 10.54 min Scan# 1437
 Delta R.T. -0.01 min
 Lab File: BF113043.D
 Acq: 13 Mar 2019 22:42

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:330 Resp: 96690
 Ion Ratio Lower Upper
 330 100
 332 96.0 76.2 114.4
 141 28.8 27.0 40.6

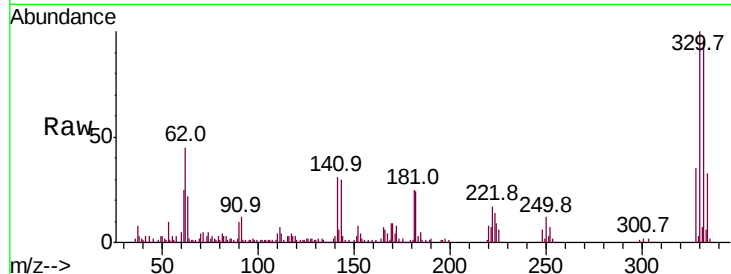


Abundance Ion 329.80 (329.50 to 330.50): E
 150000 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

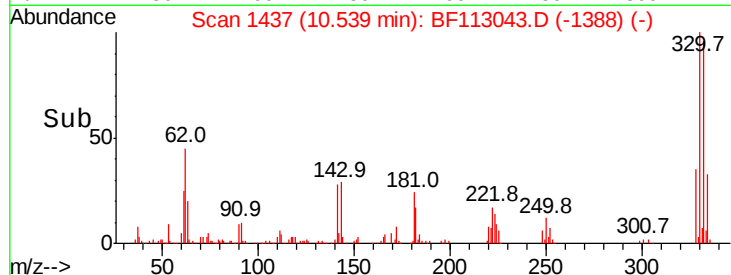
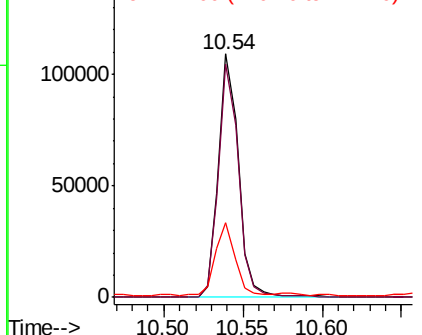



#45
 2-Fluorobiphenyl
 Concen: 11.571 ng
 RT: 9.08 min Scan# 1189
 Delta R.T. -0.01 min
 Lab File: BF113043.D
 Acq: 13 Mar 2019 22:42

Tgt Ion:172 Resp: 362899
 Ion Ratio Lower Upper
 172 100
 171 35.5 29.0 43.4
 170 23.5 20.0 30.0



Abundance Ion 172.00 (171.70 to 172.70): E
 600000 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

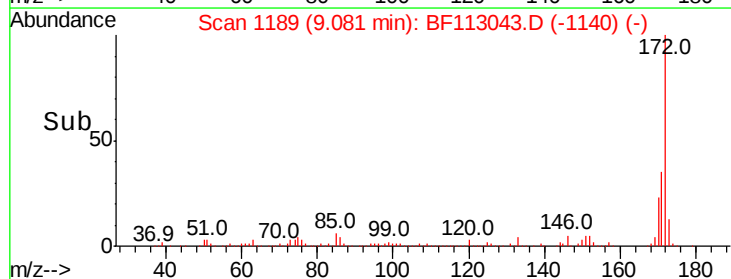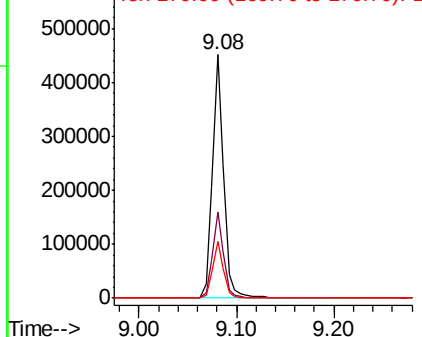

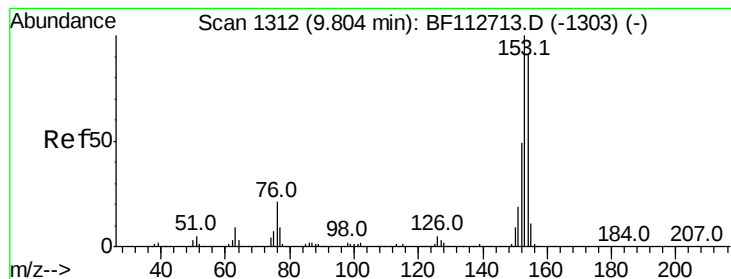

#52

Acenaphthene

Concen: 2.496 ng

RT: 9.79 min Scan# 1309

Delta R.T. -0.02 min

Lab File: BF113043.D

Acq: 13 Mar 2019 22:42

Instrument :

BNA_F

ClientSampleId :


Tot Ion:154 Resp: 60761

Ion Ratio Lower Upper

154 100

153 110.9 87.8 131.8




152 53.8 43.0 64.6



Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

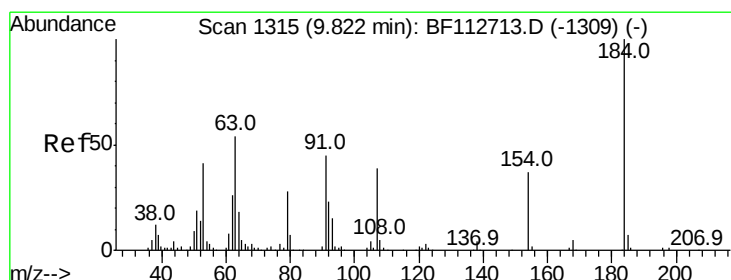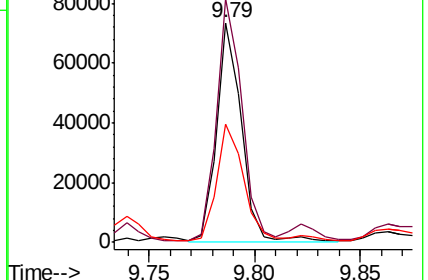

#54

2,4-Dinitrophenol

Concen: 6.541 ng

RT: 10.05 min Scan# 1354

Delta R.T. 0.22 min

Lab File: BF113043.D

Acq: 13 Mar 2019 22:42


Tgt Ion:184 Resp: 231

Ion Ratio Lower Upper

184 100

63 0.0 45.3 67.9#



154 114.5 46.0 69.0#




Abundance Ion 184.00 (183.70 to 184.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 154.00 (153.70 to 154.70): E

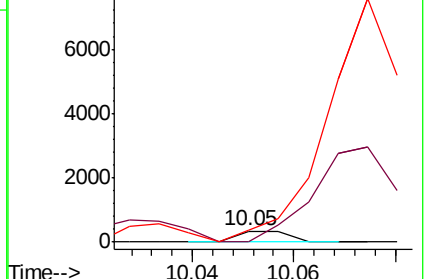

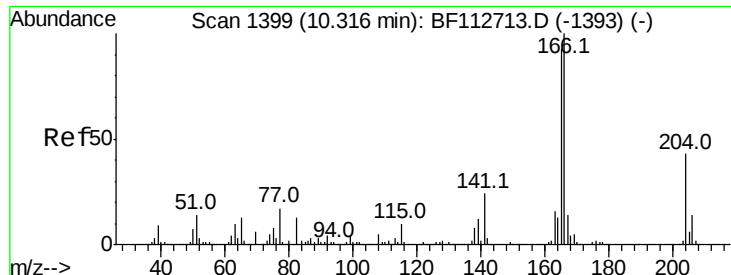

#58

Fluorene

Concen: 7.476 ng

RT: 10.30 min Scan# 1397

Delta R.T. -0.01 min

Lab File: BF113043.D

Acq: 13 Mar 2019 22:42

Instrument :

BNA_F

ClientSampleId :


Tot Ion:166 Resp: 187721

Ion Ratio Lower Upper

166 100

165 96.5 74.7 112.1




167 13.6 11.0 16.6



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

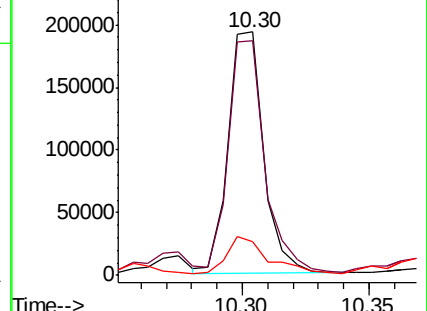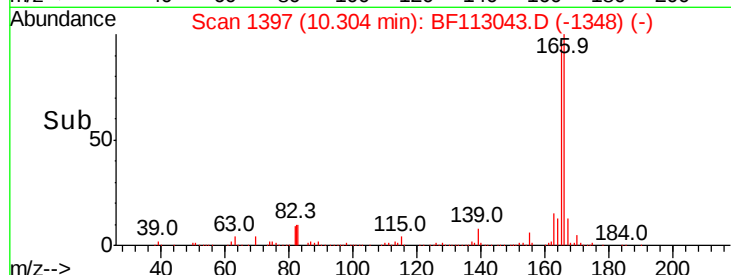

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.23 min Scan# 1555

Delta R.T. -0.01 min

Lab File: BF113043.D

Acq: 13 Mar 2019 22:42


Tgt Ion:188 Resp: 709186

Ion Ratio Lower Upper

188 100

94 9.5 9.0 13.4



80 10.1 9.2 13.8




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

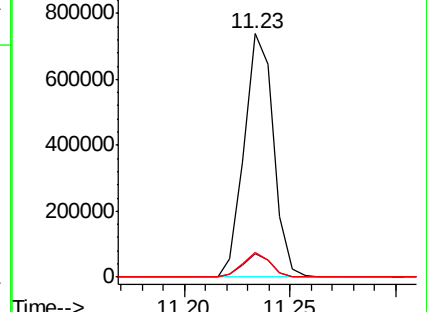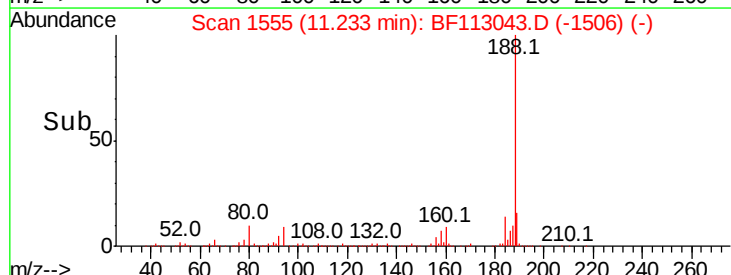


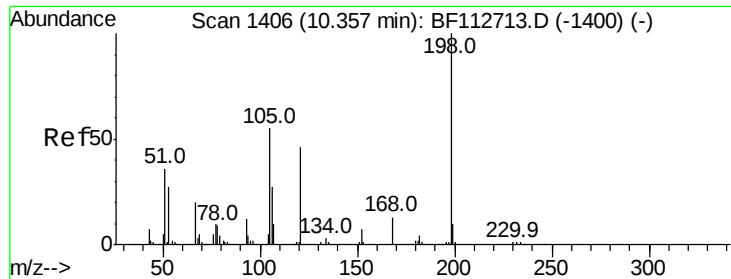




#65
4,6-Dinitro-2-methylphenol
Concen: 4.826 ng
RT: 10.58 min Scan# 1444
Delta R.T. 0.22 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Instrument :
BNA_F
ClientSampled :

Tot Ion:198 Resp: 687
Ion Ratio Lower Upper
198 100
51 201.3 43.8 83.8#
105 207.6 36.5 76.5#




Abundance Ion 198.00 (197.70 to 198.70): E
Ion 51.00 (50.70 to 51.70): BF1
Ion 105.00 (104.70 to 105.70): E

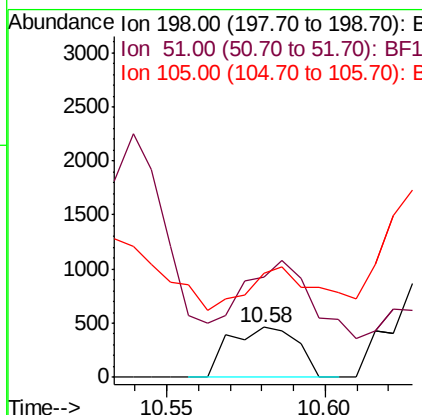




#71
Phenanthrene
Concen: 23.666 ng
RT: 11.26 min Scan# 1560
Delta R.T. -0.01 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Tgt Ion:178 Resp: 835057
Ion Ratio Lower Upper
178 100
176 19.6 16.3 24.5
179 15.6 12.7 19.1



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

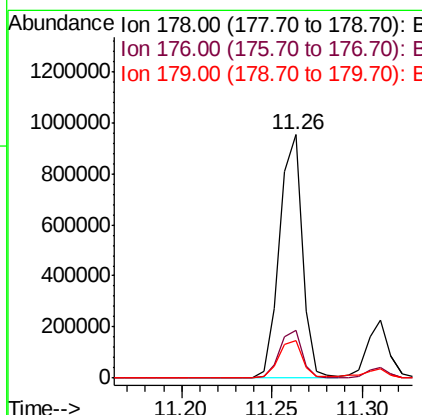

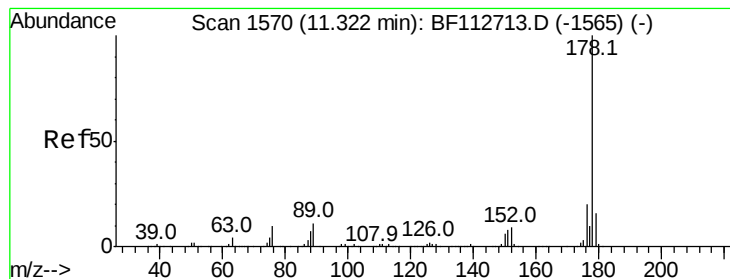

#72

Anthracene

Concen: 4.810 ng

RT: 11.31 min Scan# 1568

Delta R.T. -0.01 min

Lab File: BF113043.D

Acq: 13 Mar 2019 22:42


Instrument :

BNA_F

ClientSampleId :

Tot Ion:178 Resp: 177649

Ion	Ratio	Lower	Upper
178	100		
176	18.3	15.8	23.6
179	15.3	13.0	19.6

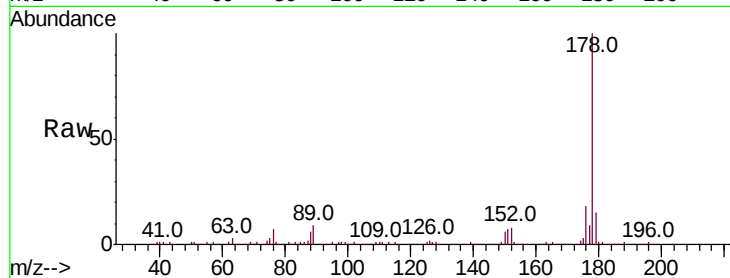



Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

Time-->

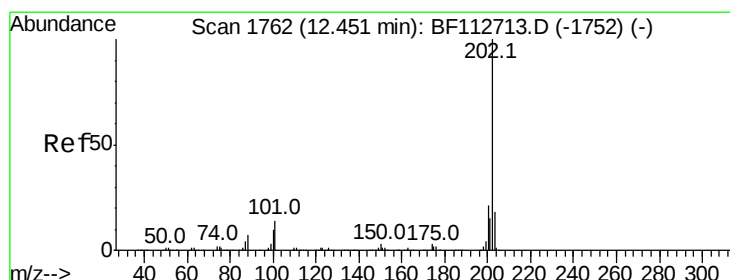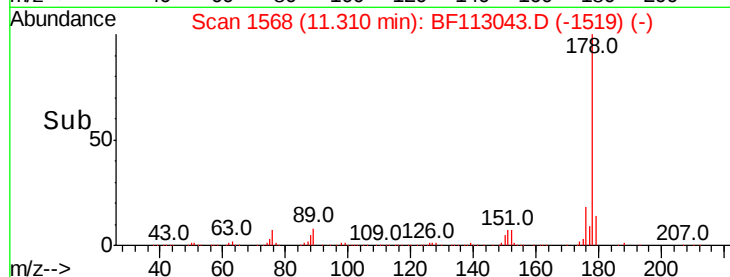

#75

Fluoranthene

Concen: 20.701 ng

RT: 12.45 min Scan# 1761


Delta R.T. -0.01 min

Lab File: BF113043.D

Acq: 13 Mar 2019 22:42

Tgt Ion:202 Resp: 782572

Ion	Ratio	Lower	Upper
202	100		
101	10.6	0.0	33.8
203	18.1	0.0	38.4

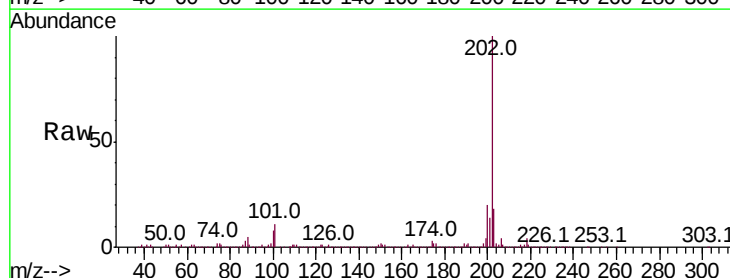


Abundance


Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

Time-->

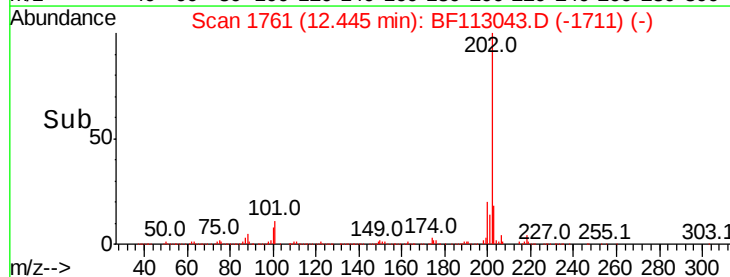







#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.86 min Scan# 2002
Delta R.T. -0.01 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Instrument :
BNA_F
ClientSampleId :

Tot Ion:240 Resp: 539976
Ion Ratio Lower Upper
240 100
120 11.3 8.9 13.3
236 25.9 20.7 31.1




Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

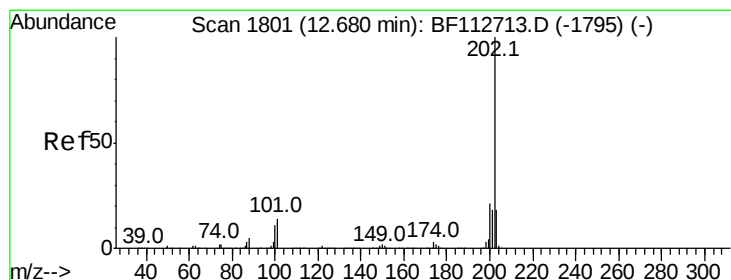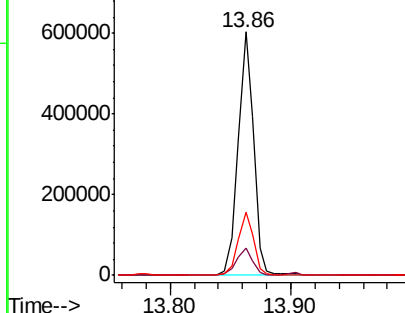




#78
Pyrene
Concen: 21.555 ng
RT: 12.67 min Scan# 1799
Delta R.T. -0.01 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Tgt Ion:202 Resp: 981229
Ion Ratio Lower Upper
202 100
200 20.3 17.0 25.4
203 18.0 14.4 21.6



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E



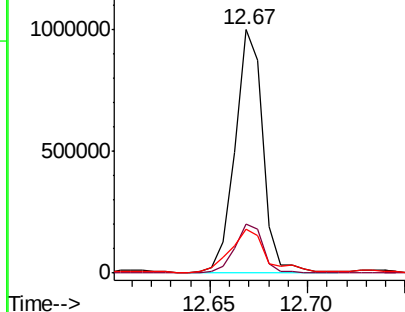
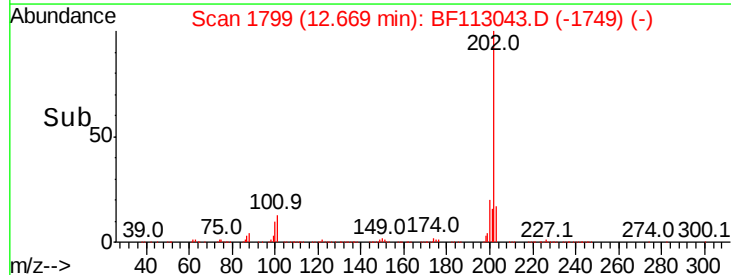


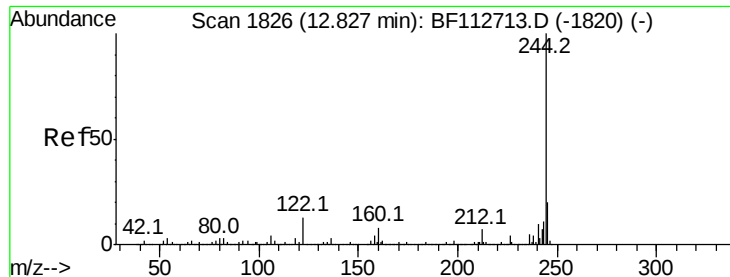

#79
 Terphenyl-d14
 Concen: 14.089 ng
 RT: 12.82 min Scan# 1824
 Delta R.T. -0.01 min
 Lab File: BF113043.D
 Acq: 13 Mar 2019 22:42




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:244 Resp: 392453
 Ion Ratio Lower Upper
 244 100
 212 6.2 5.6 8.4
 122 8.8 10.5 15.7#

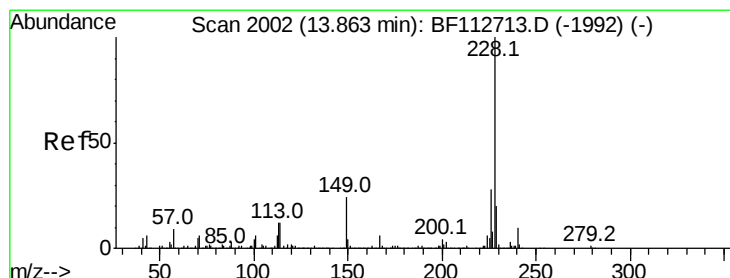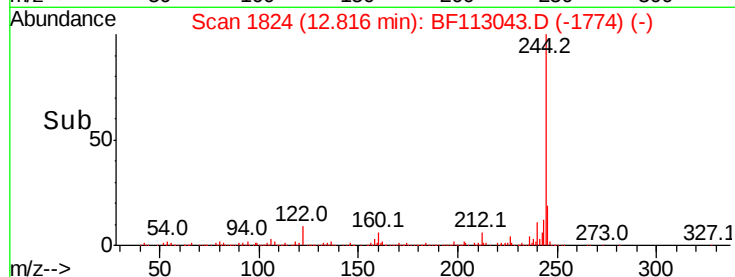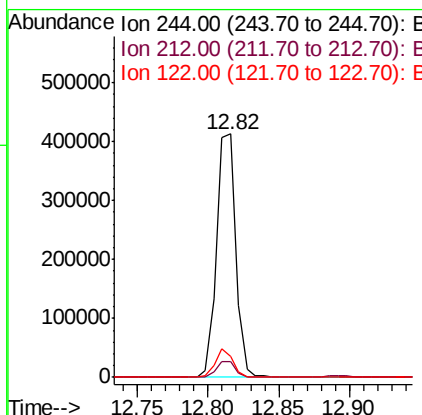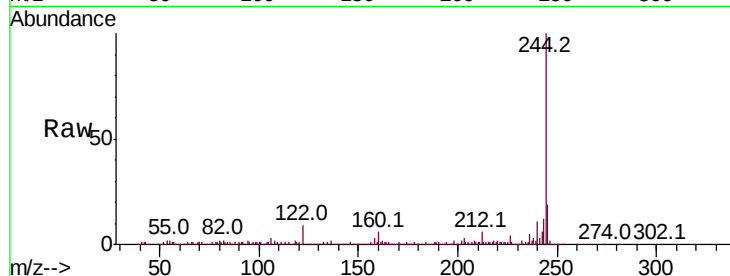

#81
 Benzo(a)anthracene
 Concen: 9.852 ng
 RT: 13.85 min Scan# 2000
 Delta R.T. -0.01 min
 Lab File: BF113043.D
 Acq: 13 Mar 2019 22:42

Tgt Ion:228 Resp: 368690
 Ion Ratio Lower Upper
 228 100
 226 30.9 22.2 33.4
 229 23.4 16.0 24.0

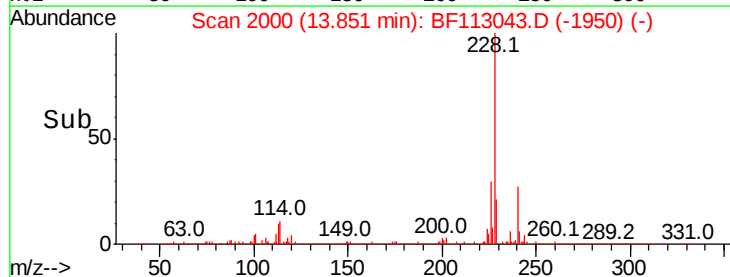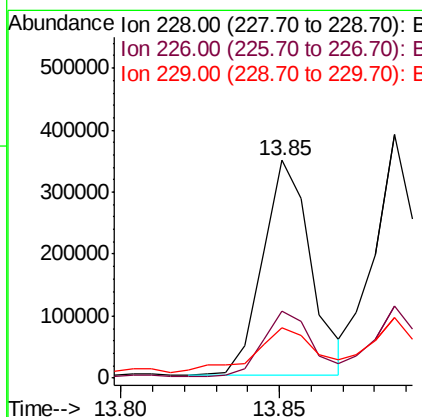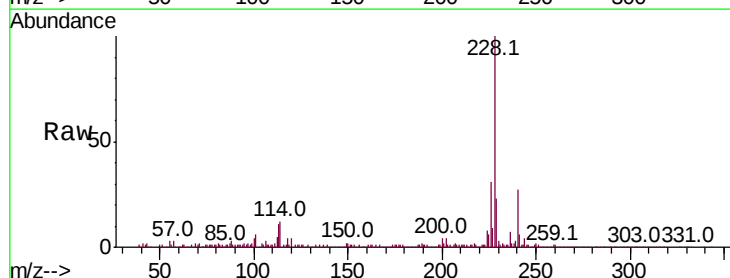







#83
Chrysene
Concen: 10.058 ng
RT: 13.85 min Scan# 2000
Delta R.T. -0.05 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Instrument :
BNA_F
ClientSampleId :

Tot	Ion:228	Resp:	368690
Ion	Ratio	Lower	Upper
228	100		
226	30.9	24.9	37.3
229	23.4	16.3	24.5




Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E


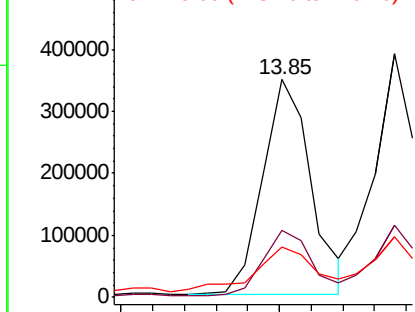



#87
Perylene-d12
Concen: 20.000 ng
RT: 15.27 min Scan# 2241
Delta R.T. -0.01 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Tgt Ion:264	Resp: 507580
Ion Ratio	Lower Upper
264 100	
260 23.9	18.7 28.1
265 23.0	17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

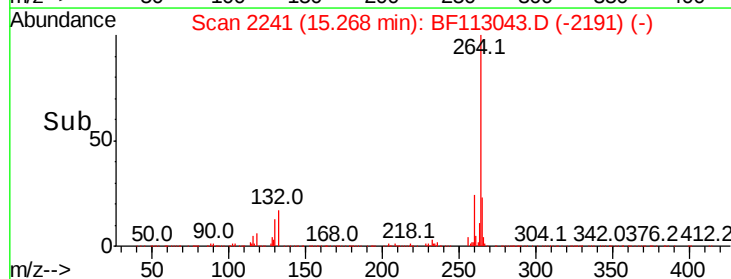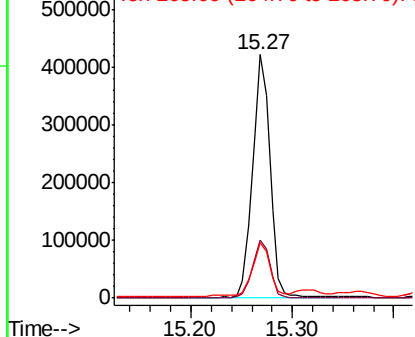



#88

Benzo(b)fluoranthene

Concen: 13.473 ng

RT: 14.87 min Scan# 2173

Delta R.T. -0.01 min





Lab File: BF113043.D

Acq: 13 Mar 2019 22:42

Instrument :
BNA_F
ClientSampleId :

Tot Ion:252 Resp: 442340

Ion	Ratio	Lower	Upper
252	100		
253	24.0	18.0	27.0
125	12.3	10.2	15.2

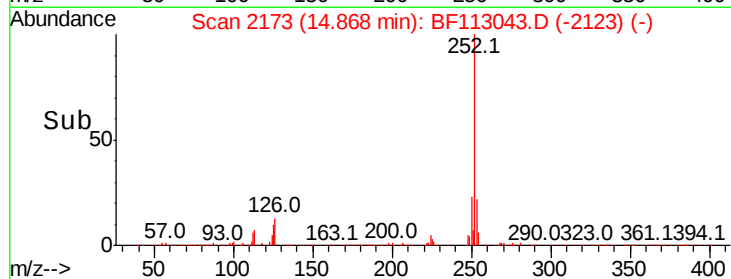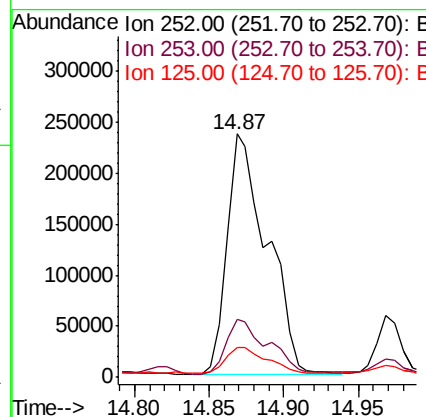

#89

Benzo(k)fluoranthene

Concen: 14.874 ng

RT: 14.87 min Scan# 2173




Delta R.T. -0.04 min


Lab File: BF113043.D

Acq: 13 Mar 2019 22:42

Tgt Ion:252 Resp: 442340

Ion	Ratio	Lower	Upper
252	100		
253	24.0	18.2	27.2
125	12.3	9.8	14.6


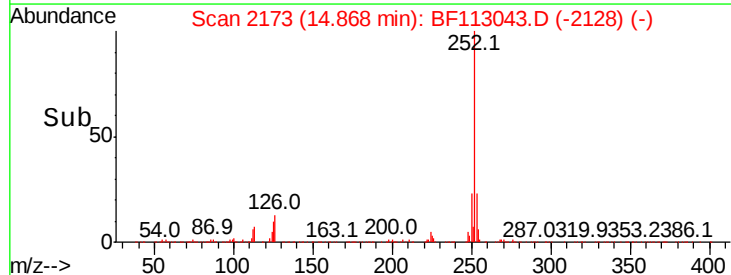
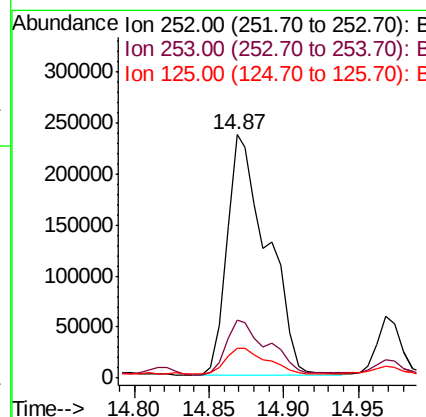





#90
Benzo(a)pyrene
Concen: 9.436 ng
RT: 15.21 min Scan# 2231
Delta R.T. -0.01 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Instrument :
BNA_F
ClientSampleId :

Tot Ion:252 Resp: 274014
Ion Ratio Lower Upper
252 100
253 23.7 18.0 27.0
125 11.2 10.7 16.1

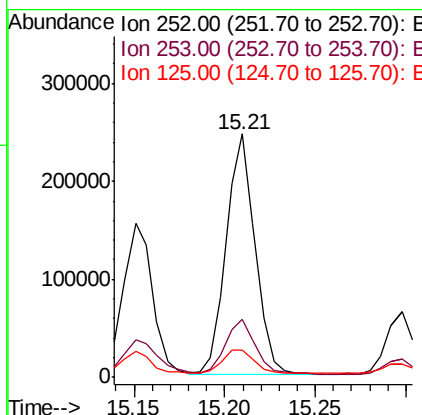

#92
Benzo(g,h,i)perylene
Concen: 5.131 ng
RT: 17.03 min Scan# 2541
Delta R.T. -0.01 min
Lab File: BF113043.D
Acq: 13 Mar 2019 22:42

Tgt Ion:276 Resp: 127673
Ion Ratio Lower Upper
276 100
277 24.8 18.6 27.8
138 22.2 19.4 29.0

