
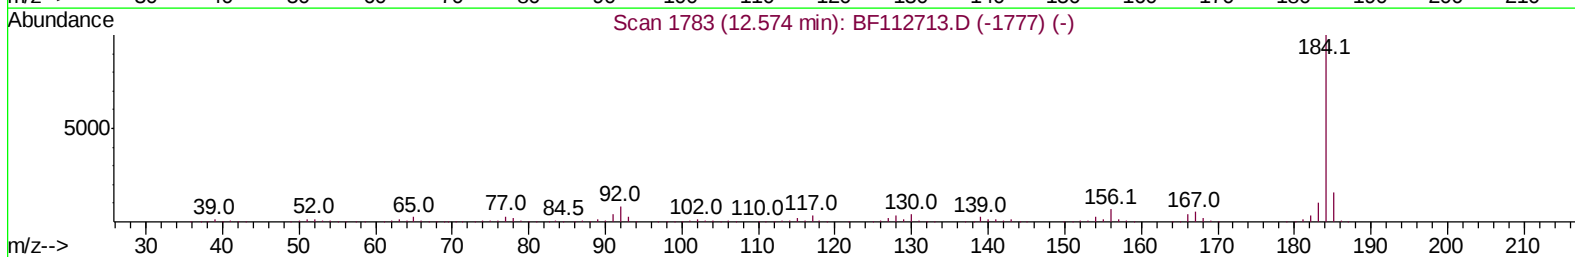
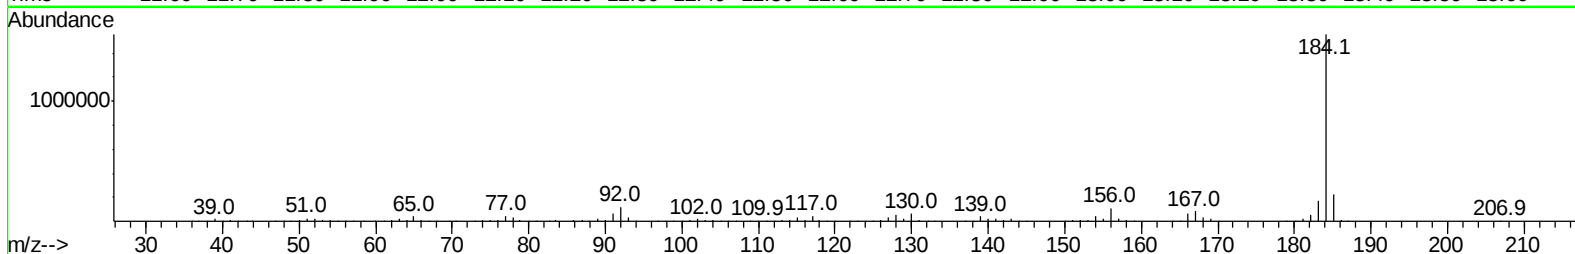


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF031319\
Data File : BF113031.D
Acq On : 13 Mar 2019 14:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 03:51:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 13 03:42:55 2019
Response via : Initial Calibration

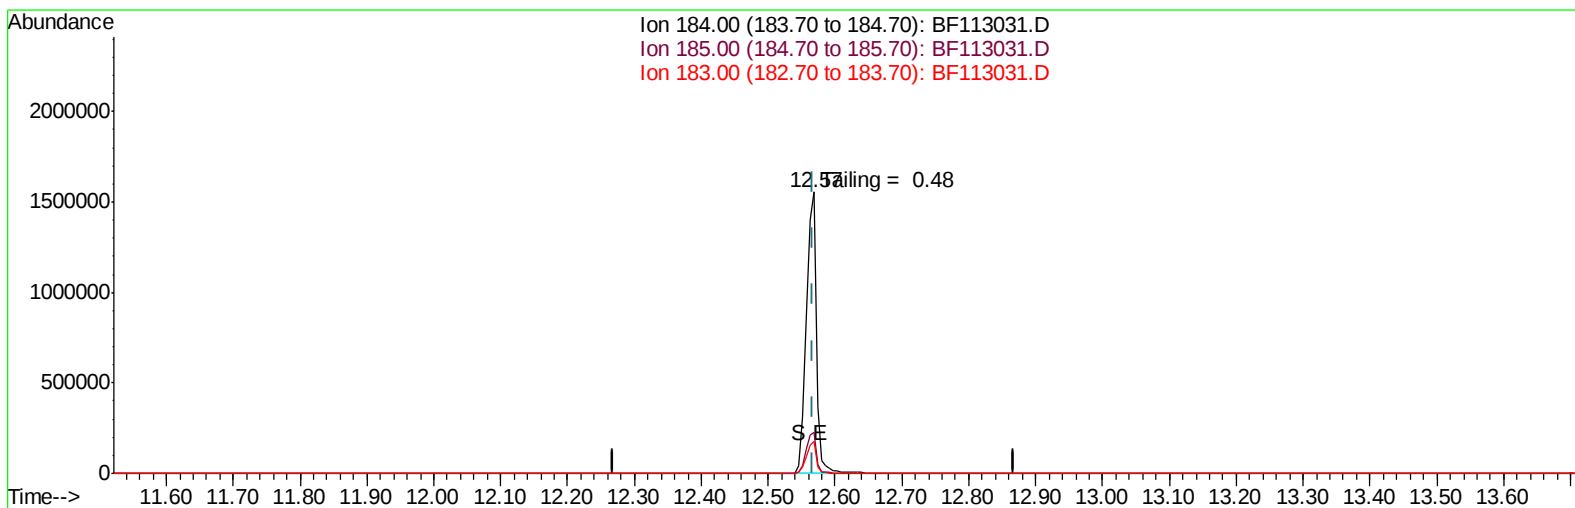

TIC: BF113031.D

(77) Benzidine

12.568min (-0.000) 59282.07ng

response 1685459

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.73
183.00	10.70	11.25
0.00	0.00	0.00