


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031319\
 Data File : BF113031.D
 Acq On : 13 Mar 2019 14:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 13 03:42:55 2019

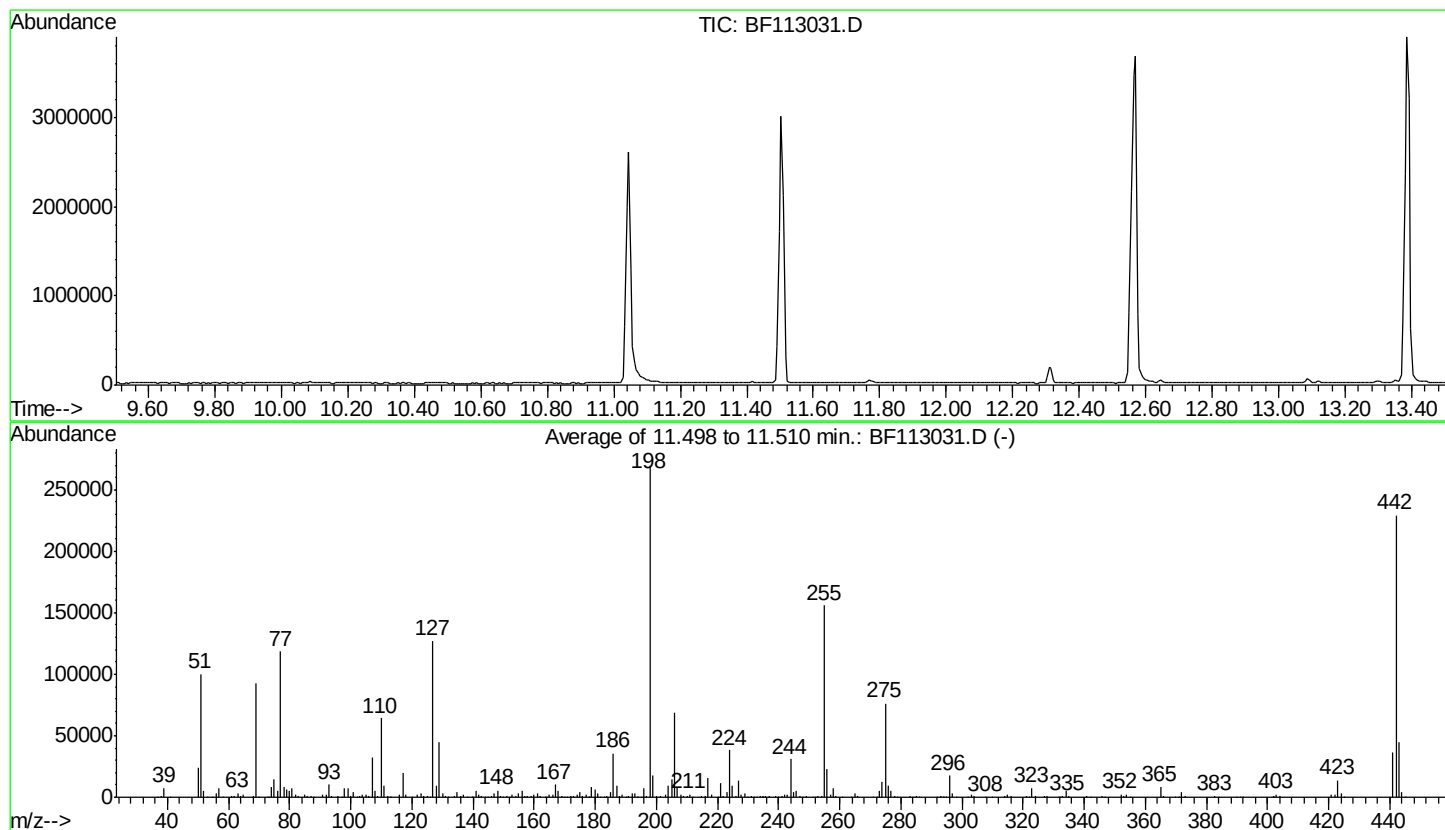

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	100421	PASS
68	69	0.00	2	1.6	1483	PASS
69	198	0.00	100	34.4	92738	PASS
70	69	0.00	2	0.6	550	PASS
127	198	10	80	47.2	127309	PASS
197	198	0.00	2	0.3	904	PASS
198	198	100	100	100.0	269525	PASS
199	198	5	9	6.7	18180	PASS
275	198	10	60	28.3	76338	PASS
365	198	1	100	3.2	8742	PASS
441	198	0.01	100	13.6	36717	PASS
442	198	50	100	84.9	228946	PASS
443	442	15	24	19.4	44349	PASS