
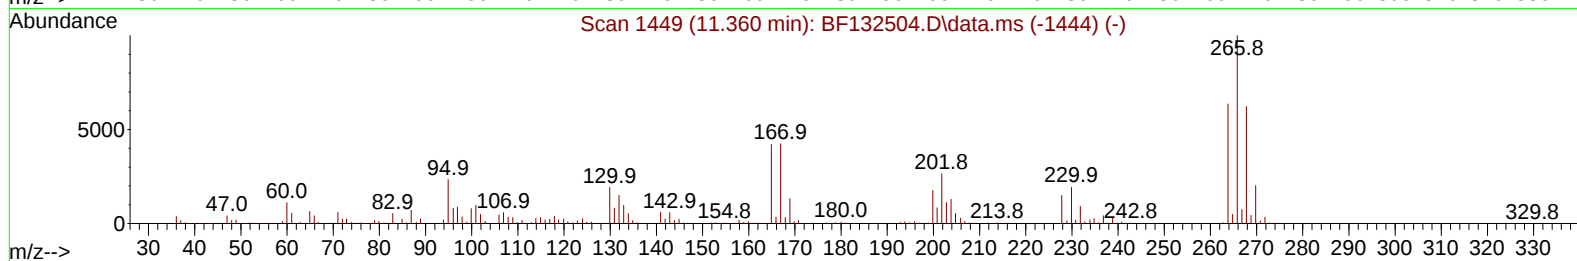
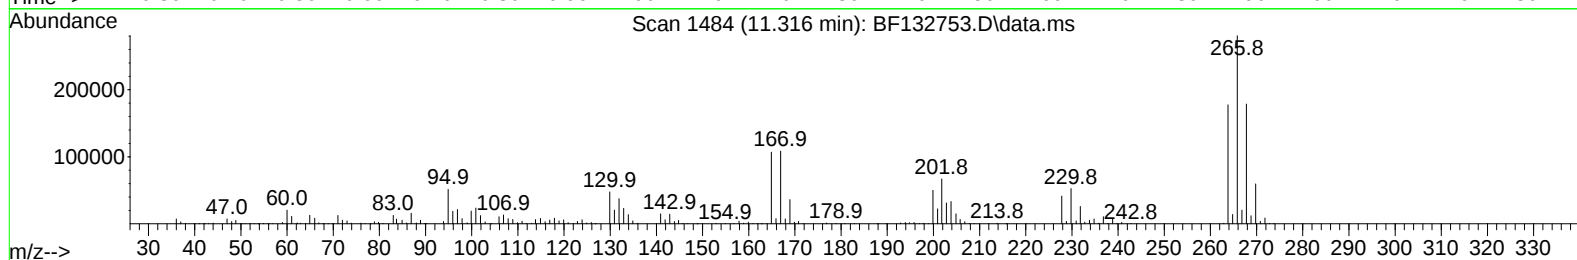


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031323\
 Data File : BF132753.D
 Acq On : 13 Mar 2023 10:26
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 03:31:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 13 13:44:13 2023
 Response via : Initial Calibration

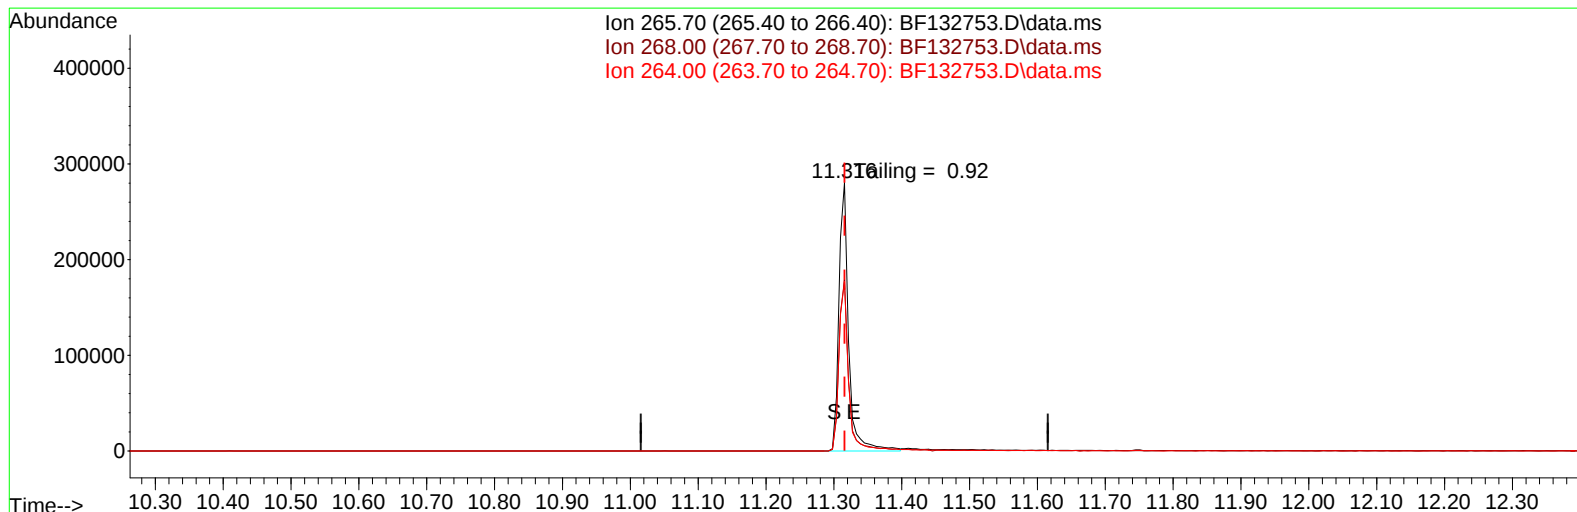

TIC: BF132753.D\data.ms




(70) Pentachlorophenol (C)

11.316min (-0.000) 623681.44 ng

response 278246

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.66
264.00	63.60	63.22
0.00	0.00	0.00

Quant Time: Mar 14 03:31:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 13 13:44:13 2023
Response via : Initial Calibration

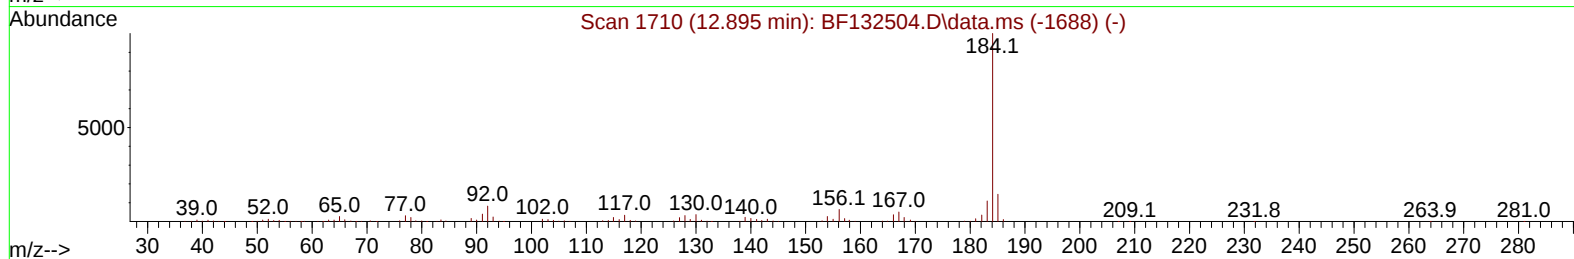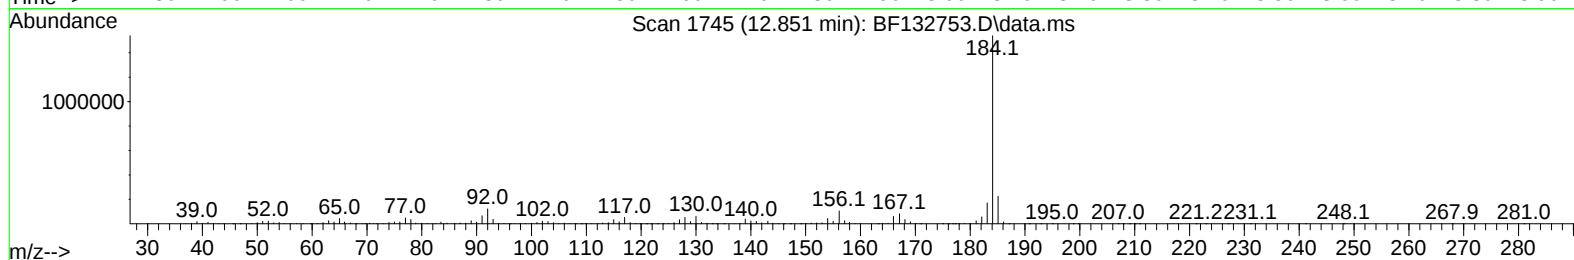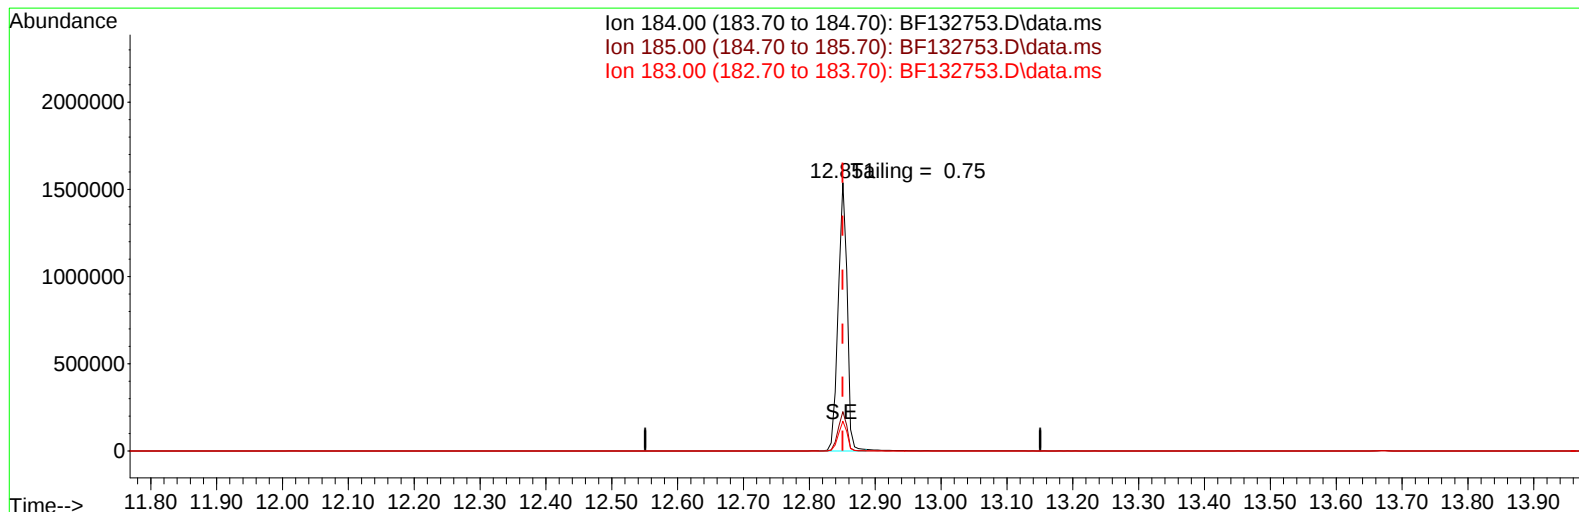

TIC: BF132753.D\data.ms

(77) Benzidine

12.851min (-0.000) 103018.84 ng

```
response      1479586
```

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.67
183.00	10.90	11.12
0.00	0.00	0.00