


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031323\
 Data File : BF132753.D
 Acq On : 13 Mar 2023 10:26
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 13 13:44:13 2023

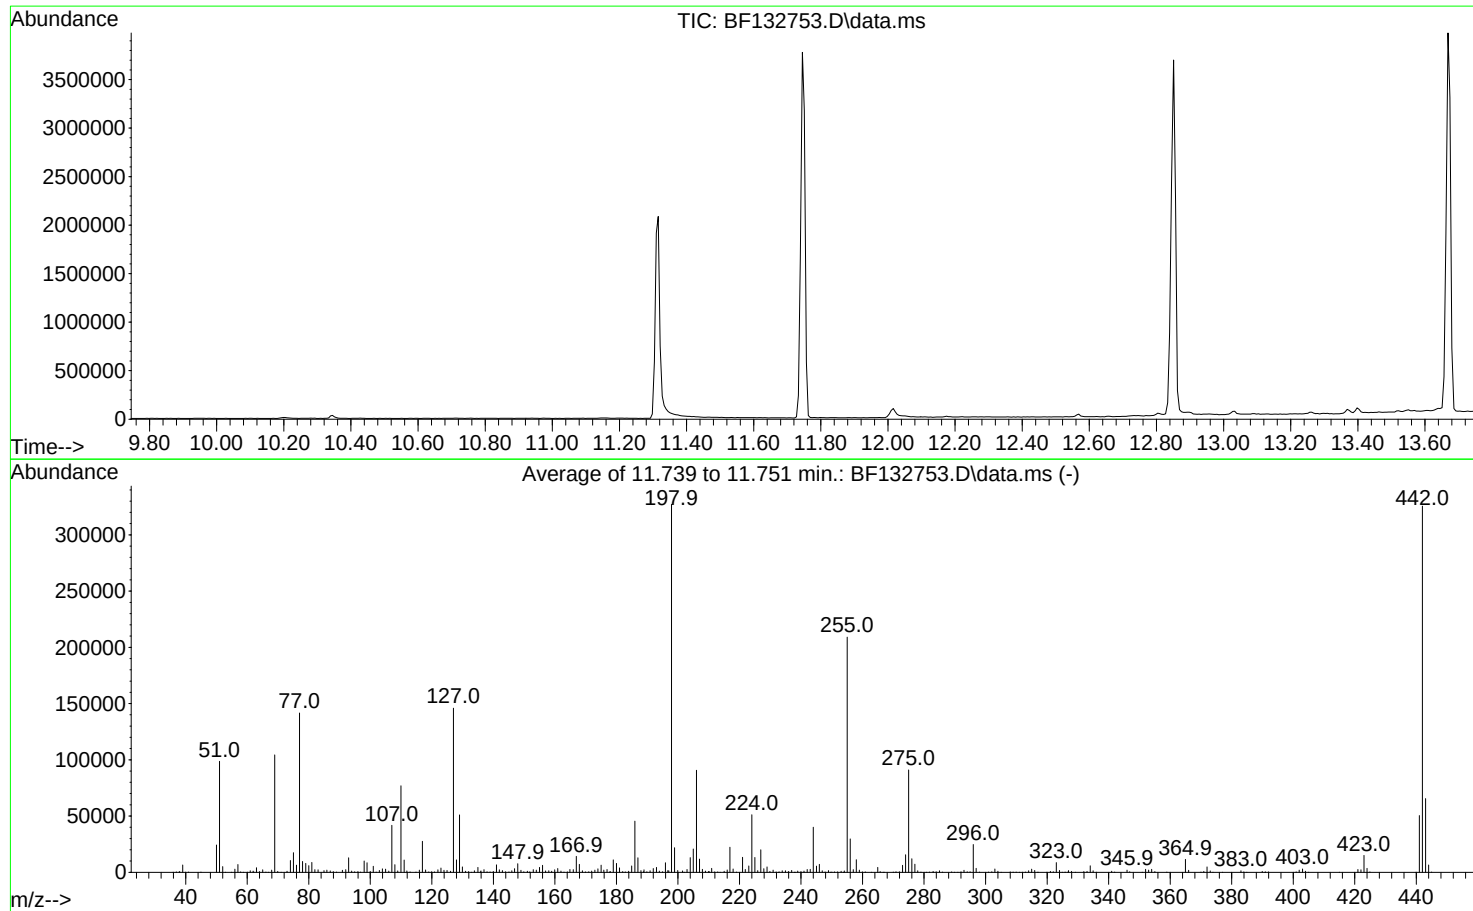




AutoFind: Scans 1556, 1557, 1558; Background Corrected with Scan 1551

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	98608	PASS
68	69	0.00	2	1.9	1965	PASS
69	198	0.00	100	31.9	104310	PASS
70	69	0.00	2	0.7	737	PASS
127	198	10	80	44.6	145952	PASS
197	198	0.00	2	0.5	1543	PASS
198	198	100	100	100.0	327083	PASS
199	198	5	9	6.7	21908	PASS
275	198	10	60	27.8	90973	PASS
365	198	1	100	3.5	11517	PASS
441	198	0.01	100	15.4	50485	PASS
442	442	50	100	100.0	325603	PASS
443	442	15	24	20.1	65467	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031323\
 Data File : BF132753.D
 Acq On : 13 Mar 2023 10:26
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 14 03:31:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 13 13:44:13 2023
 Response via : Initial Calibration

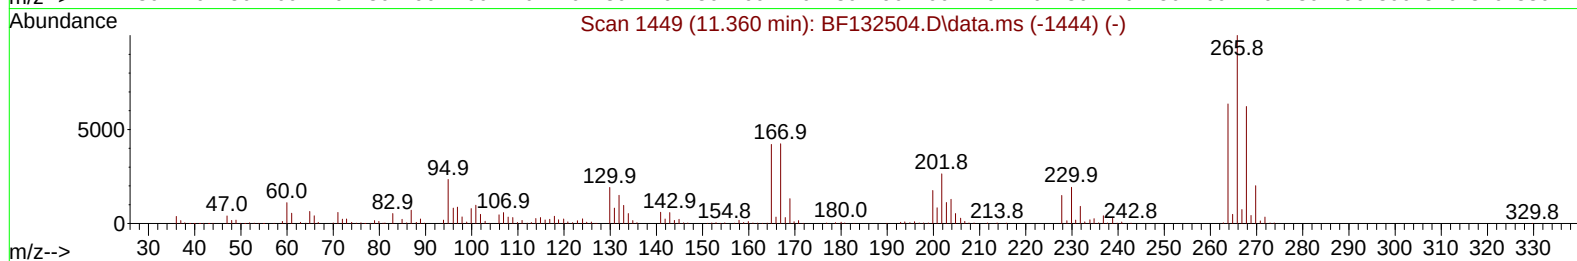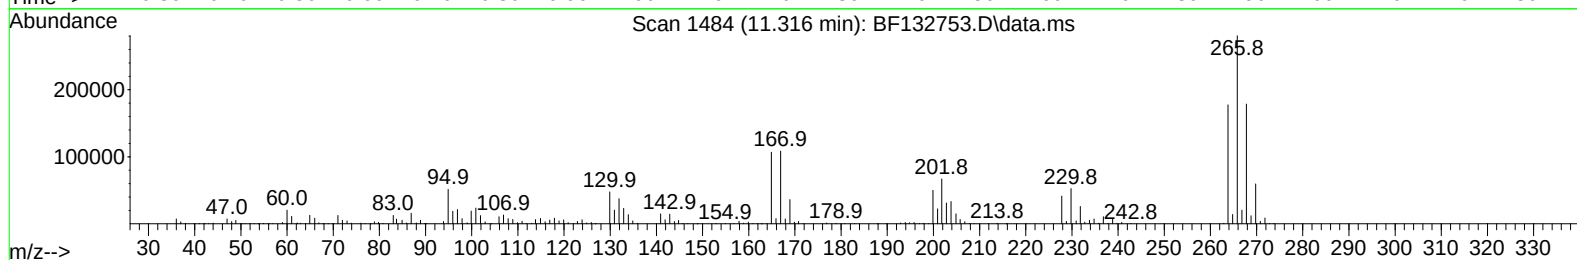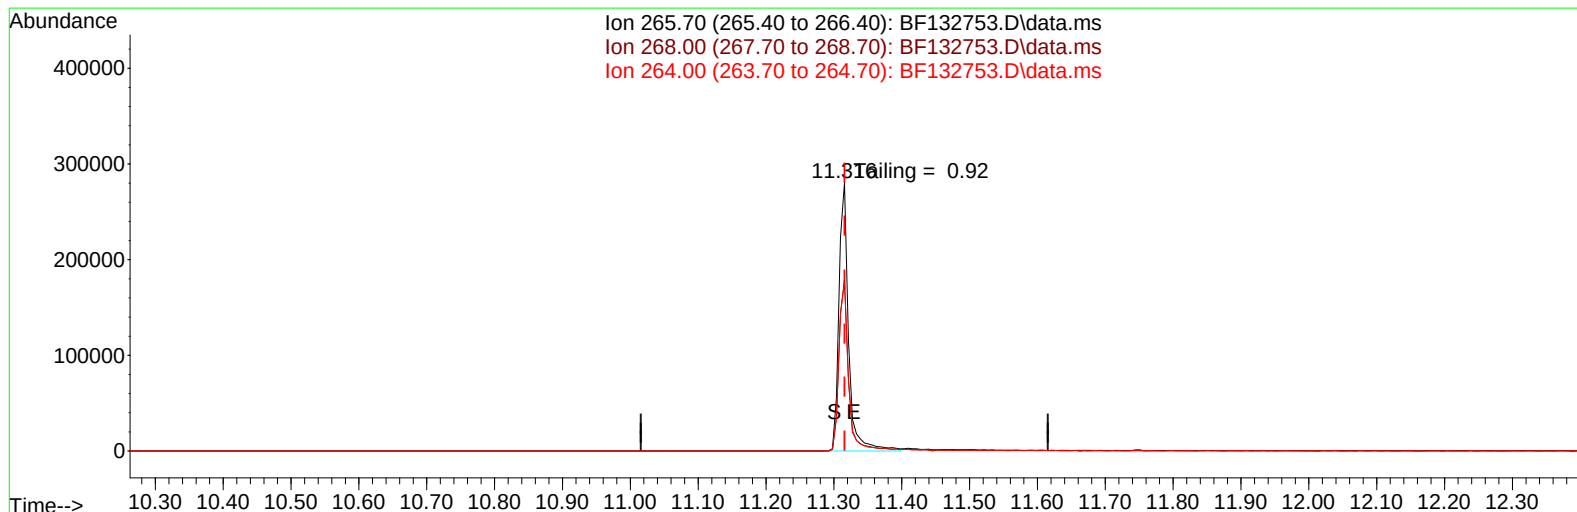

TIC: BF132753.D\data.ms

(70) Pentachlorophenol (C)

11.316min (-0.000) 623681.44 ng




response 278246

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.66
264.00	63.60	63.22
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031323\  
Data File : BF132753.D  
Acq On    : 13 Mar 2023  10:26  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 14 03:31:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 13 13:44:13 2023
Response via : Initial Calibration

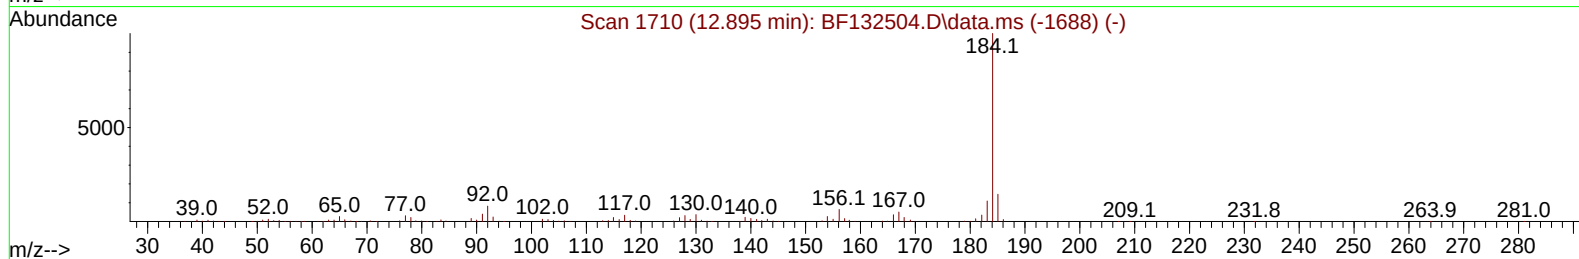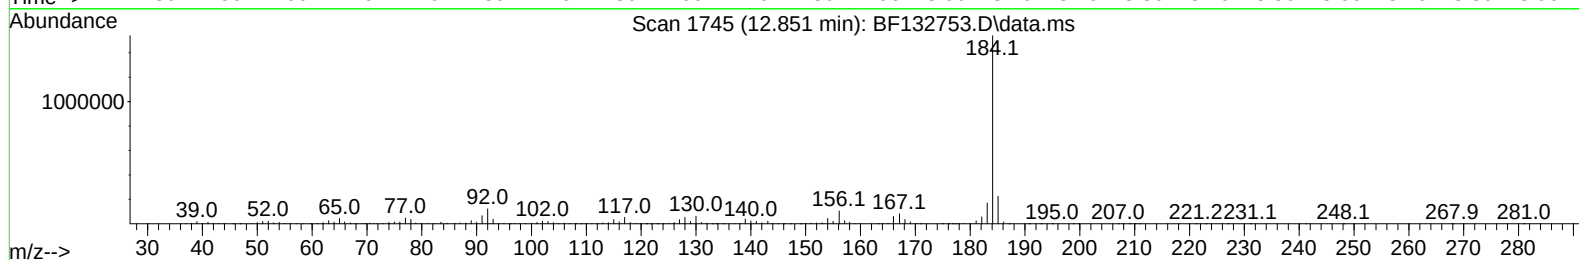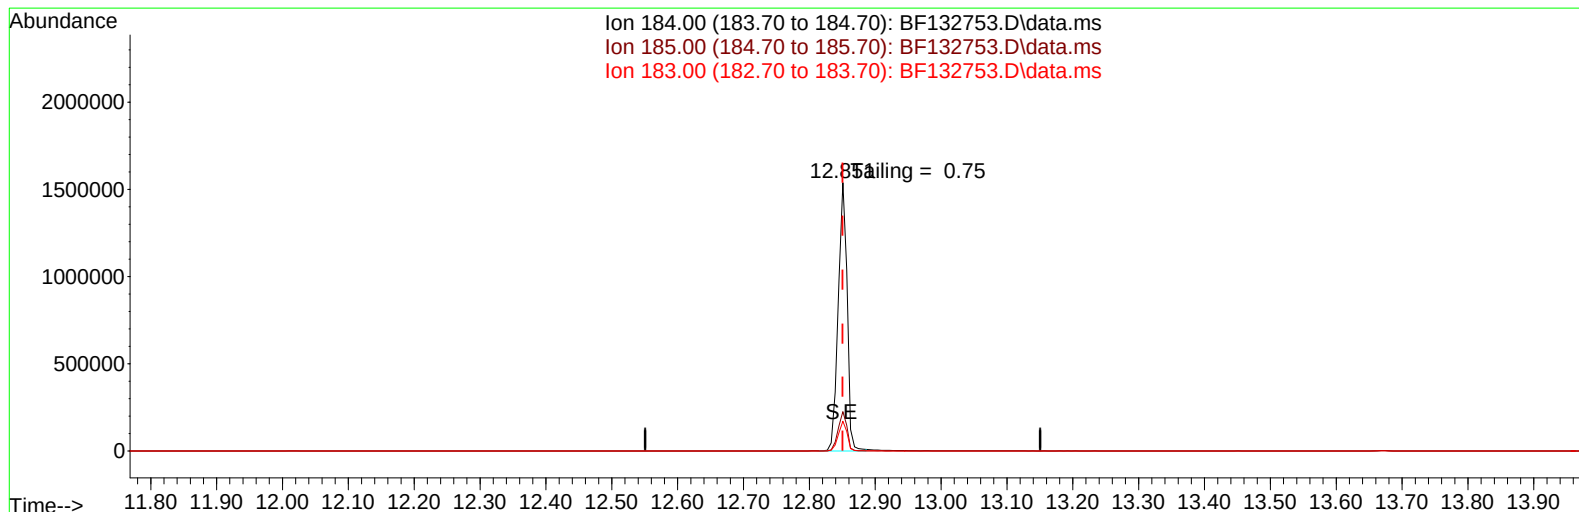

TIC: BF132753.D\data.ms

(77) Benzidine

12.851min (-0.000) 103018.84 ng

response **1479586**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.67
183.00	10.90	11.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/13/2023	BNA_F	<u>BF132753.D</u>
Compound Name	Response	Retention Time
DDT	750952	13.668
DDD	18436	13.398
DDE	4748	13.033
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23184	774136	2.99

Instrument :
BNA_F
ClientSampleId :
DFTPP