
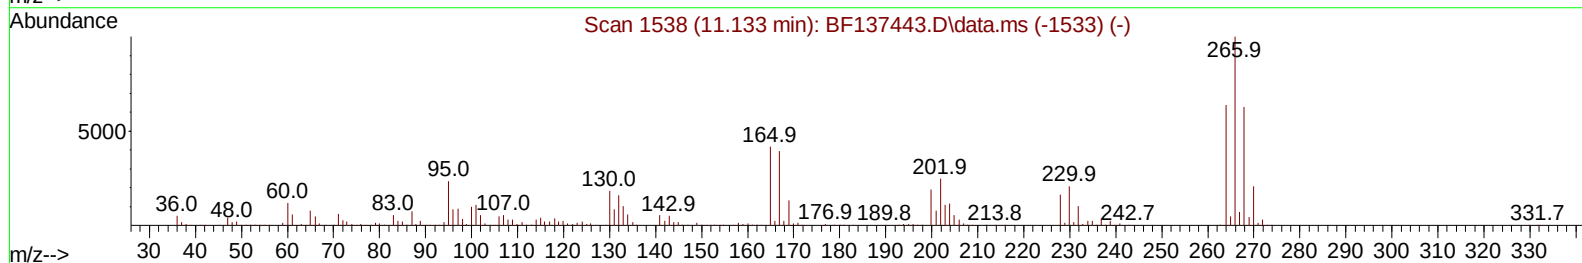
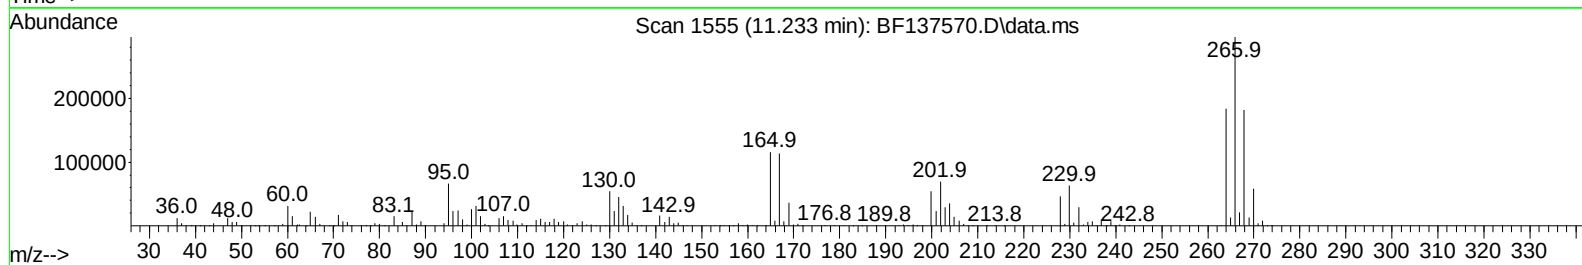


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031324\
Data File : BF137570.D
Acq On : 13 Mar 2024 08:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 04:25:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 04:02:20 2024
Response via : Initial Calibration

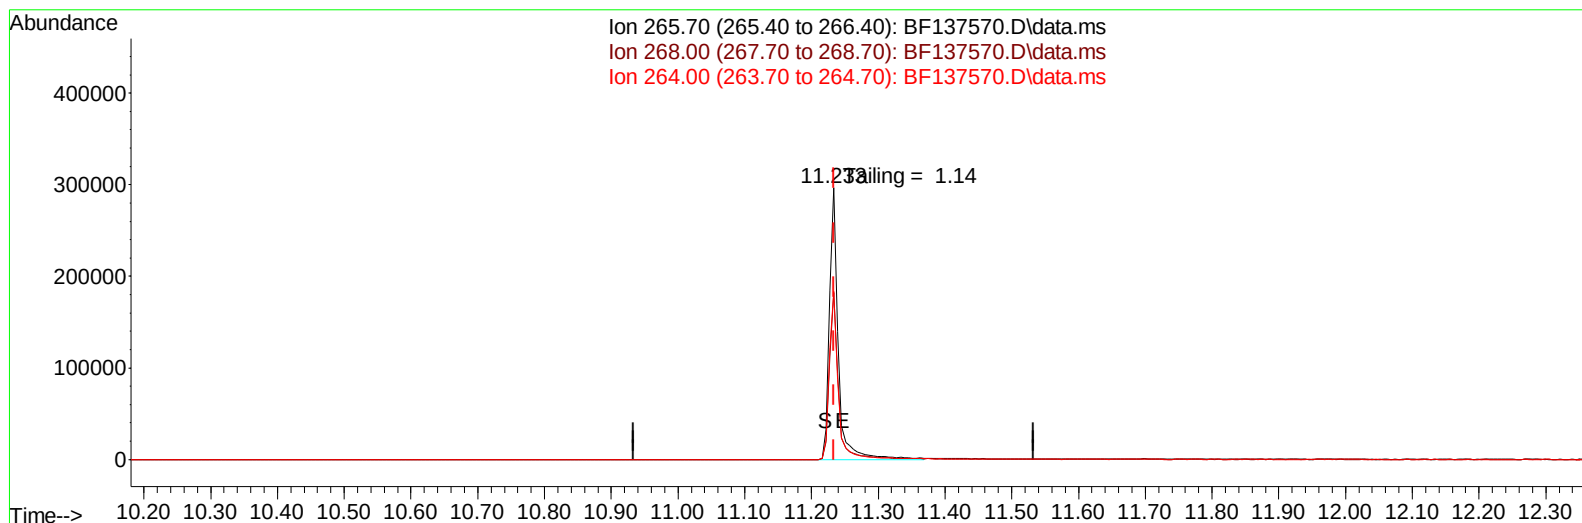

TIC: BF137570.D\data.ms

(70) Pentachlorophenol (C)




11.233min (+ 0.000) 270605.16 ng

response 278936

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	61.38
264.00	63.60	62.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031324\
Data File : BF137570.D
Acq On : 13 Mar 2024 08:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 04:25:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 04:02:20 2024
Response via : Initial Calibration

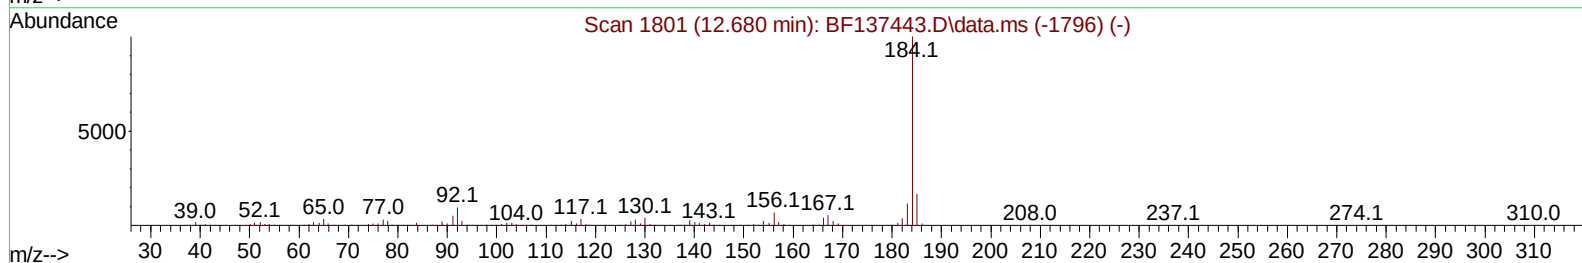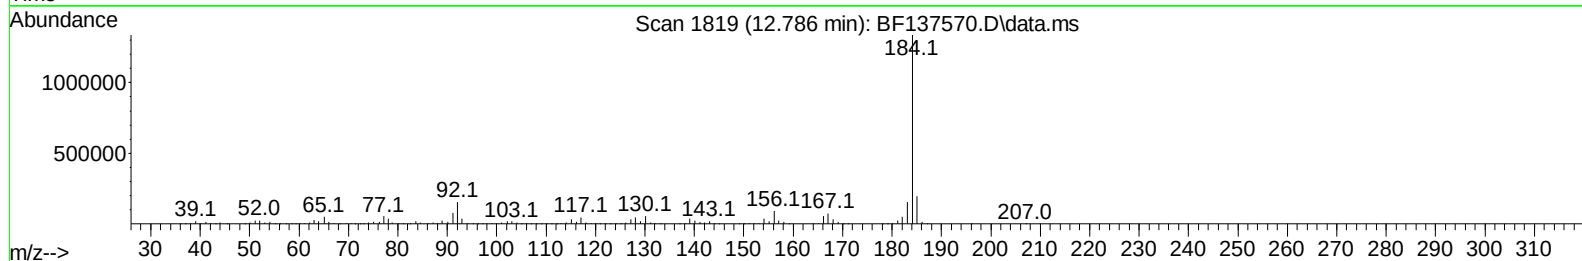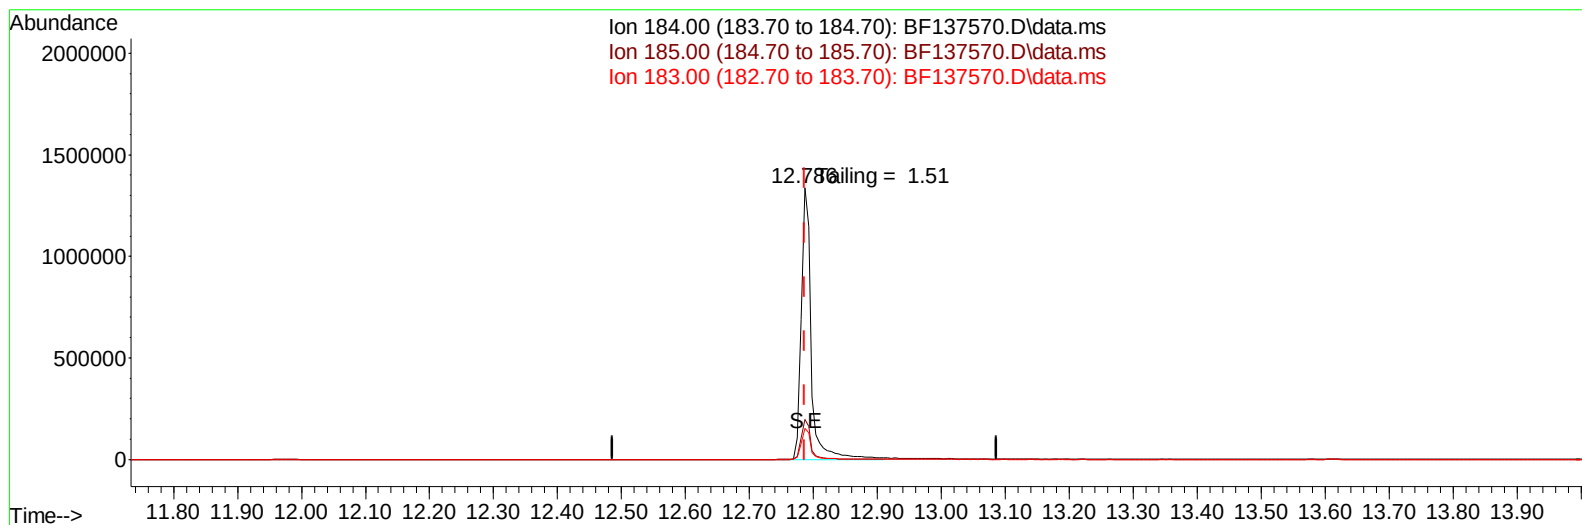

TIC: BF137570.D\data.ms

(77) Benzidine**12.786min (+ 0.000) 197956.36 ng****response 1492087**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.70
183.00	11.60	11.54
0.00	0.00	0.00