
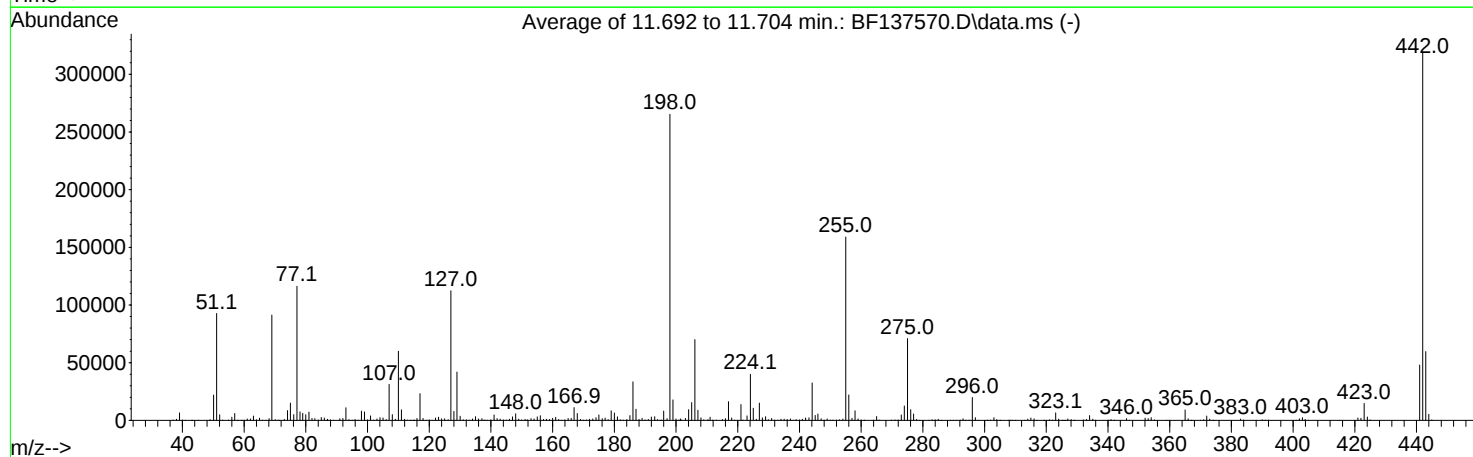


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031324\
Data File : BF137570.D
Acq On : 13 Mar 2024 08:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 04:02:20 2024

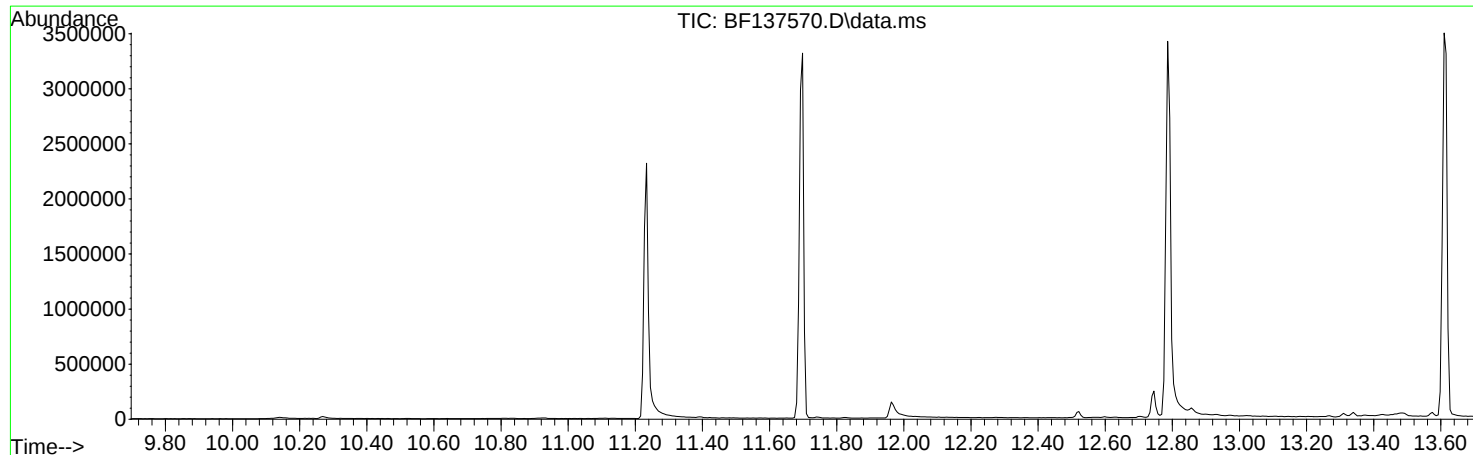




AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	92695	PASS
68	69	0.00	2	1.6	1477	PASS
69	198	0.00	100	34.4	91351	PASS
70	69	0.00	2	0.7	647	PASS
127	198	10	80	42.4	112445	PASS
197	198	0.00	2	0.6	1558	PASS
198	198	100	100	100.0	265360	PASS
199	198	5	9	6.7	17771	PASS
275	198	10	60	26.7	70845	PASS
365	198	1	100	3.4	9053	PASS
441	198	0.01	100	18.1	48035	PASS
442	442	50	100	100.0	318933	PASS
443	442	15	24	18.7	59616	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031324\
Data File : BF137570.D
Acq On : 13 Mar 2024 08:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 14 04:25:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 04:02:20 2024
Response via : Initial Calibration

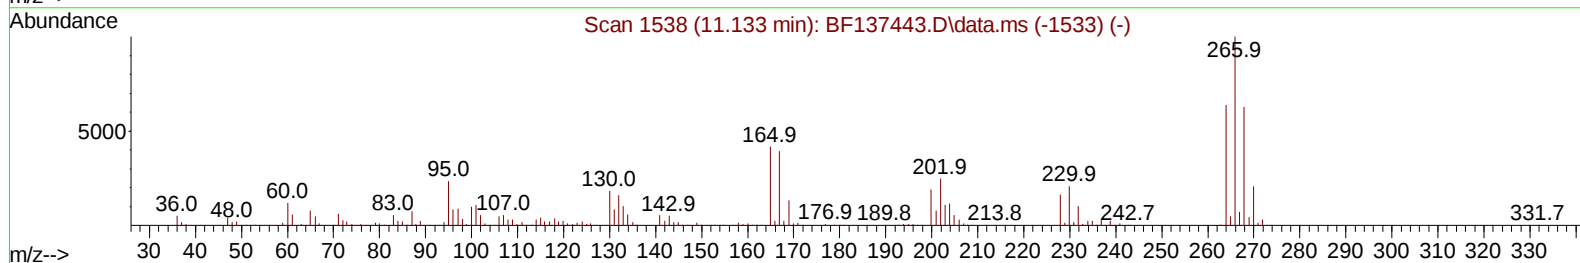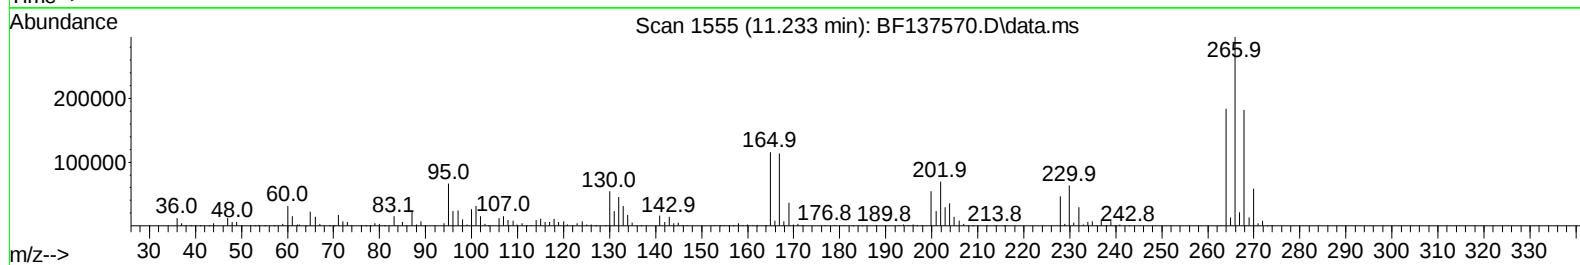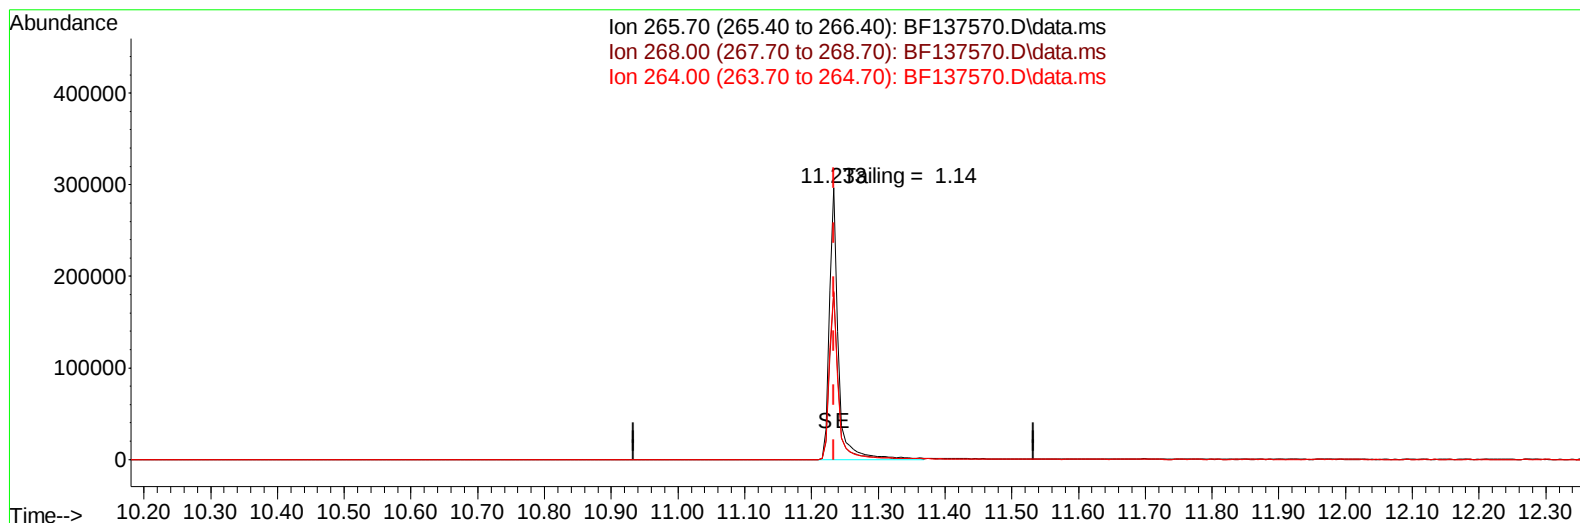

TIC: BF137570.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.000) 270605.16 ng

response 278936

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	61.38
264.00	63.60	62.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/13/2024	BNA_F	<u>BF137570.D</u>
Compound Name	Response	Retention Time
DDT	660951	13.616
DDD	12366	13.339
DDE	1055	12.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13421	674372	1.99

Instrument :
BNA_F
ClientSampleId :
DFTPP