
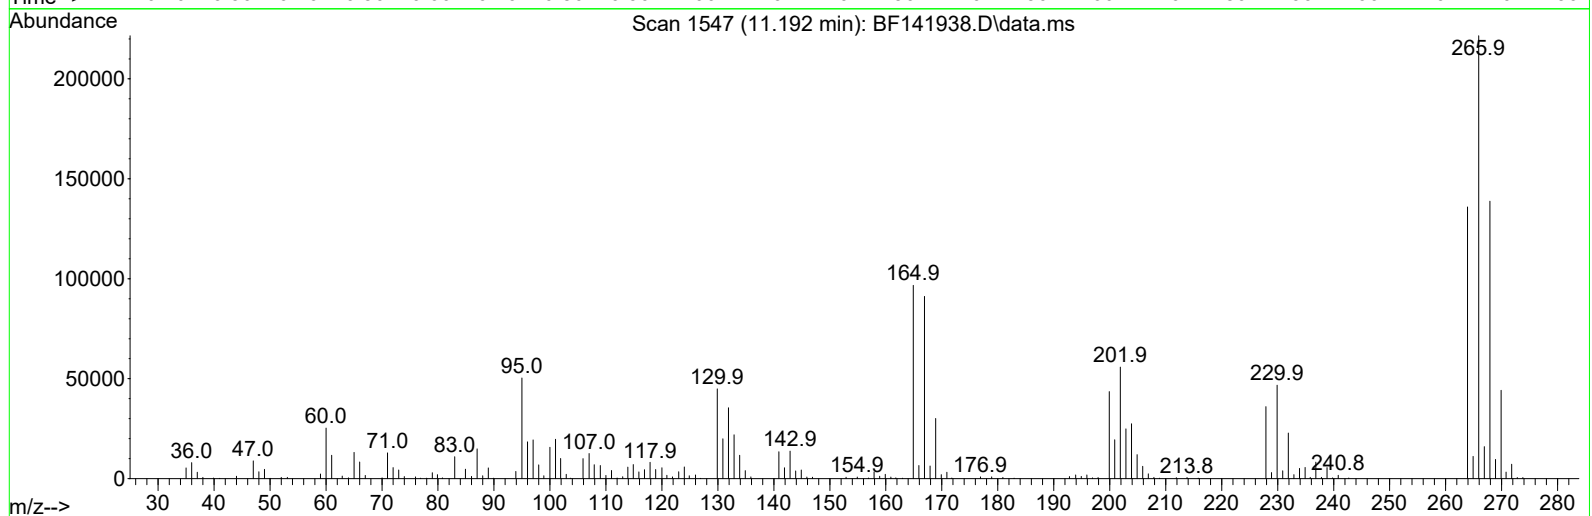


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031325\
Data File : BF141938.D
Acq On : 13 Mar 2025 11:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 13:04:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

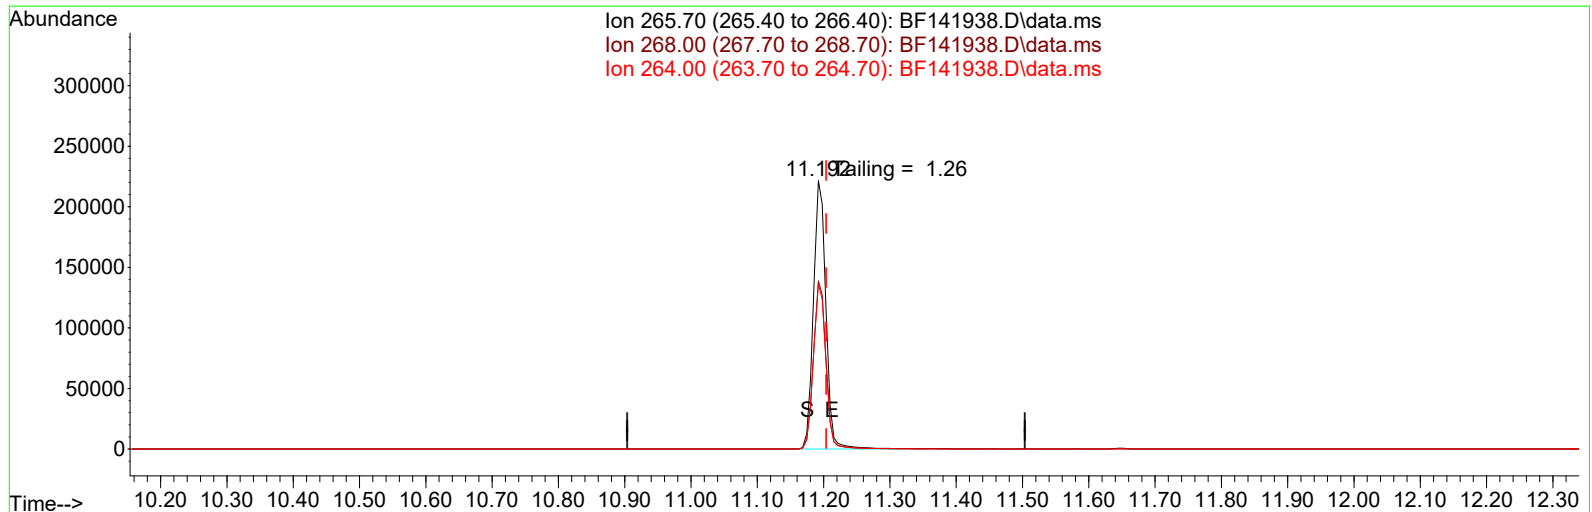

TIC: BF141938.D\data.ms

(70) Pentachlorophenol (C)



11.192min (-0.012) 133427.78 ng

response 291016

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.65
264.00	62.70	61.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031325\
Data File : BF141938.D
Acq On : 13 Mar 2025 11:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 13:04:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

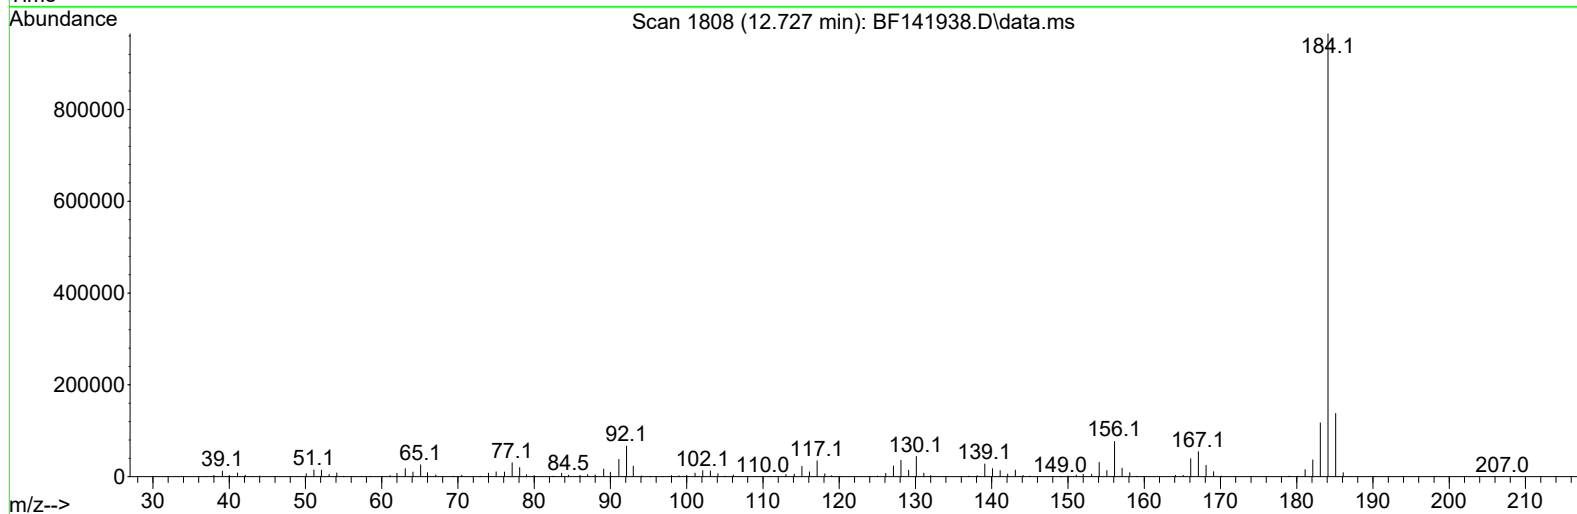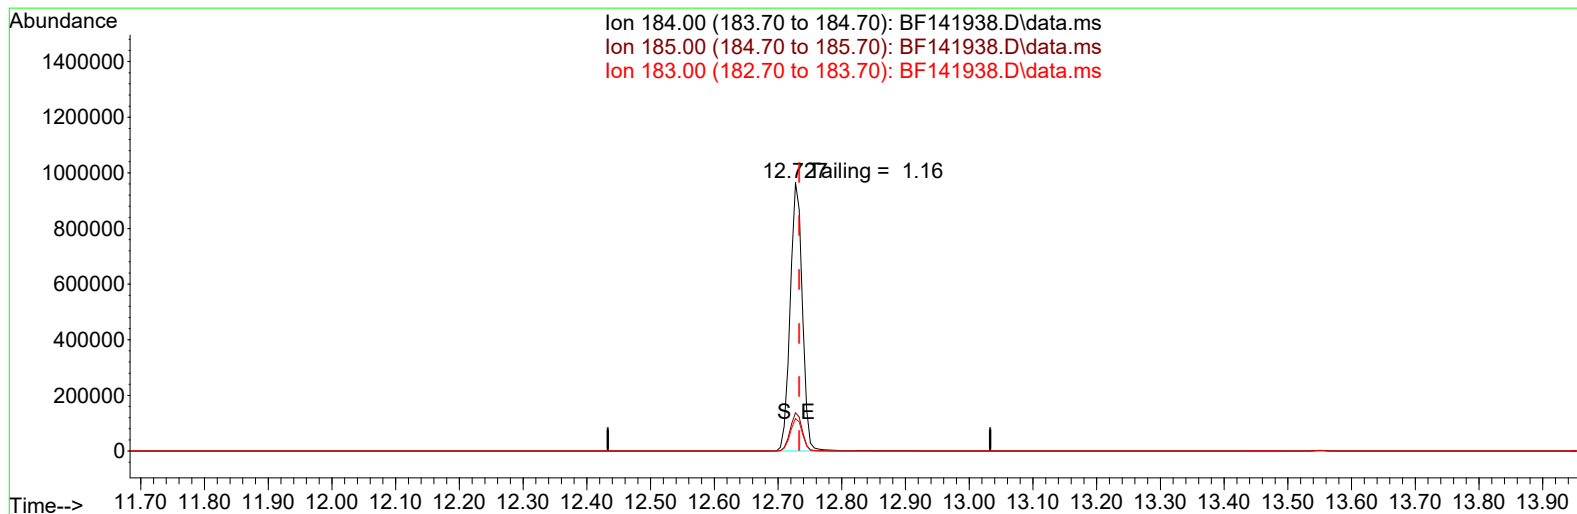

TIC: BF141938.D\data.ms

(77) Benzidine

12.727min (-0.006) 527010.30 ng

response 1286738

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.29
183.00	12.10	12.13
0.00	0.00	0.00