
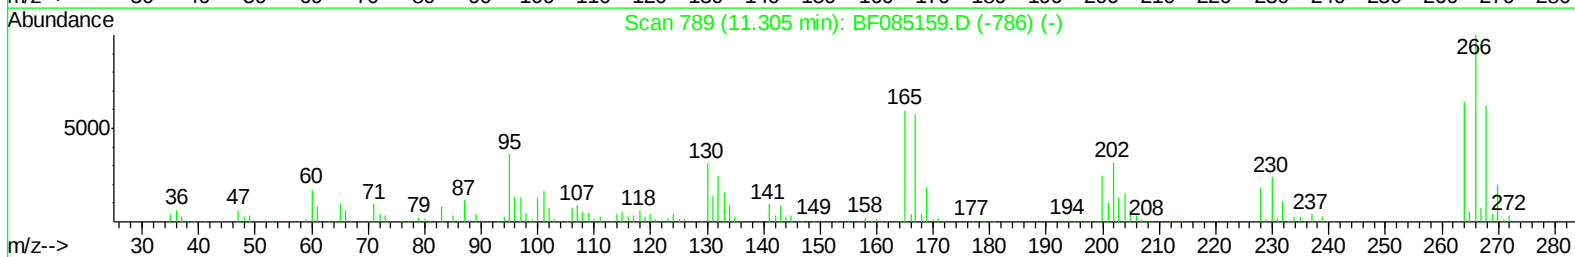
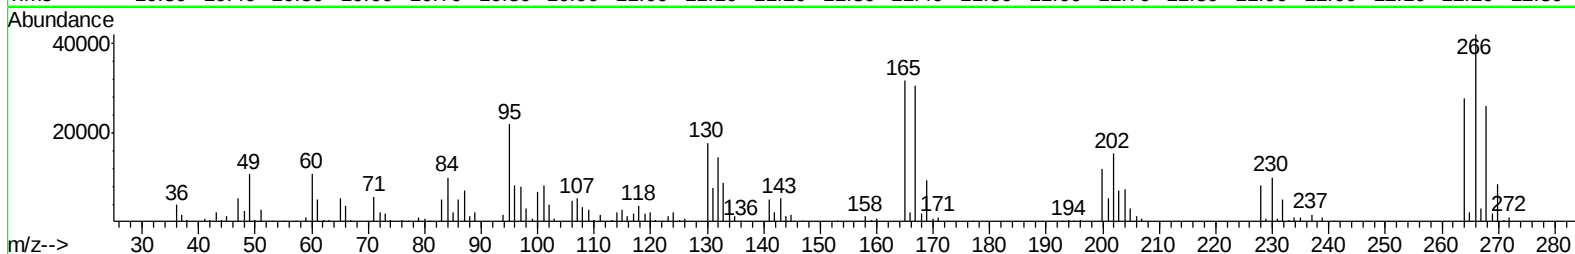


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
Data File : BF085419.D
Acq On : 14 Mar 2016 10:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 04:41:45 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

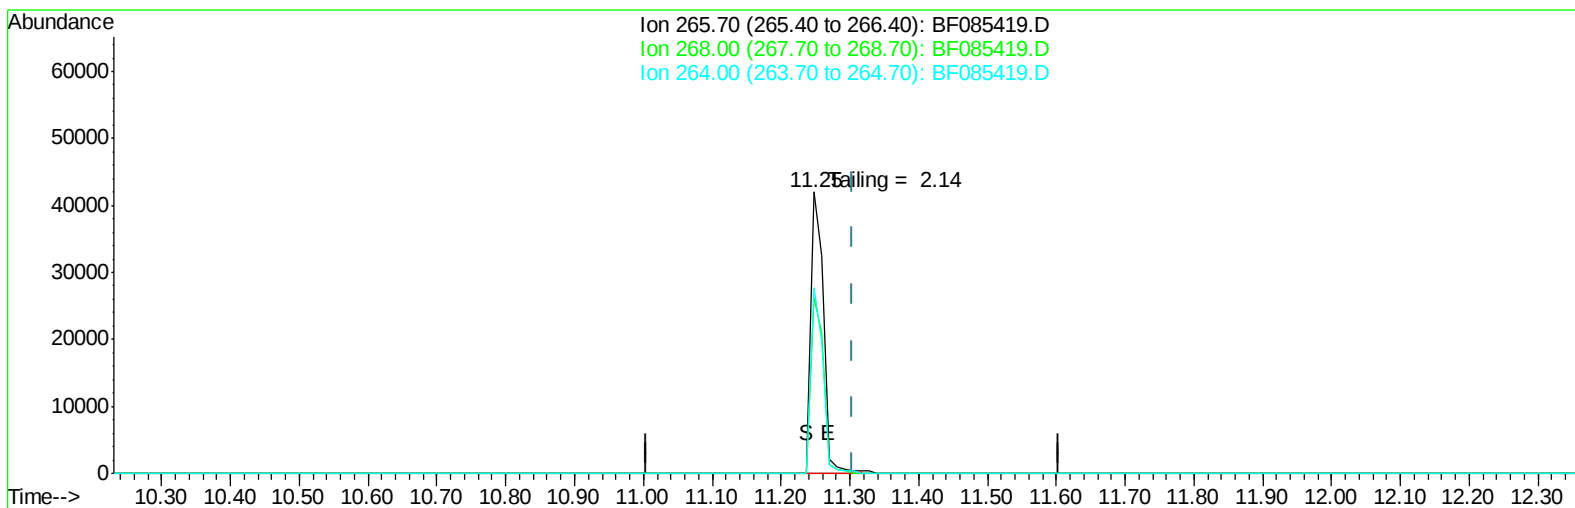

TIC: BF085419.D

(69) Pentachlorophenol (C)




11.248min (-0.057) 16947.69ng

response 54278

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	62.28
264.00	64.30	65.89
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
Data File : BF085419.D
Acq On : 14 Mar 2016 10:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 04:41:45 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

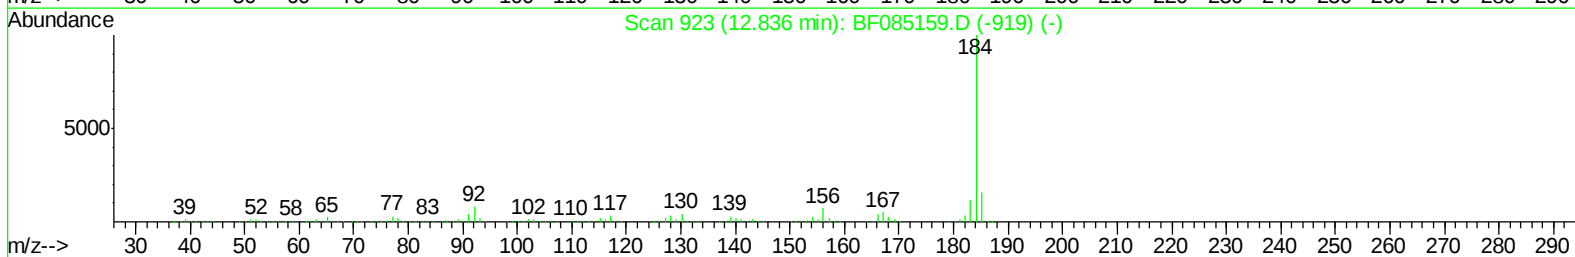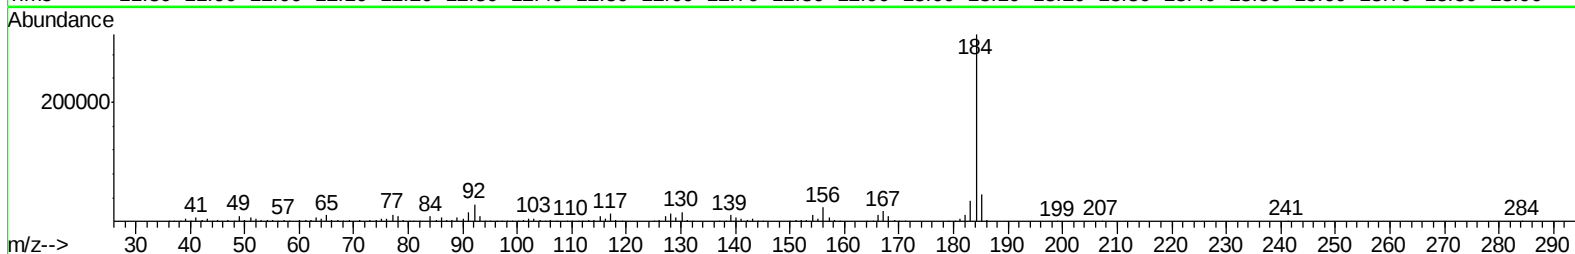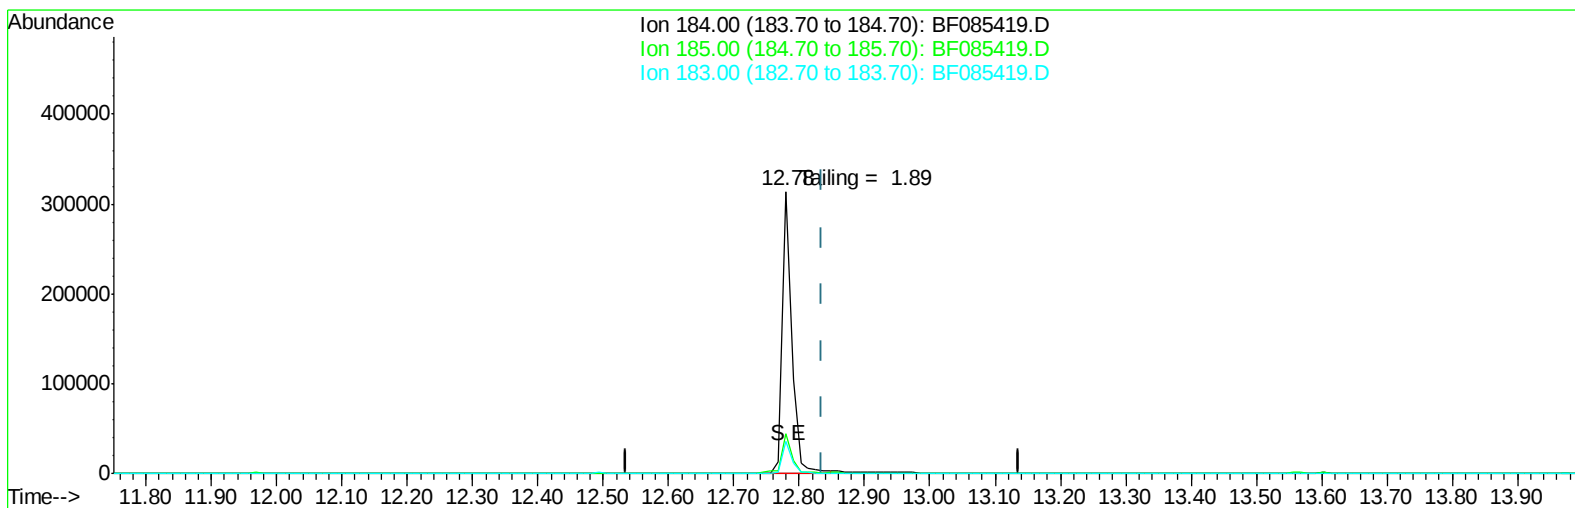

TIC: BF085419.D

(76) Benzidine

12.779min (-0.057) 0.00ng

response 324204

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.24
183.00	11.80	11.31
0.00	0.00	0.00