
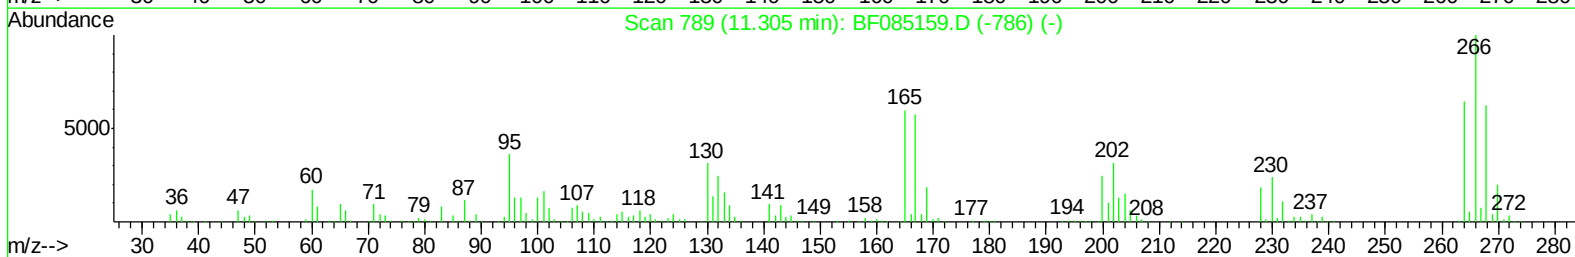
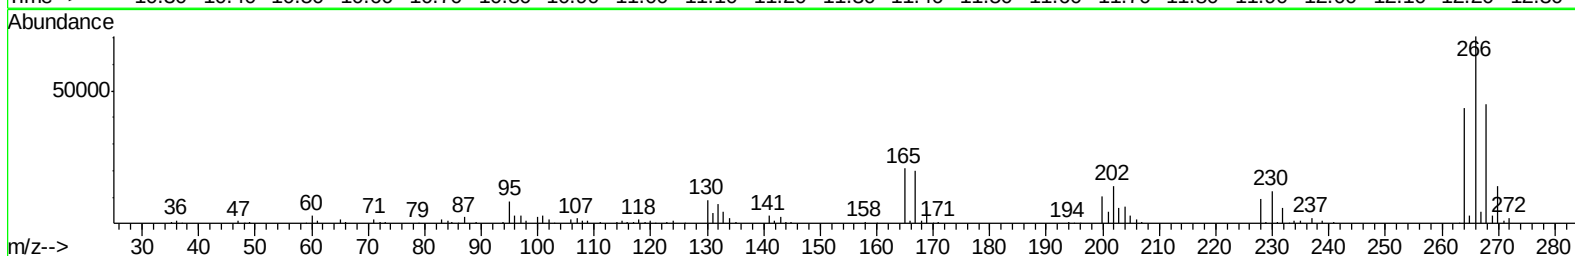


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
Data File : BF085445.D
Acq On : 15 Mar 2016 00:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 04:48:57 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

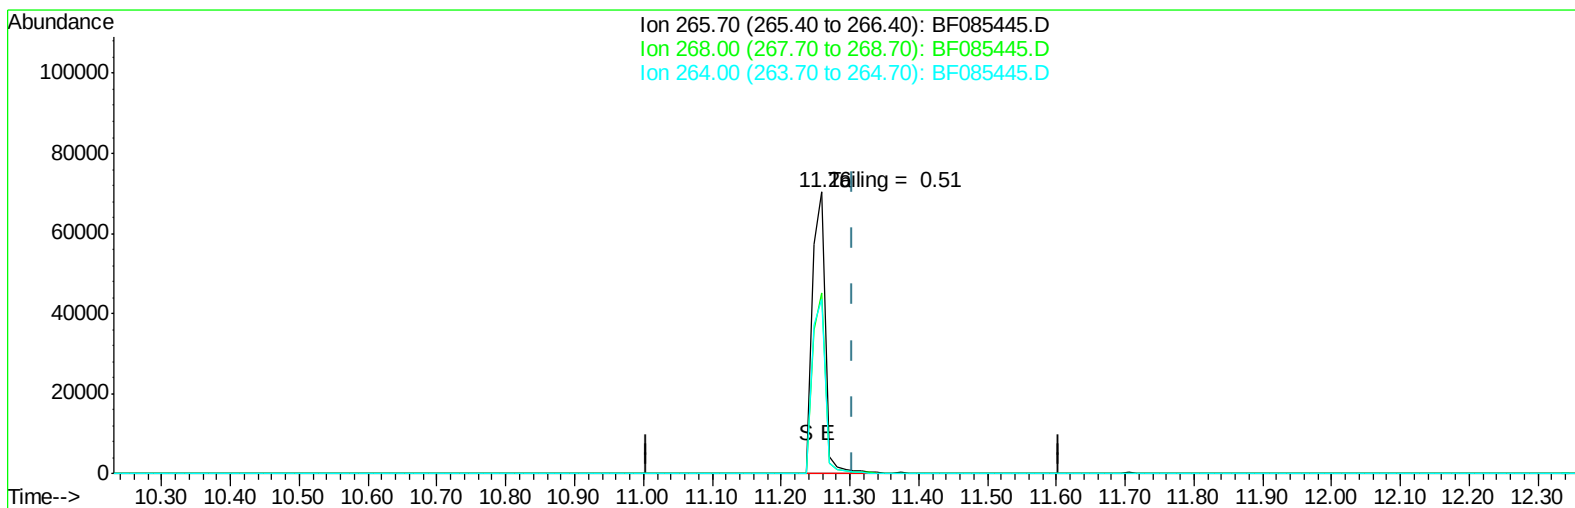

TIC: BF085445.D

(69) Pentachlorophenol (C)




11.259min (-0.046) 30003.24ng

response 93158

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	64.06
264.00	64.30	61.93
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\  
Data File : BF085445.D  
Acq On    : 15 Mar 2016  00:13  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Mar 15 04:48:57 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

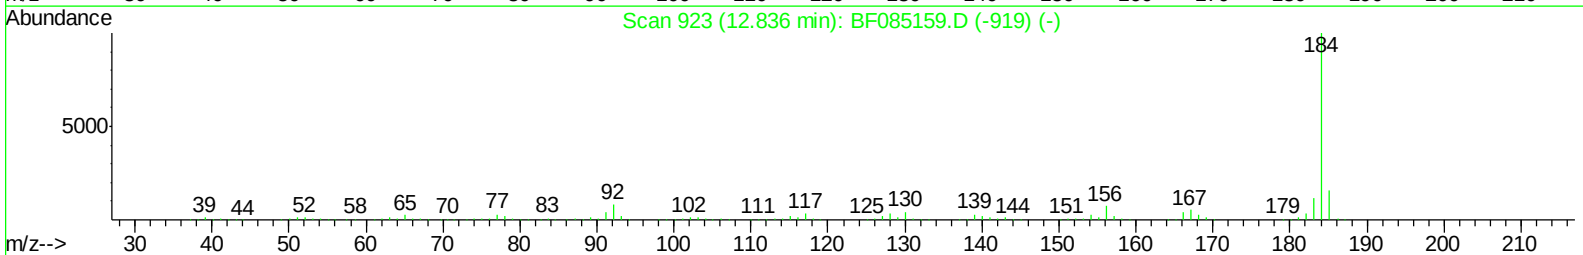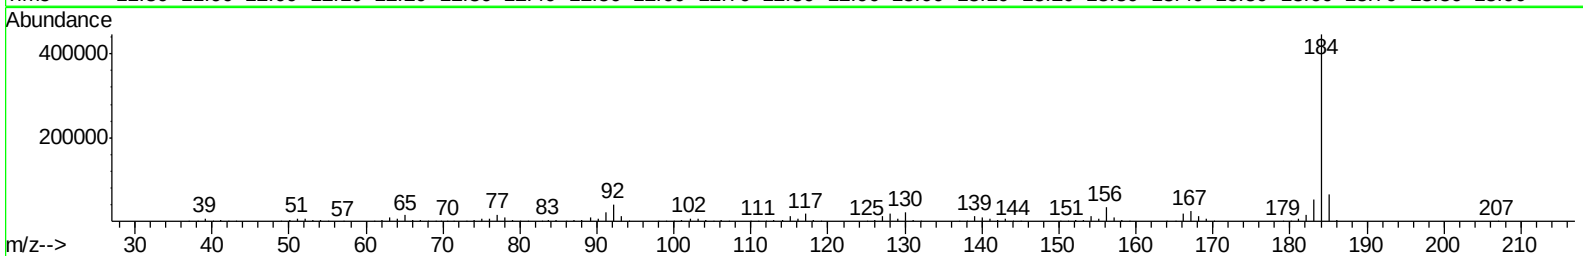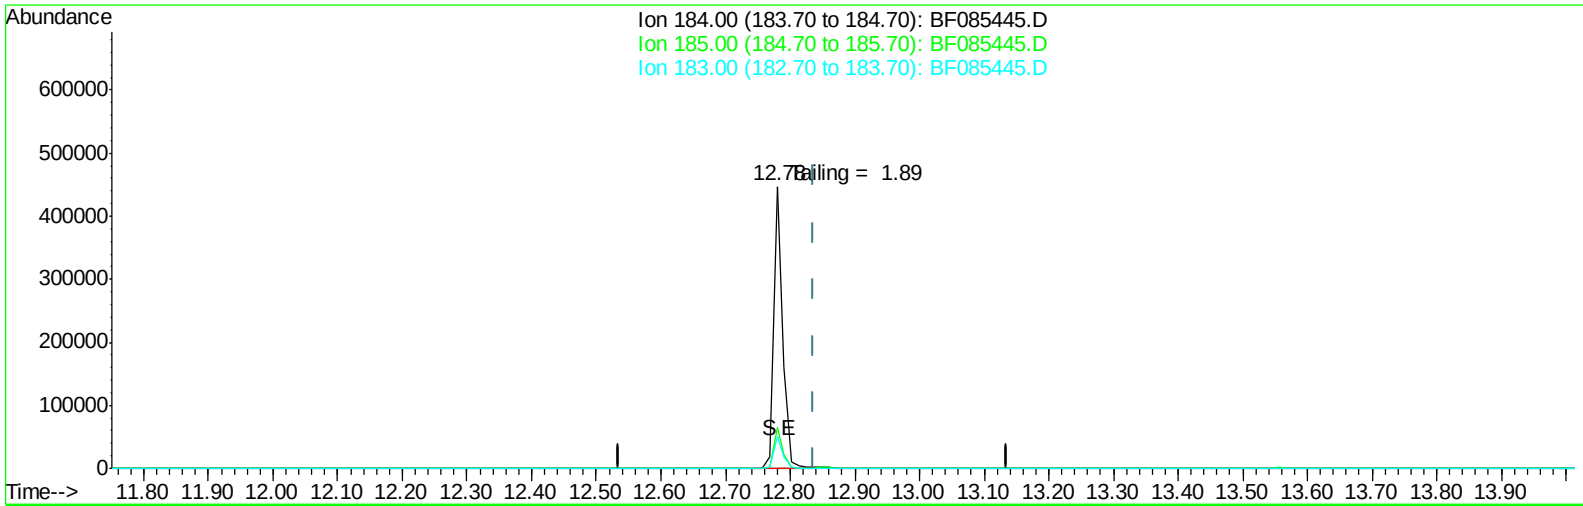

TIC: BF085445.D

(76) Benzidine

12.779min (-0.057) 0.00ng

response 447009

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.65
183.00	11.80	11.57
0.00	0.00	0.00