

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
 Data File : BF085425.D
 Acq On : 14 Mar 2016 13:29
 Operator : UM/SJ
 Sample : H1744-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	245	247	252	rVB	87040	120513	2.07%	0.335%
2	5.521	280	283	286	rBV	2230862	2068728	35.52%	5.746%
3	6.550	370	373	375	rBV	1074908	1395687	23.97%	3.877%
4	6.687	382	385	388	rBV	3462828	3628082	62.30%	10.078%
5	6.916	403	405	408	rBV	816113	1034191	17.76%	2.873%
6	7.076	417	419	422	rVB	3022730	3606377	61.93%	10.018%
7	7.487	452	455	457	rBV	2728581	3006579	51.63%	8.352%
8	8.207	515	518	520	rBV	1771120	1469403	25.23%	4.082%
9	9.293	609	613	615	rBV	4416678	5823368	100.00%	16.176%
10	9.968	669	672	674	rBV	1732567	1635895	28.09%	4.544%
11	10.756	738	741	743	rBV	3276188	3321707	57.04%	9.227%
12	11.454	799	802	804	rBV	1453953	1638958	28.14%	4.553%
13	13.042	938	941	943	rBV	4554601	5388890	92.54%	14.969%
14	14.082	1030	1032	1035	rBV	1134587	1087696	18.68%	3.021%
15	15.534	1157	1159	1162	rBV	488407	774097	13.29%	2.150%


Sum of corrected areas: 36000171

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
Data File : BF085425.D
Acq On : 14 Mar 2016 13:29
Operator : UM/SJ
Sample : H1744-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-4

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

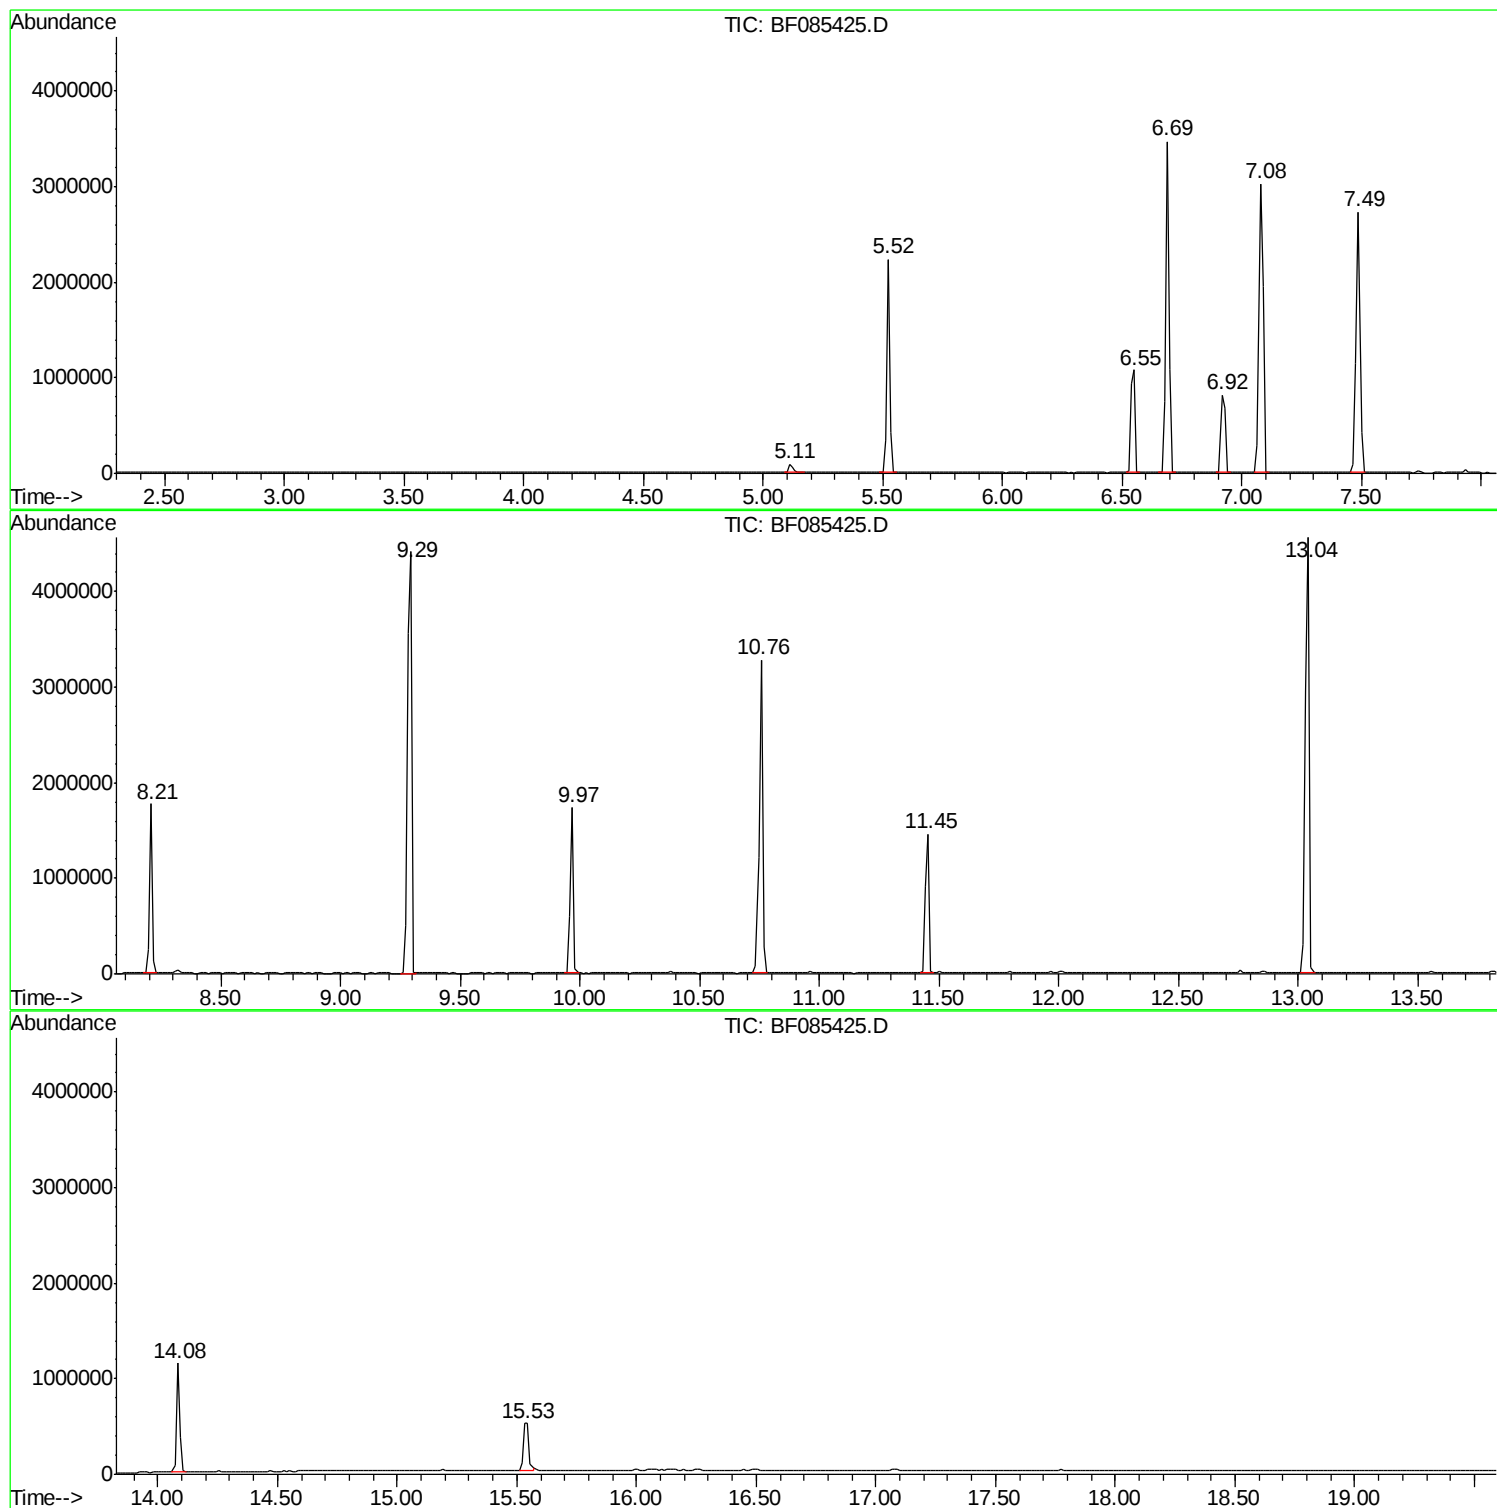

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
Data File : BF085425.D
Acq On : 14 Mar 2016 13:29
Operator : UM/SJ
Sample : H1744-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-4









Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.11	2.33 ng	120513	1,4-Dichlorobenzene-d4	6.93

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56	
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	27	
3	Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	23	
4	5-Hexen-2-one	98	C6H10O	000109-49-9	9	
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9	

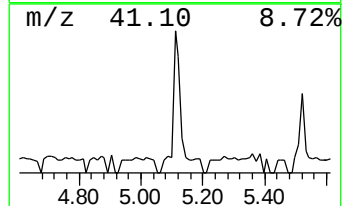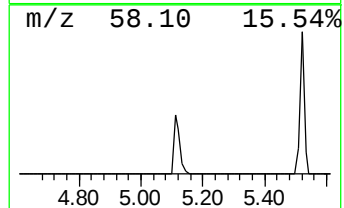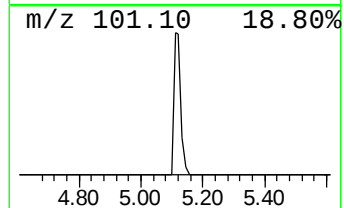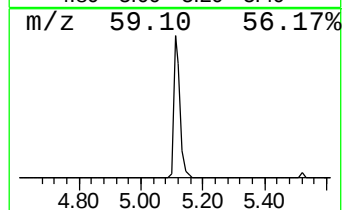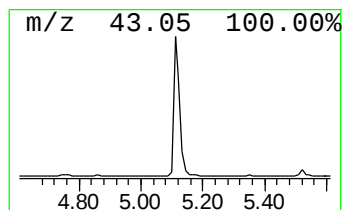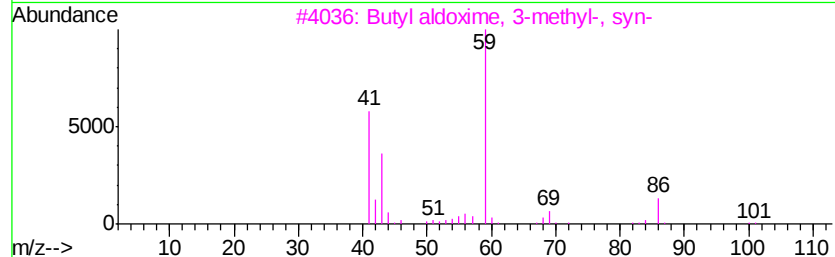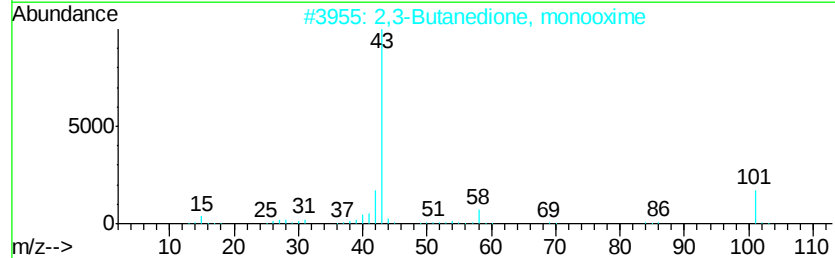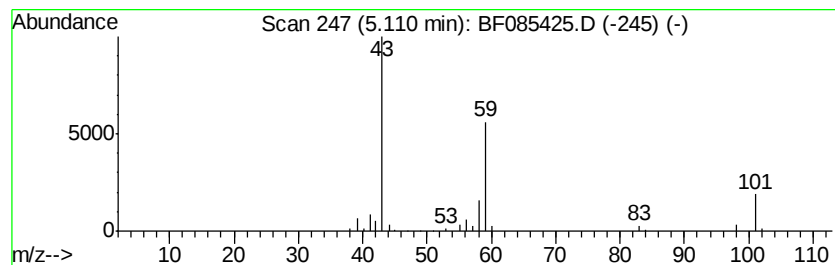

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
Data File : BF085425.D
Acq On : 14 Mar 2016 13:29
Operator : UM/SJ
Sample : H1744-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-4

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.11	2.3	ng	120513	1	6.93	1034190	20.0