

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
 Data File : BF085438.D
 Acq On : 14 Mar 2016 19:34
 Operator : UM/SJ
 Sample : PB88851BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB88851BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.144	247	250	255	rBV	180550	302187	6.09%	0.775%
2	5.533	281	284	287	rBV	3055703	4256737	85.85%	10.914%
3	6.562	370	374	376	rBV	2947569	4479031	90.34%	11.484%
4	6.687	382	385	388	rBV	3305325	4314378	87.02%	11.062%
5	6.916	403	405	408	rBV	790363	1006959	20.31%	2.582%
6	7.076	417	419	422	rBV	3096424	3336971	67.30%	8.556%
7	7.487	452	455	457	rBV	2759292	2900209	58.49%	7.436%
8	8.208	515	518	520	rBV	1624699	1421790	28.68%	3.646%
9	9.282	609	612	615	rBV	3717070	4958061	100.00%	12.713%
10	9.968	669	672	674	rBV	1363369	1481934	29.89%	3.800%
11	10.756	738	741	743	rBV	2925812	2968155	59.87%	7.610%
12	11.454	799	802	804	rBV	1157687	1428154	28.80%	3.662%
13	13.042	938	941	943	rBV	3373917	4491364	90.59%	11.516%
14	14.082	1030	1032	1035	rBV	960383	879949	17.75%	2.256%
15	15.545	1156	1160	1162	rBV	499552	775102	15.63%	1.987%


Sum of corrected areas: 39000981

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
Data File : BF085438.D
Acq On : 14 Mar 2016 19:34
Operator : UM/SJ
Sample : PB88851BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88851BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

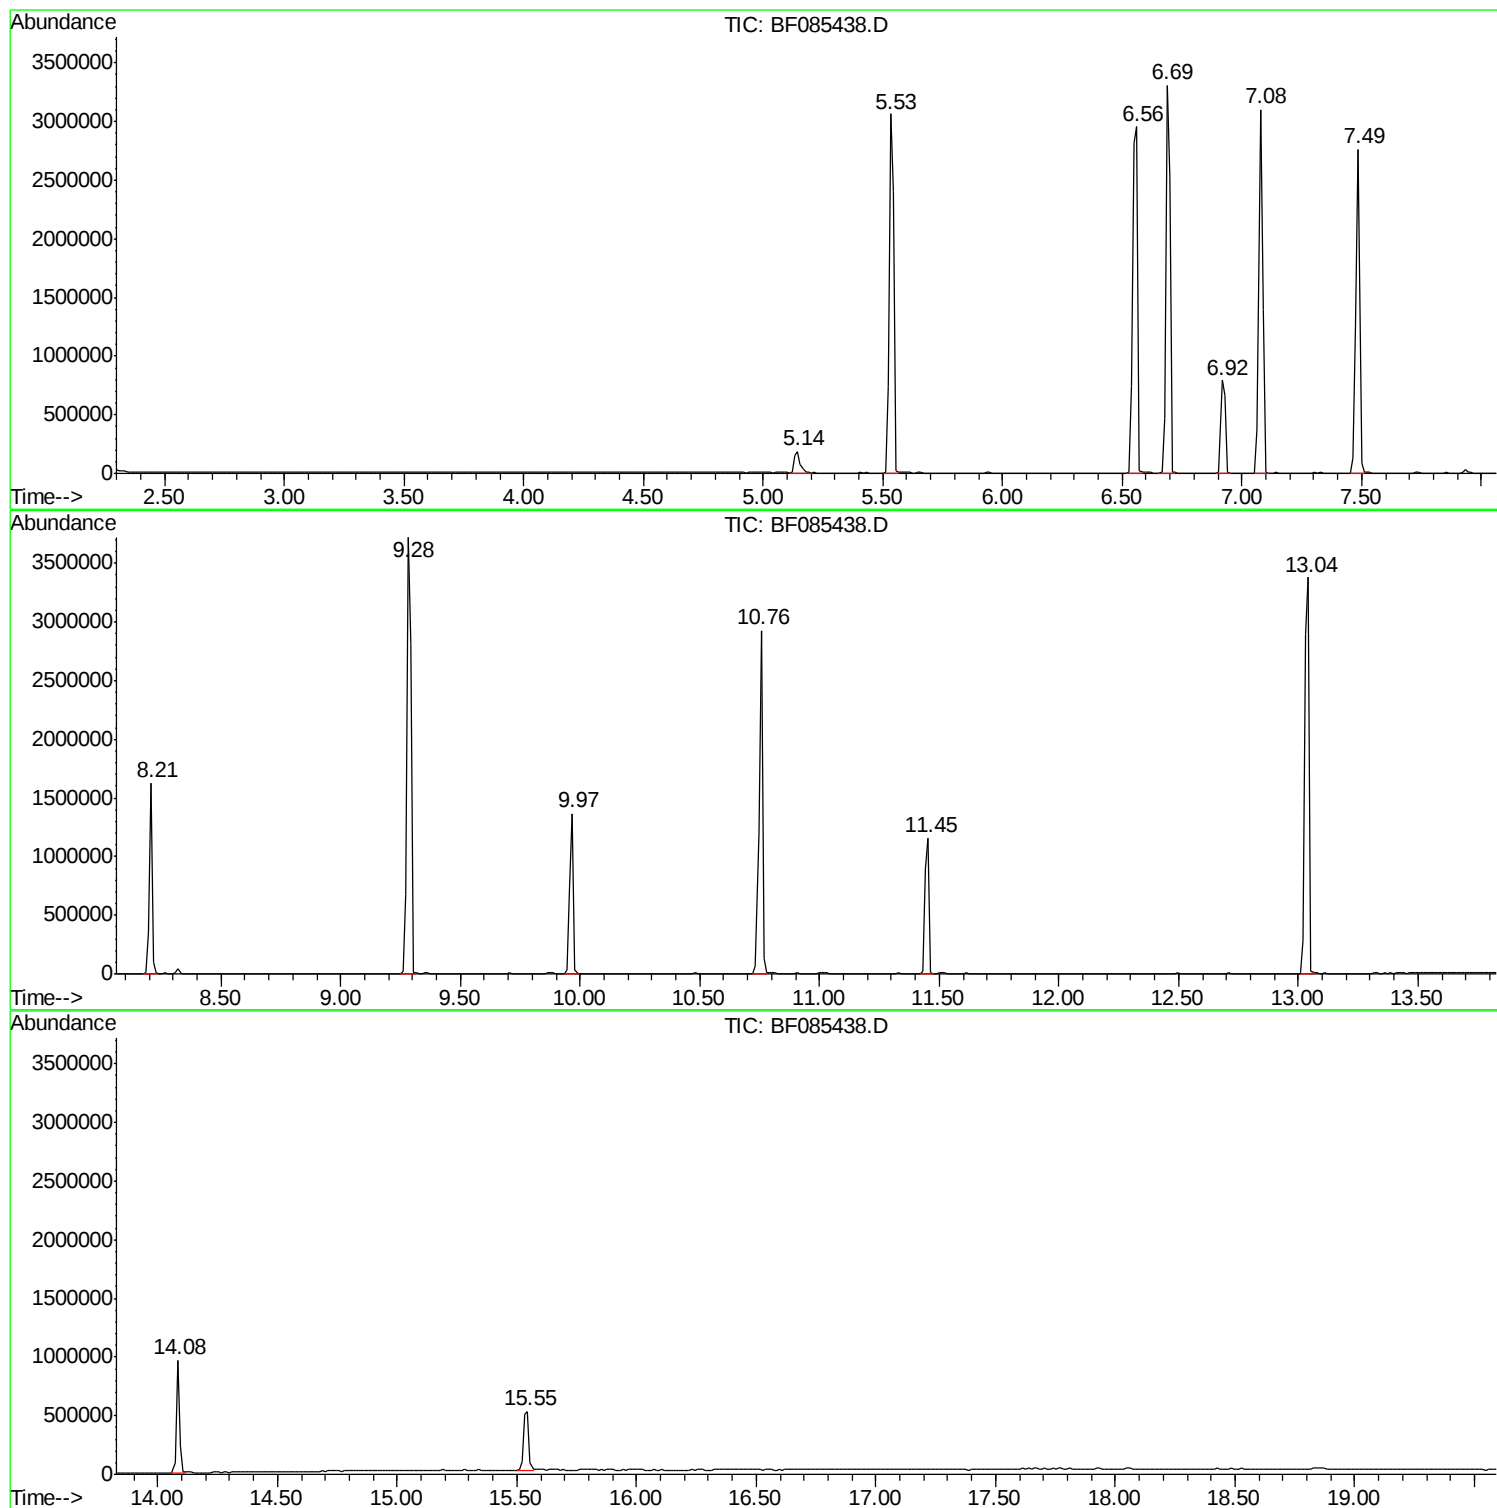

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
Data File : BF085438.D
Acq On : 14 Mar 2016 19:34
Operator : UM/SJ
Sample : PB88851BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88851BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.14	6.00 ng	302187	1,4-Dichlorobenzene-d4	6.93

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25
3			(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9
4			5-Hexen-2-one	98	C6H10O	000109-49-9	9
5			Acetone	58	C3H6O	000067-64-1	9

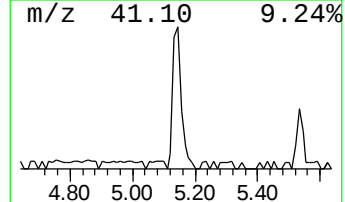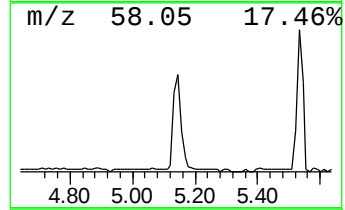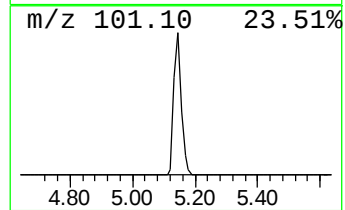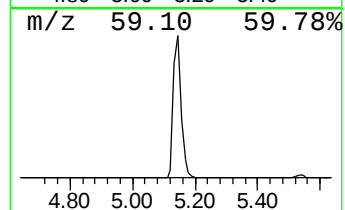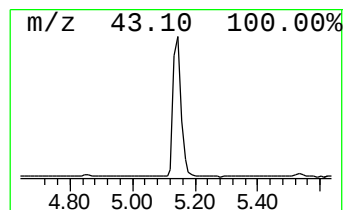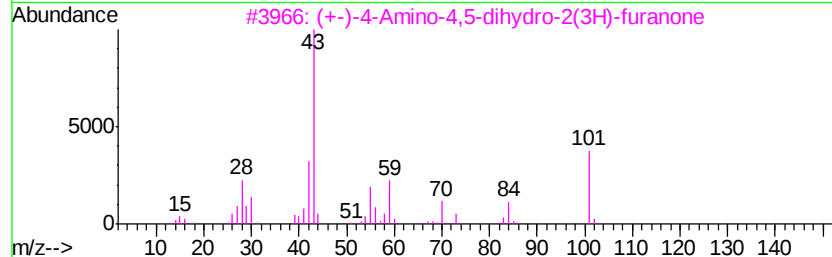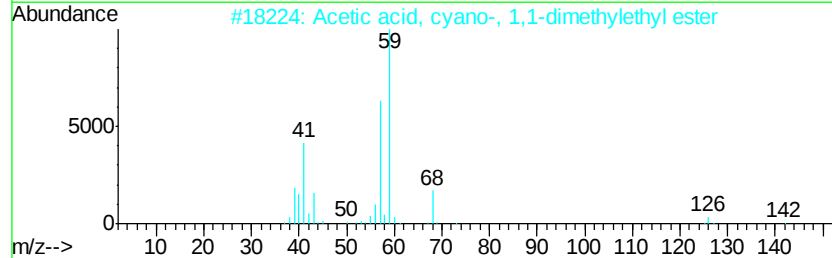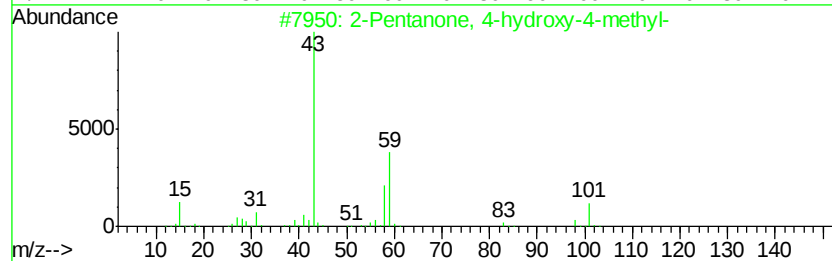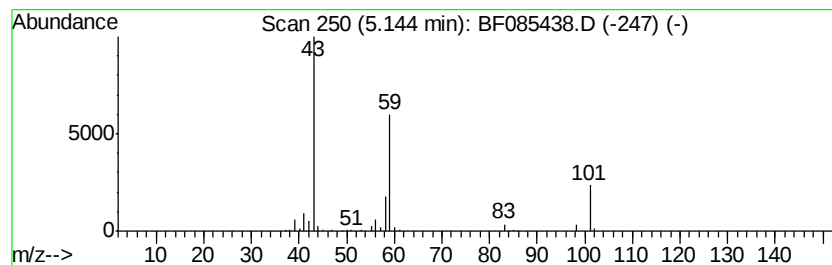

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
Data File : BF085438.D
Acq On : 14 Mar 2016 19:34
Operator : UM/SJ
Sample : PB88851BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88851BL







Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.69 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.69	85.69 ng	4314380	1,4-Dichlorobenzene-d4	6.93

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4			4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

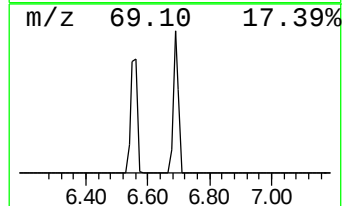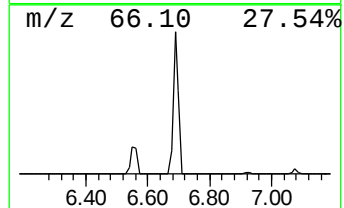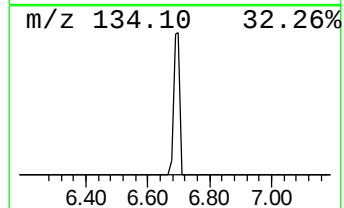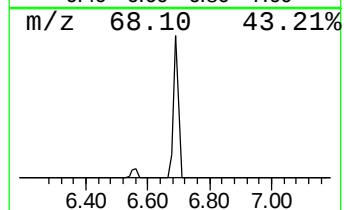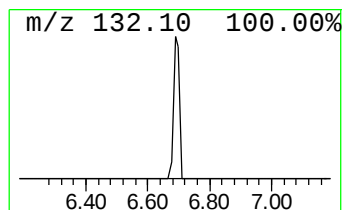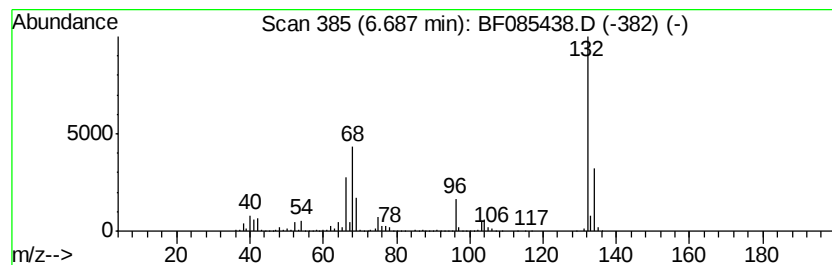

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
Data File : BF085438.D
Acq On : 14 Mar 2016 19:34
Operator : UM/SJ
Sample : PB88851BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88851BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.14	6.0	ng	302187	1	6.93	1006960	20.0
unknown6.69	6.69	85.7	ng	4314380	1	6.93	1006960	20.0