


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
 Data File : BF085419.D
 Acq On : 14 Mar 2016 10:37
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 04 00:54:58 2016

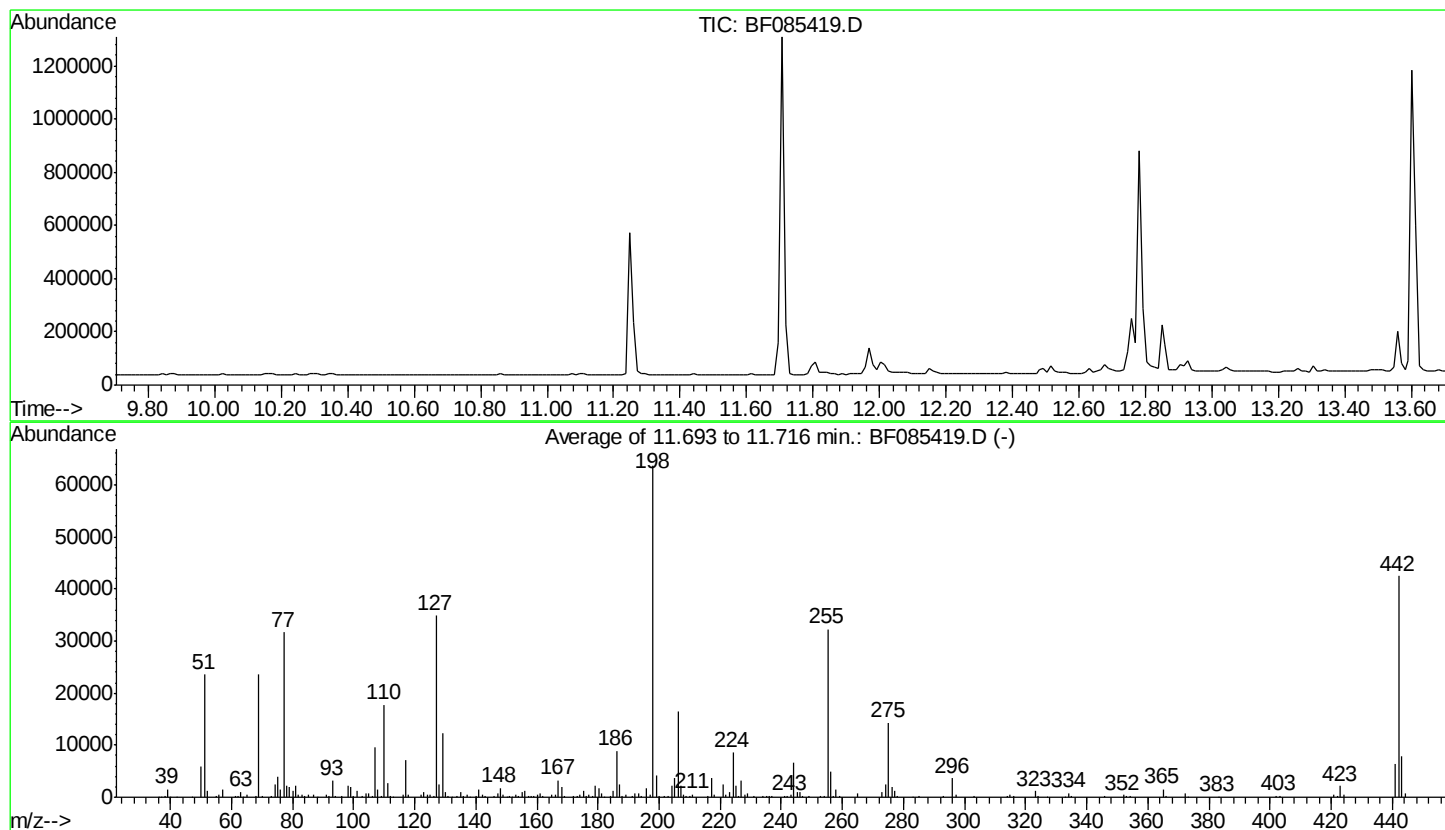

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	23486	PASS
68	69	0.00	2	1.5	344	PASS
69	198	0.00	100	37.1	23629	PASS
70	69	0.00	2	0.7	166	PASS
127	198	10	80	54.7	34822	PASS
197	198	0.00	2	0.7	441	PASS
198	198	100	100	100.0	63665	PASS
199	198	5	9	6.6	4176	PASS
275	198	10	60	22.5	14344	PASS
365	198	1	100	2.4	1549	PASS
441	442	0.01	24	15.3	6478	PASS
442	198	50	100	66.7	42473	PASS
443	442	15	24	18.8	7987	PASS