


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031416\
 Data File : BF085445.D
 Acq On : 15 Mar 2016 00:13
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 04 00:54:58 2016

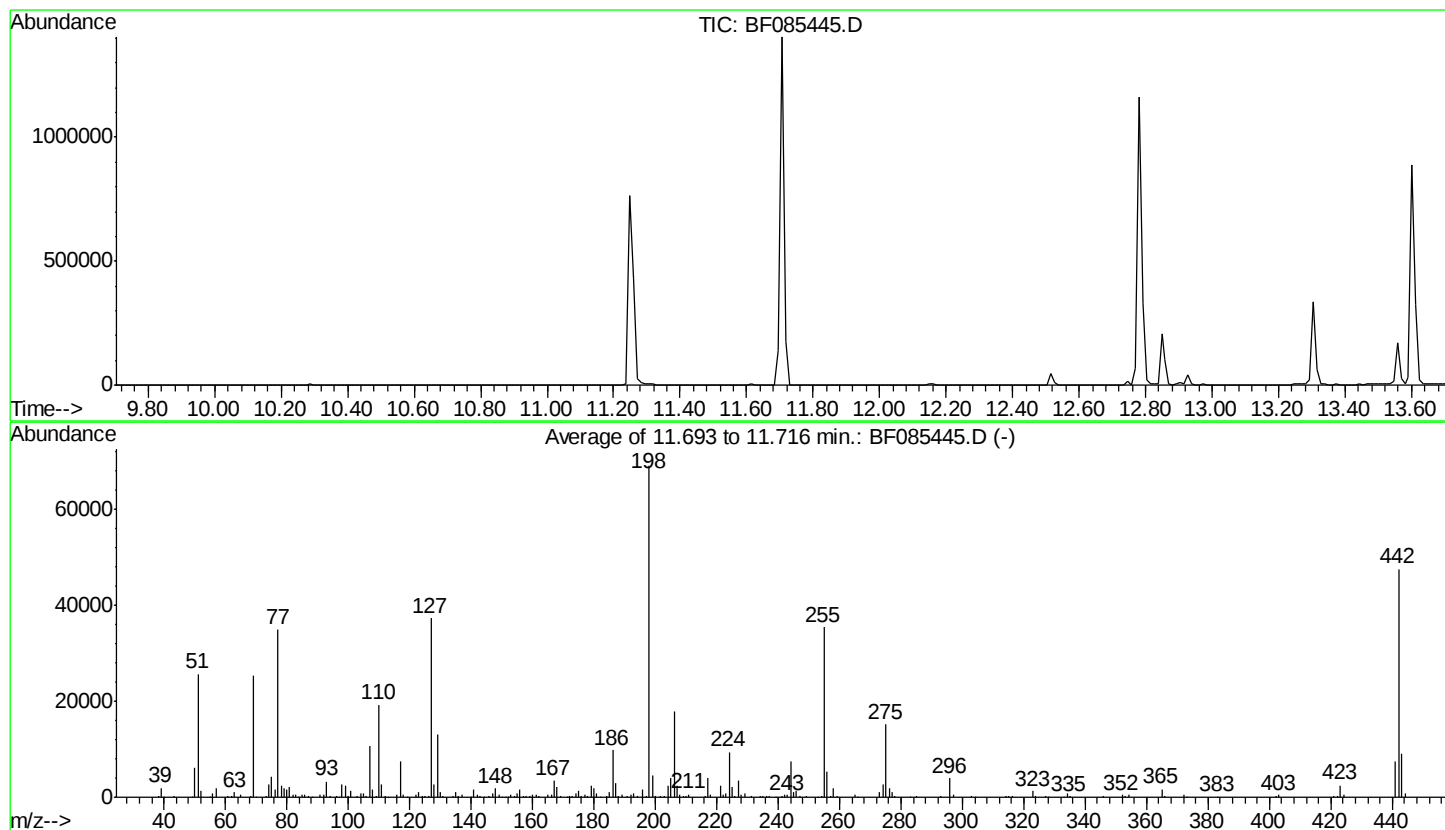

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	25739	PASS
68	69	0.00	2	1.3	338	PASS
69	198	0.00	100	36.7	25399	PASS
70	69	0.00	2	0.5	138	PASS
127	198	10	80	54.0	37337	PASS
197	198	0.00	2	0.6	402	PASS
198	198	100	100	100.0	69121	PASS
199	198	5	9	6.7	4604	PASS
275	198	10	60	21.9	15149	PASS
365	198	1	100	2.5	1732	PASS
441	442	0.01	24	15.5	7367	PASS
442	198	50	100	68.8	47538	PASS
443	442	15	24	19.3	9187	PASS