
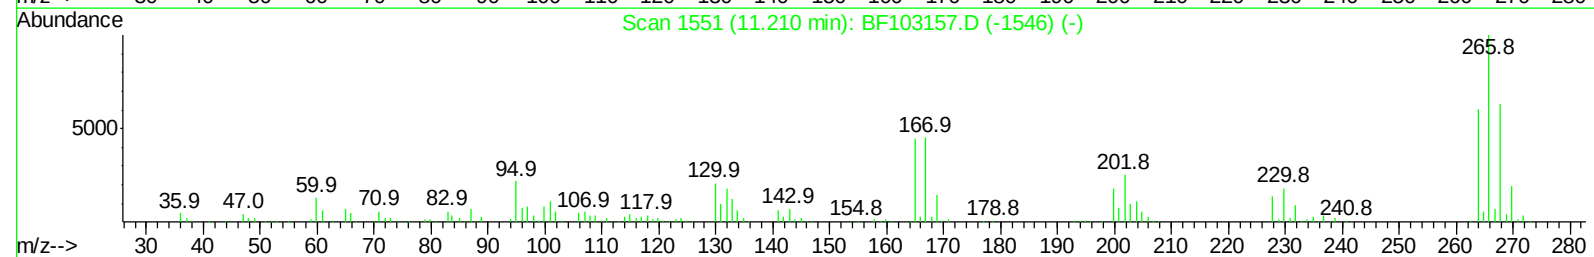
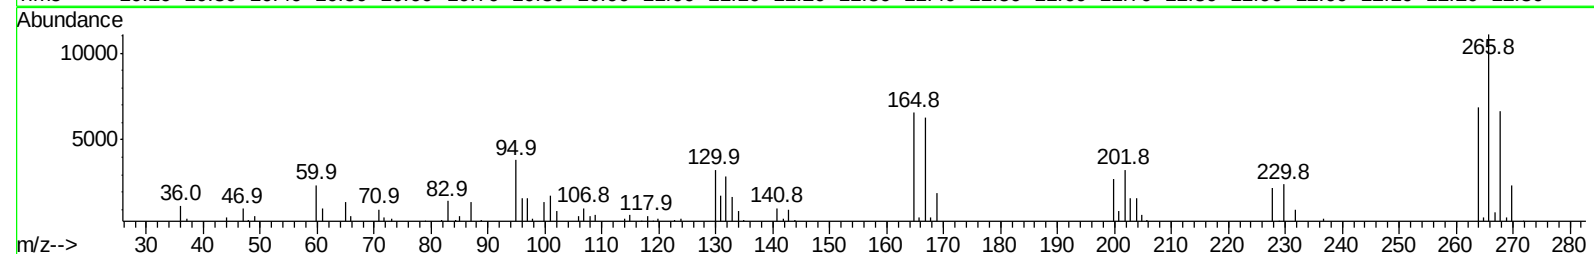


Data Path : Z:\HPCHEM1\BNA F\DATA\BF031418\
Data File : BF103636.D
Acq On : 14 Mar 2018 12:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 04:29:01 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 14 18:08:29 2018
Response via : Initial Calibration

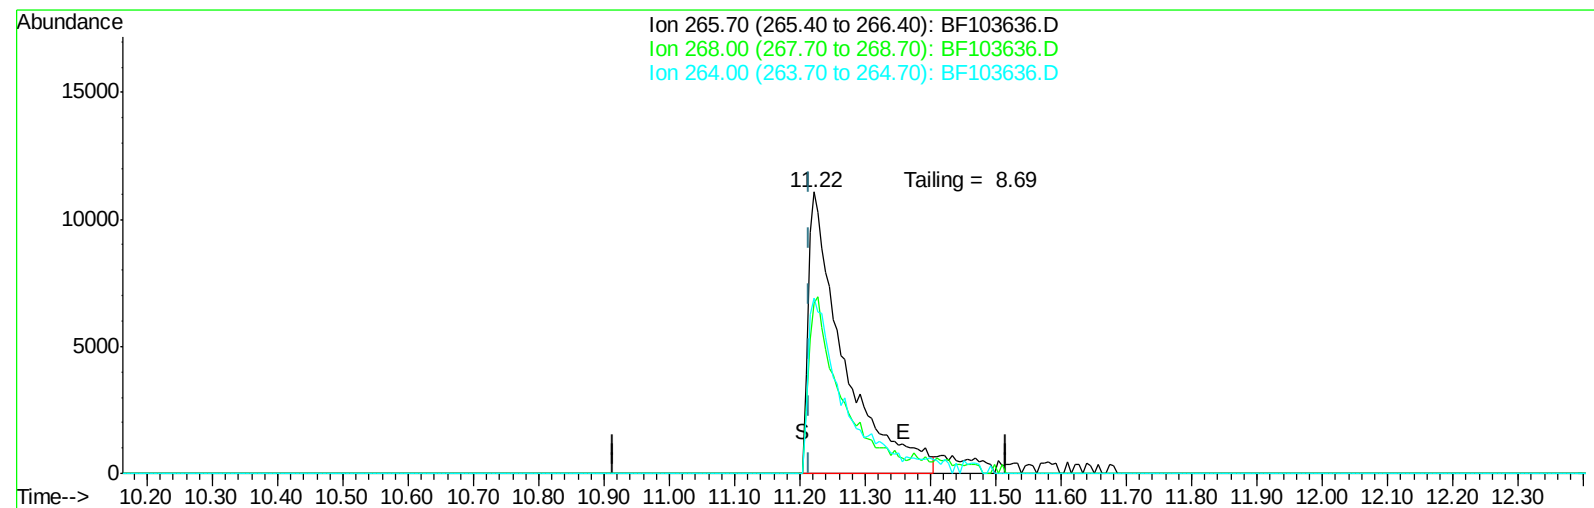

TIC: BF103636.D

(69) Pentachlorophenol (C)




11.222min (+0.006) 33085.78ng

response 41602

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.25
264.00	61.90	67.26
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031418\
Data File : BF103636.D
Acq On : 14 Mar 2018 12:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 04:29:01 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 14 18:08:29 2018
Response via : Initial Calibration

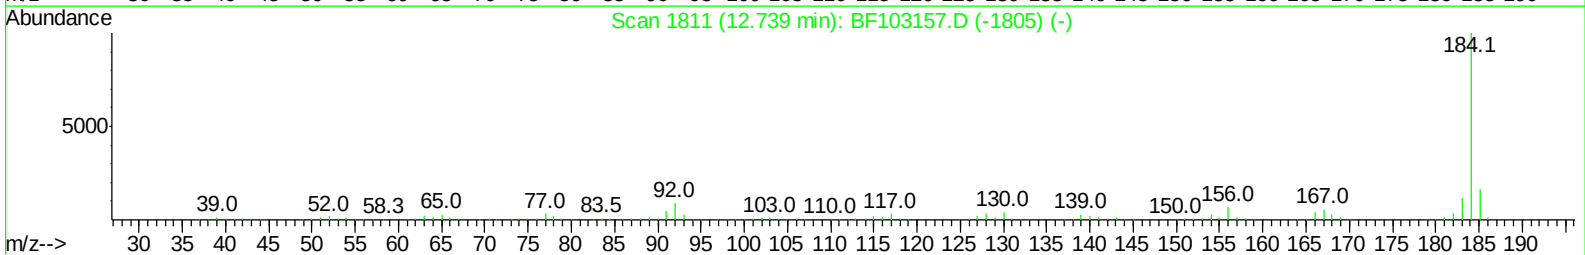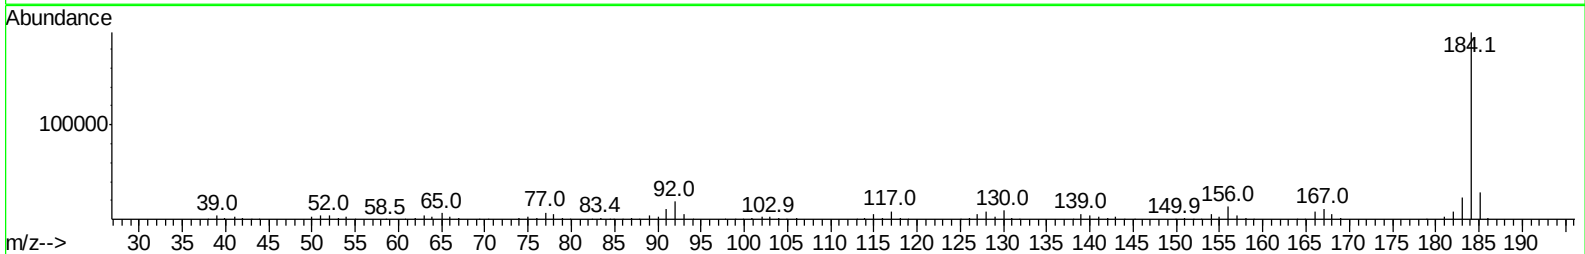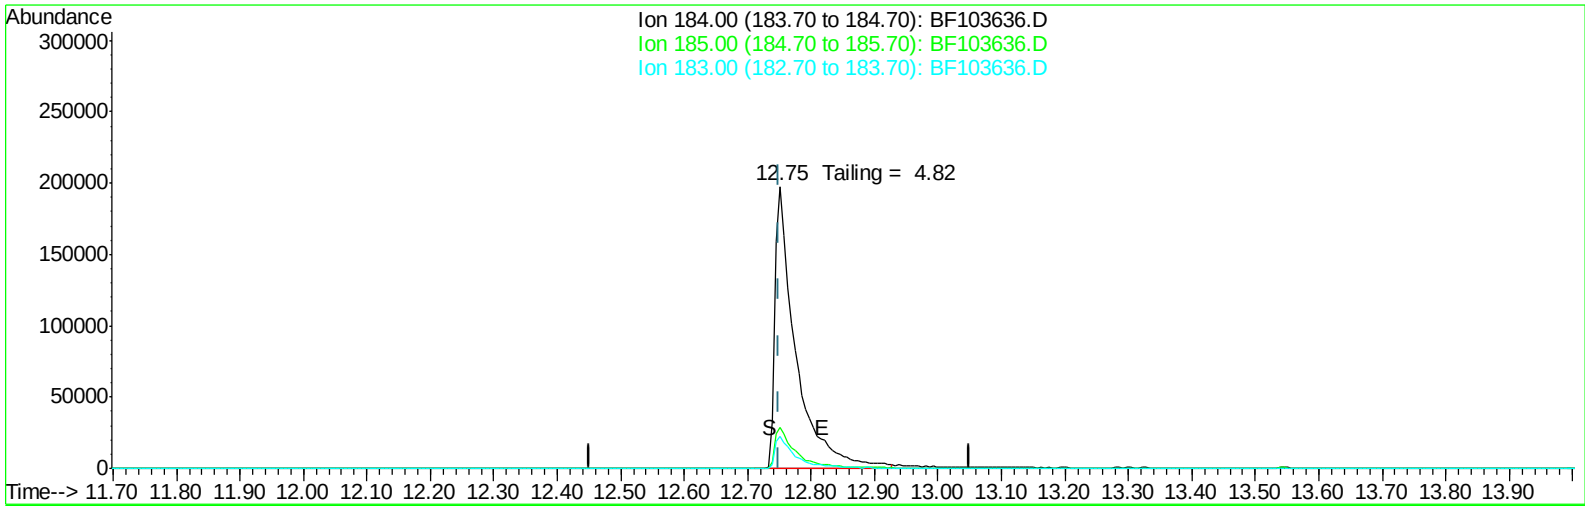

TIC: BF103636.D

(76) Benzidine

12.751min (+0.000) 0.00ng

response 454112

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.55
183.00	11.60	11.55
0.00	0.00	0.00