


Data Path : Z:\HPCHEM1\BNA F\Data\BF031418\
 Data File : BF103636.D
 Acq On : 14 Mar 2018 12:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 14 18:08:29 2018

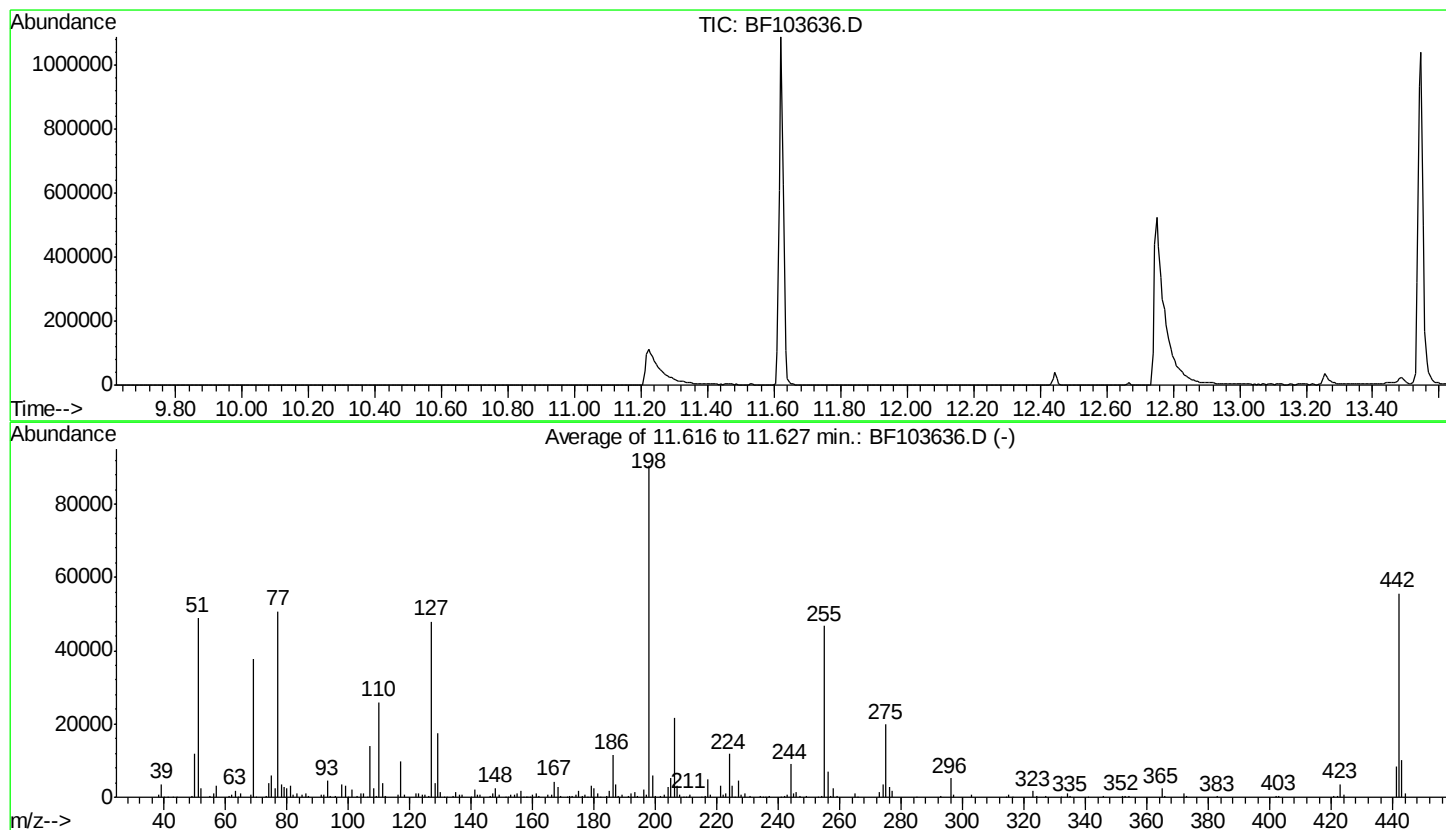

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.1	48992	PASS
68	69	0.00	2	1.5	576	PASS
69	198	0.00	100	41.9	37888	PASS
70	69	0.00	2	0.4	136	PASS
127	198	10	80	53.0	47978	PASS
197	198	0.00	2	0.7	665	PASS
198	198	100	100	100.0	90482	PASS
199	198	5	9	6.6	5944	PASS
275	198	10	60	21.9	19792	PASS
365	198	1	100	2.6	2387	PASS
441	443	0.01	100	84.0	8421	PASS
442	198	50	100	61.6	55693	PASS
443	442	15	24	18.0	10021	PASS