


Data Path : Z:\HPCHEM1\BNA F\Data\BF031418\
 Data File : BF103661.D
 Acq On : 15 Mar 2018 00:52
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 14 18:08:29 2018

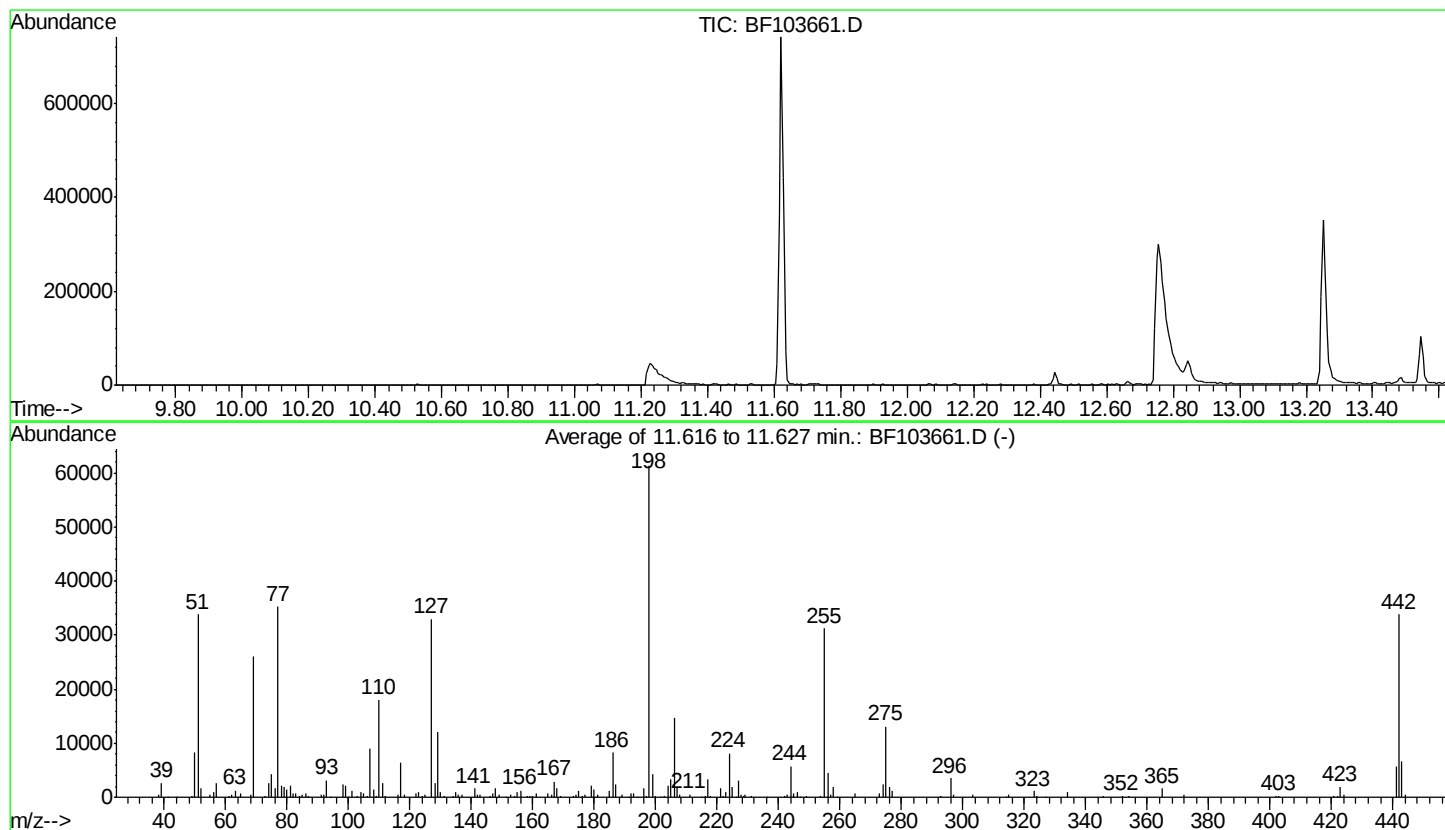

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.2	33866	PASS
68	69	0.00	2	2.0	517	PASS
69	198	0.00	100	42.3	25986	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.9	33066	PASS
197	198	0.00	2	0.5	337	PASS
198	198	100	100	100.0	61394	PASS
199	198	5	9	6.9	4226	PASS
275	198	10	60	21.3	13082	PASS
365	198	1	100	2.6	1601	PASS
441	443	0.01	100	85.1	5668	PASS
442	198	50	100	55.1	33840	PASS
443	442	15	24	19.7	6664	PASS