


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031419\
 Data File : BF113047.D
 Acq On : 14 Mar 2019 12:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 13 03:42:55 2019

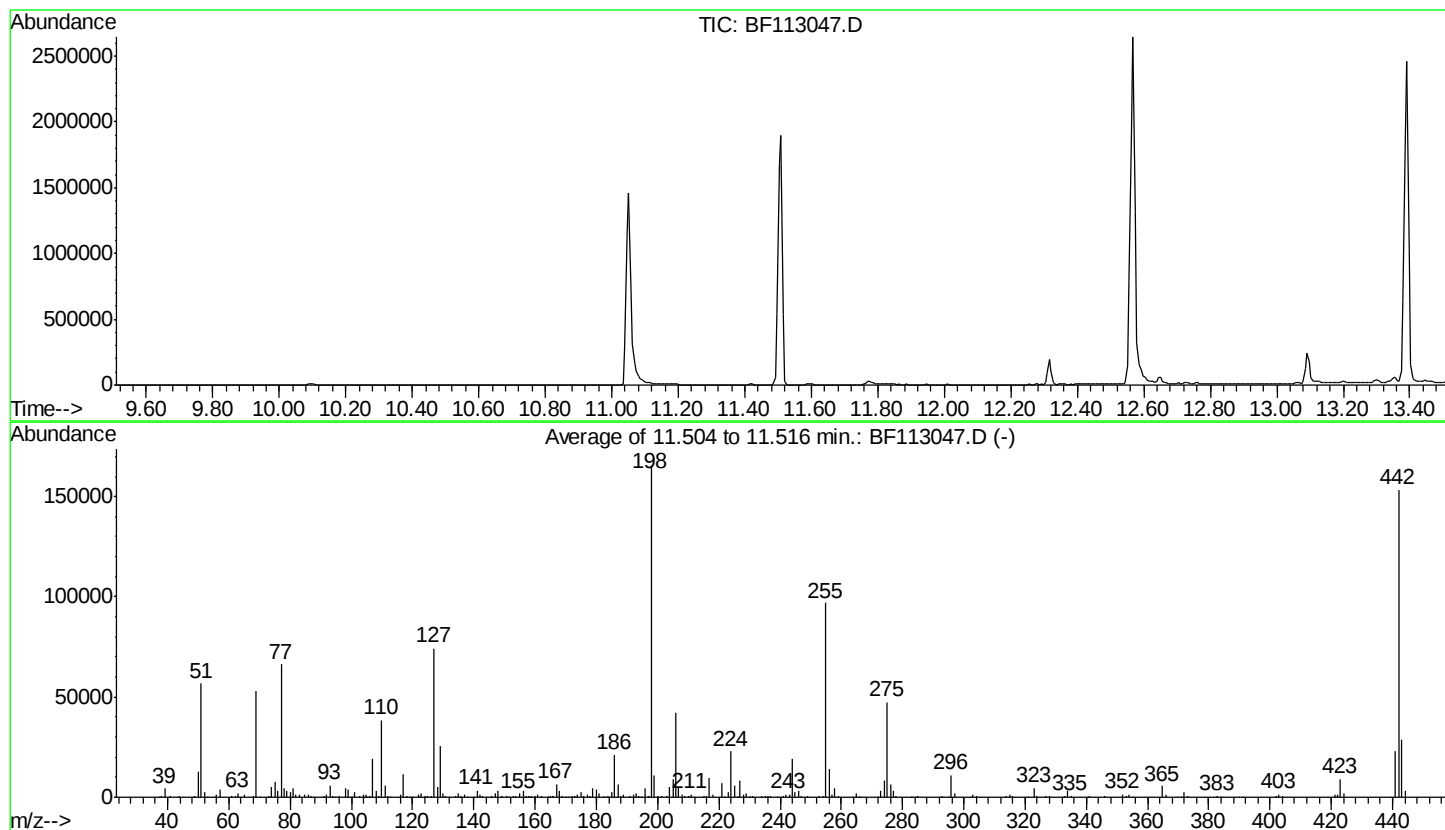

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	56782	PASS
68	69	0.00	2	1.4	727	PASS
69	198	0.00	100	32.1	53098	PASS
70	69	0.00	2	0.5	247	PASS
127	198	10	80	44.8	74200	PASS
197	198	0.00	2	0.6	975	PASS
198	198	100	100	100.0	165461	PASS
199	198	5	9	6.6	10942	PASS
275	198	10	60	28.7	47504	PASS
365	198	1	100	3.3	5536	PASS
441	198	0.01	100	14.1	23333	PASS
442	198	50	100	92.8	153629	PASS
443	442	15	24	18.6	28645	PASS