
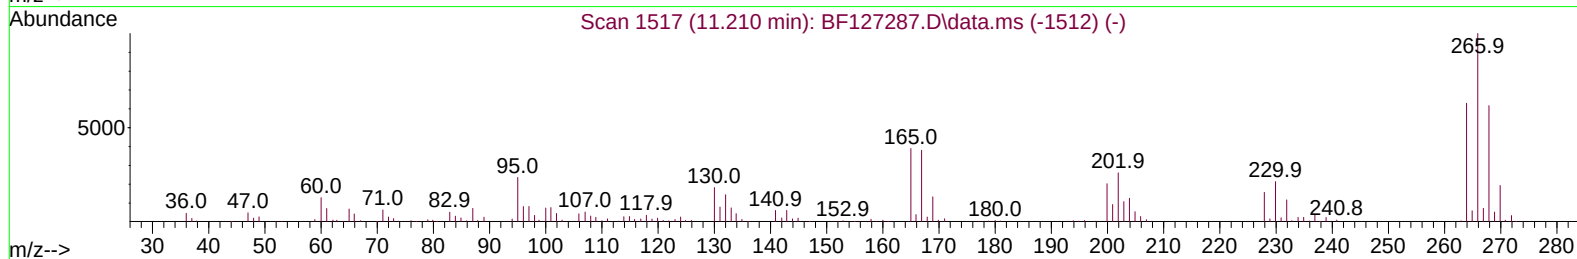
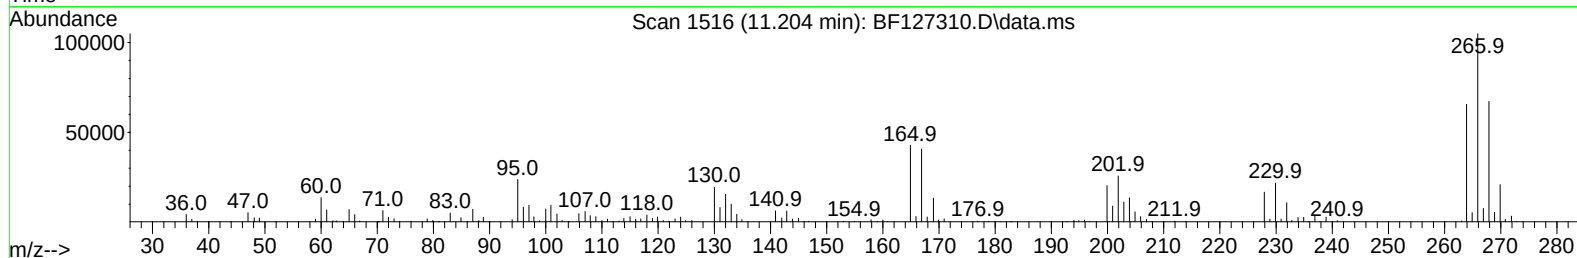


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031422\
 Data File : BF127310.D
 Acq On : 14 Mar 2022 09:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 12:15:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 10 16:51:53 2022
 Response via : Initial Calibration

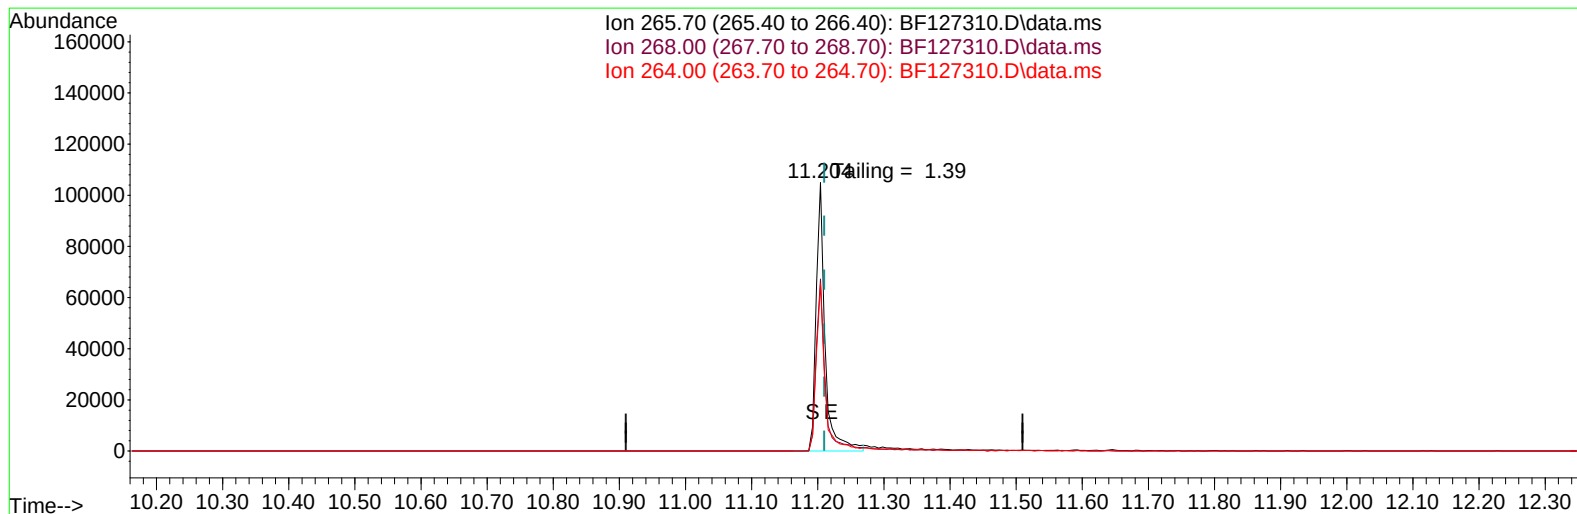

TIC: BF127310.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.006) 29666.83 ng

response 104645

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	64.08
264.00	63.00	62.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031422\
 Data File : BF127310.D
 Acq On : 14 Mar 2022 09:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 12:15:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 10 16:51:53 2022
 Response via : Initial Calibration

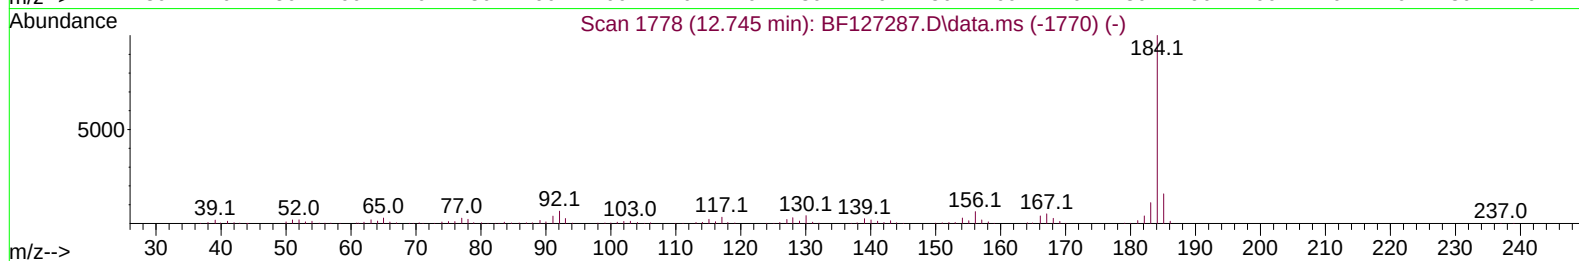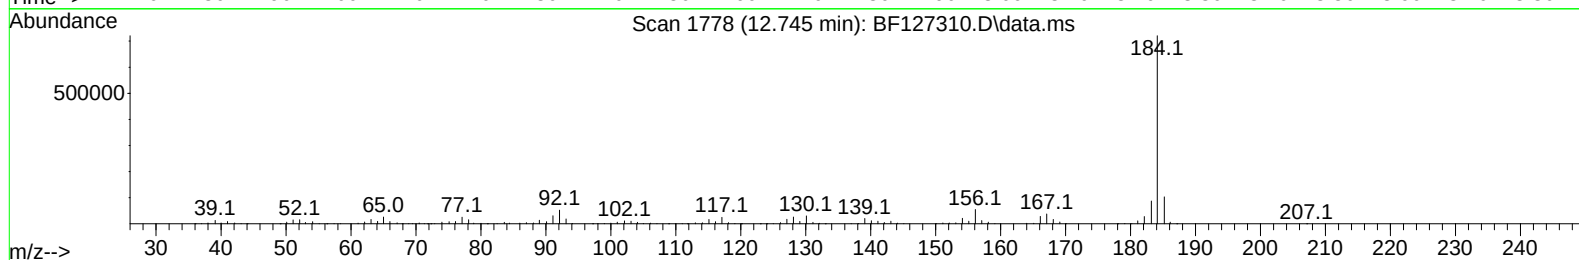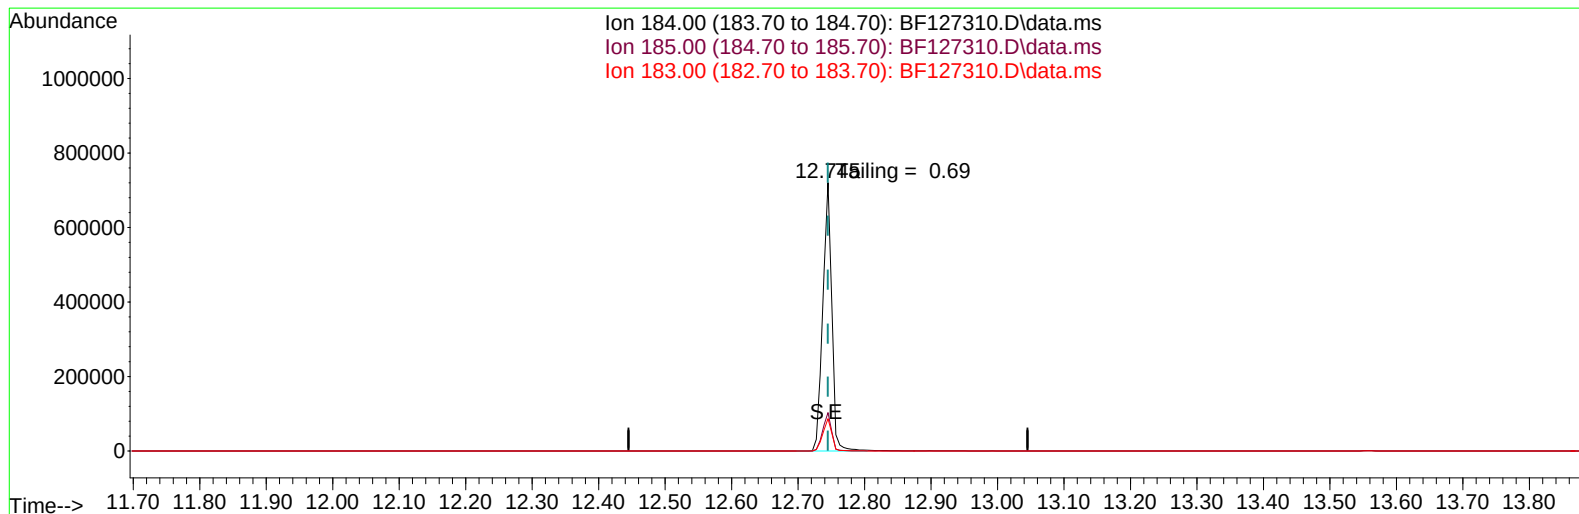

TIC: BF127310.D\data.ms

(77) Benzidine

12.745min (-0.000) 0.00 ng

response 681856

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.30
183.00	10.20	12.08
0.00	0.00	0.00