

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031422\
 Data File : BF127317.D
 Acq On : 14 Mar 2022 13:28
 Operator : CG\JU
 Sample : PB143209BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143209BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127317.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	542	548	551	rBV	3672969	3919466	81.41%	13.246%
2	6.504	711	717	720	rBV	3253806	4122937	85.63%	13.934%
3	6.863	775	778	782	rBV	866814	805575	16.73%	2.723%
4	7.434	869	875	878	rBV	2250685	2878001	59.78%	9.726%
5	8.151	991	997	1000	rBV	1082873	1053124	21.87%	3.559%
6	9.228	1173	1180	1183	rBV	4463875	4742561	98.50%	16.028%
7	9.910	1289	1296	1299	rBV	1253073	1211650	25.17%	4.095%
8	10.704	1424	1431	1434	rBV	2911211	2875197	59.72%	9.717%
9	11.398	1545	1549	1553	rBV	1487090	1234273	25.64%	4.171%
10	12.992	1814	1820	1823	rBV	4786717	4814602	100.00%	16.271%
11	14.045	1995	1999	2009	rVB	1227506	1063446	22.09%	3.594%
12	15.527	2246	2251	2263	rBV	681444	868622	18.04%	2.936%




Sum of corrected areas: 29589454

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031422\
Data File : BF127317.D
Acq On : 14 Mar 2022 13:28
Operator : CG\JU
Sample : PB143209BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143209BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

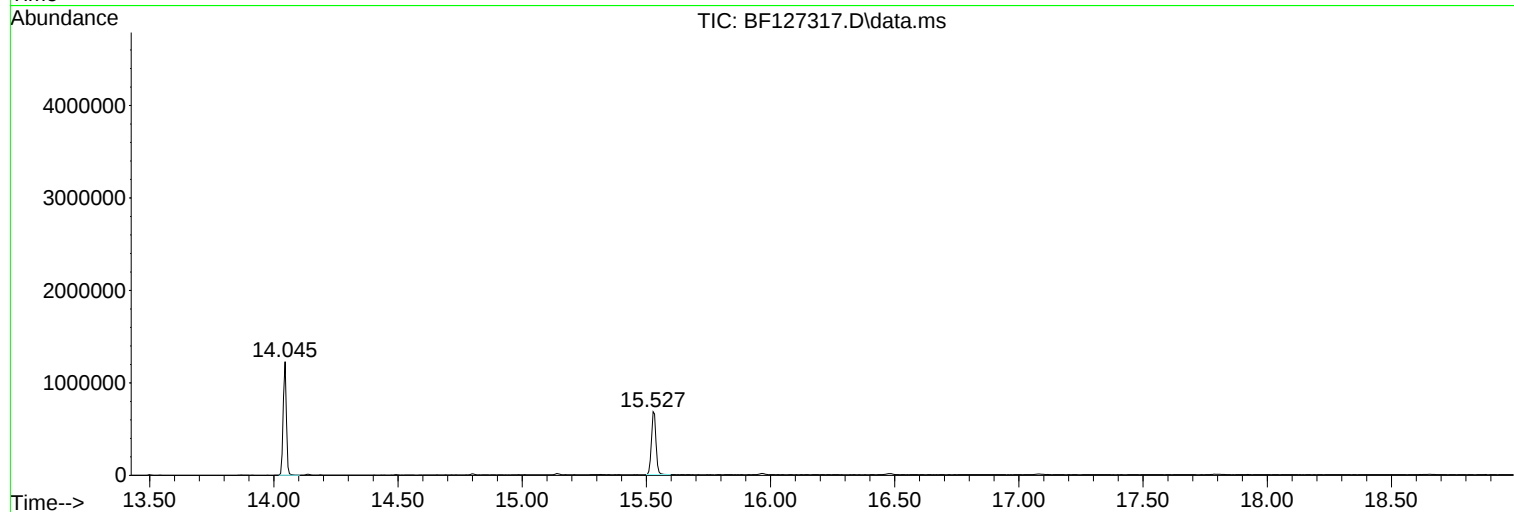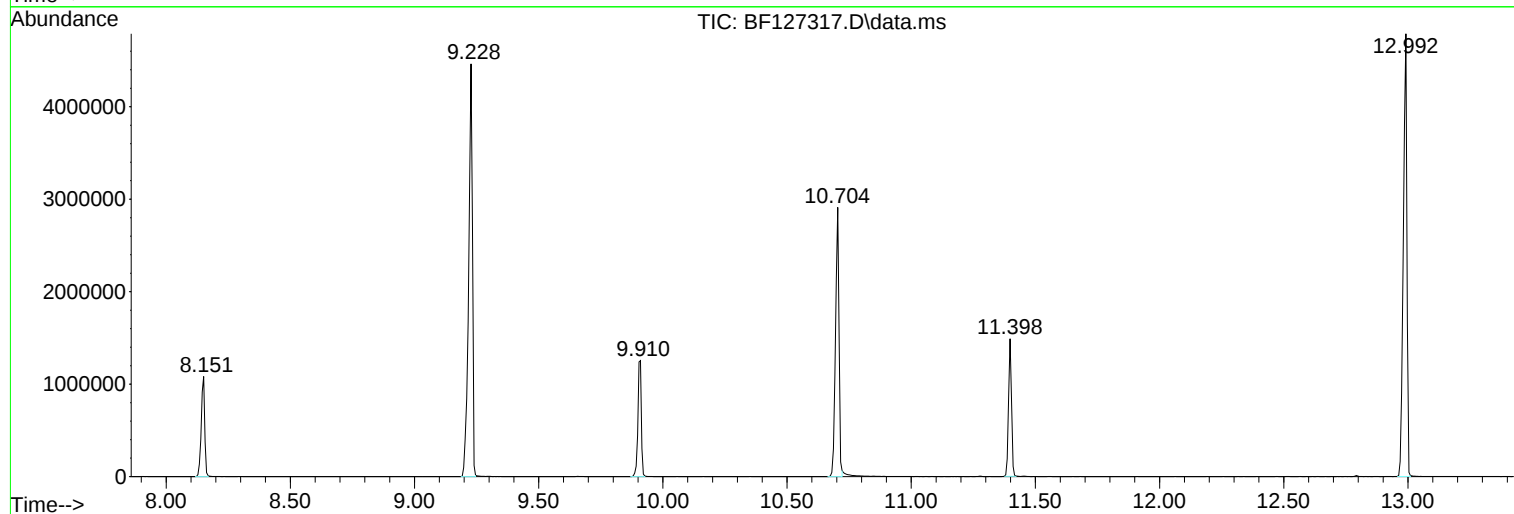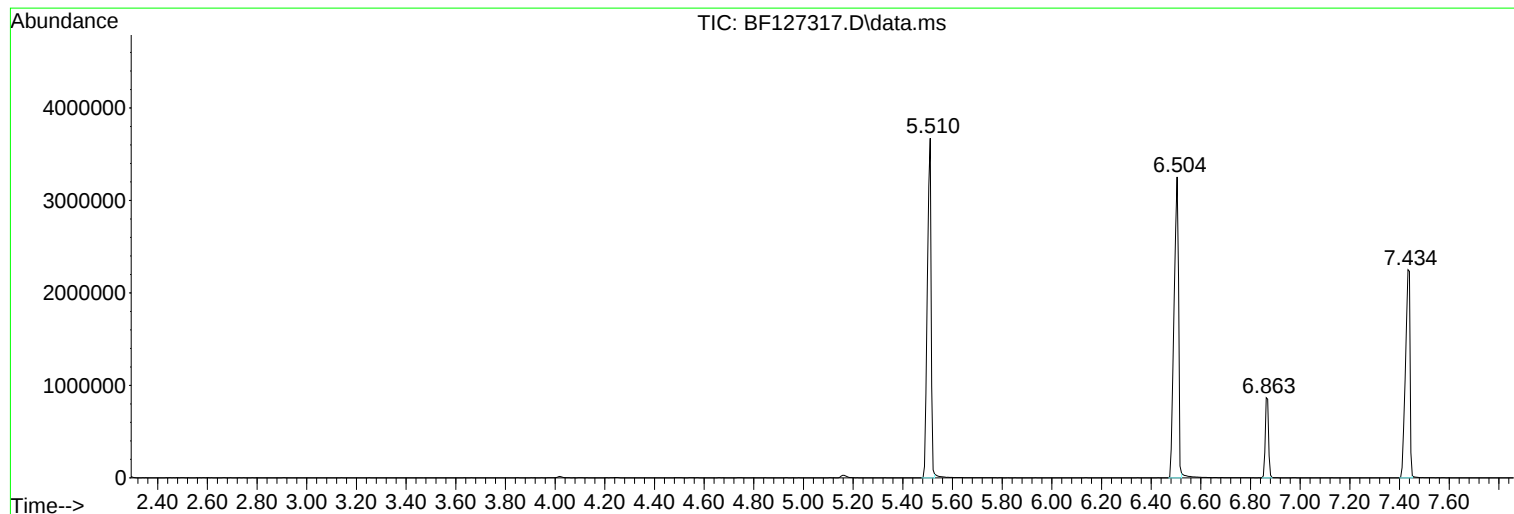

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031422\
Data File : BF127317.D
Acq On : 14 Mar 2022 13:28
Operator : CG\JU
Sample : PB143209BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143209BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031422\
Data File : BF127317.D
Acq On : 14 Mar 2022 13:28
Operator : CG\JU
Sample : PB143209BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143209BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------